
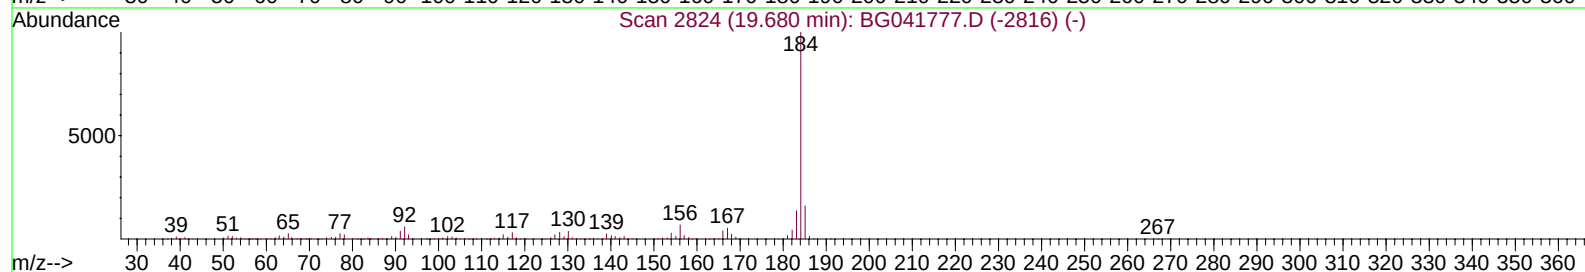
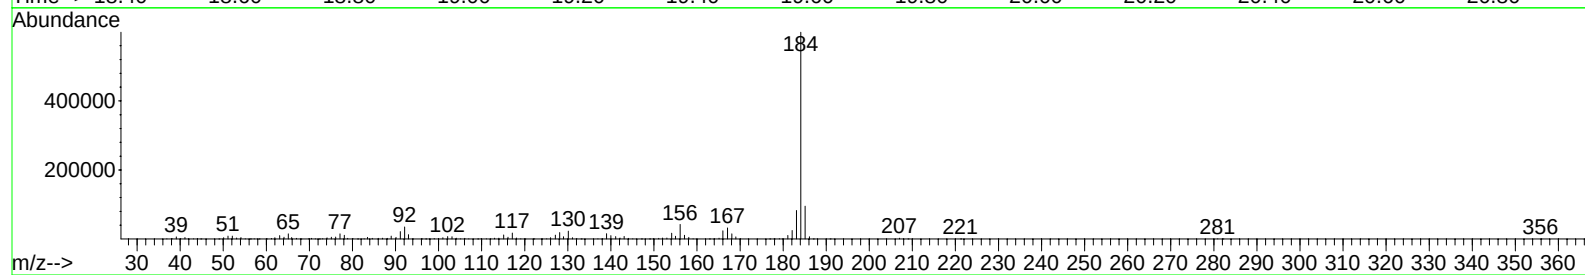


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080219\
 Data File : BG041879.D
 Acq On : 2 Aug 2019 8:41
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 18:51:26 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG072719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 31 08:57:26 2019
 Response via : Initial Calibration

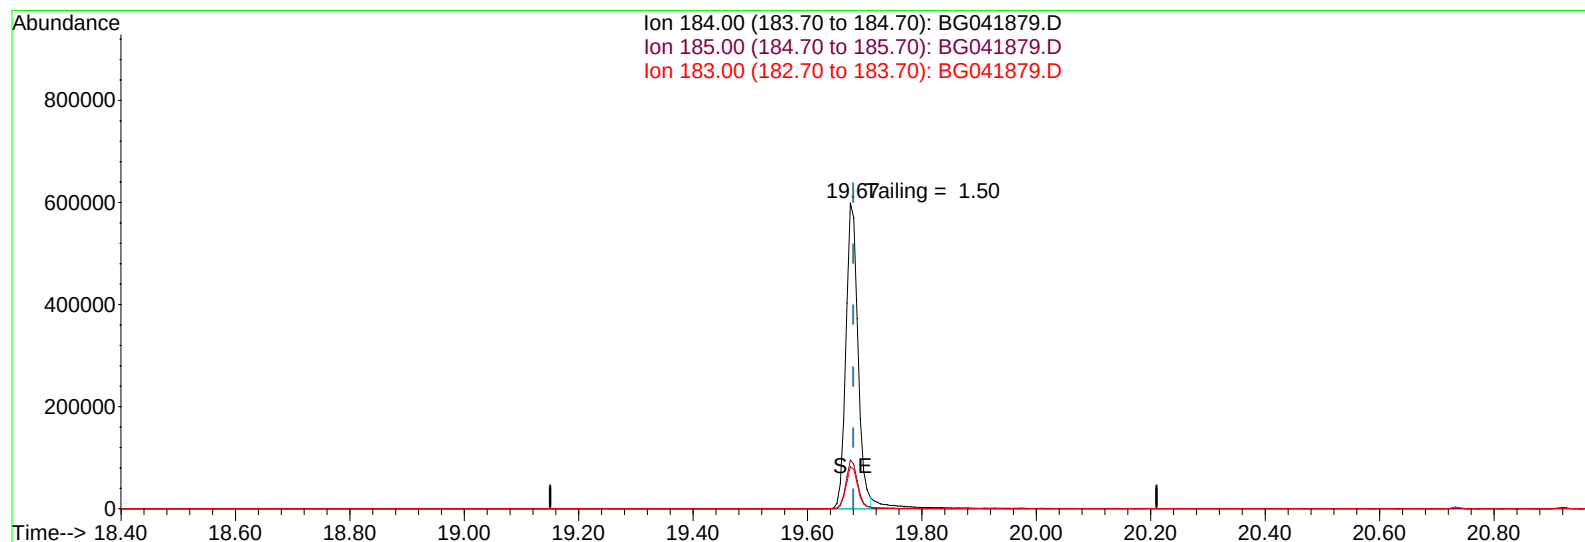

TIC: BG041879.D

(77) Benzidine




19.675min (-0.005) 108399.14ng

response 919922

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	15.89
183.00	14.70	13.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080219\
Data File : BG041879.D
Acq On : 2 Aug 2019 8:41
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 18:51:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG072719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 08:57:26 2019
Response via : Initial Calibration

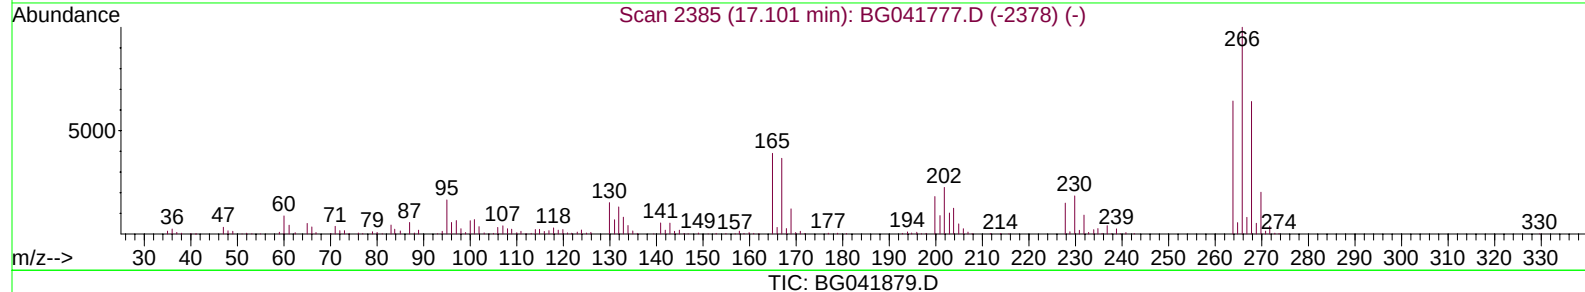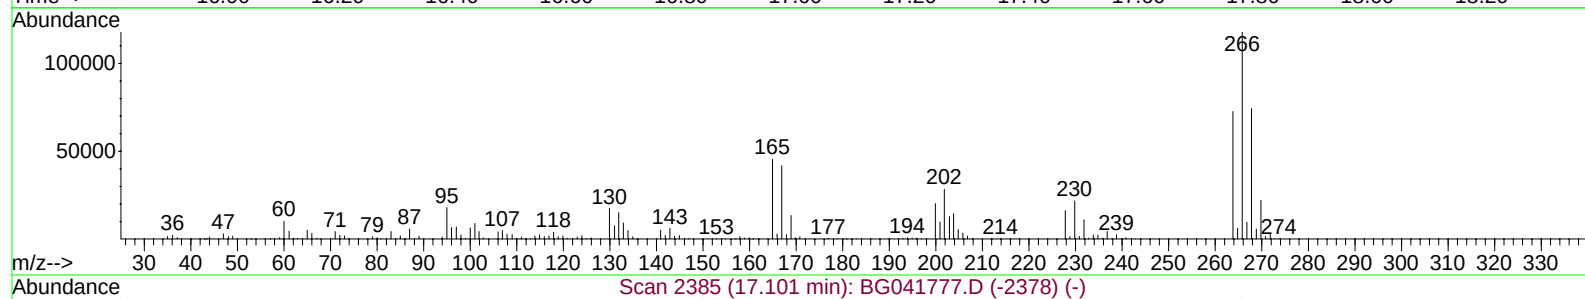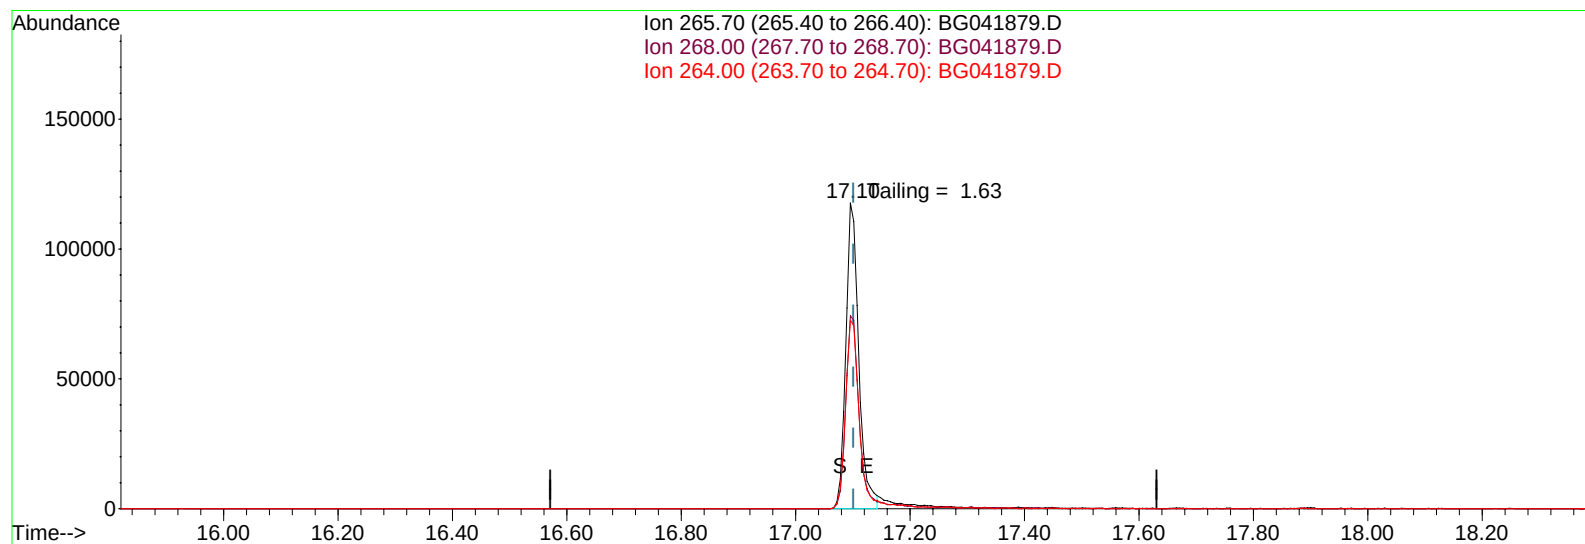

(70) Pentachlorophenol (C)

17.096min (-0.005) 239029.56ng

response 195987

Ion	Exp%	Act%
265.70	100	100
268.00	66.10	63.11
264.00	64.30	61.72
0.00	0.00	0.00