
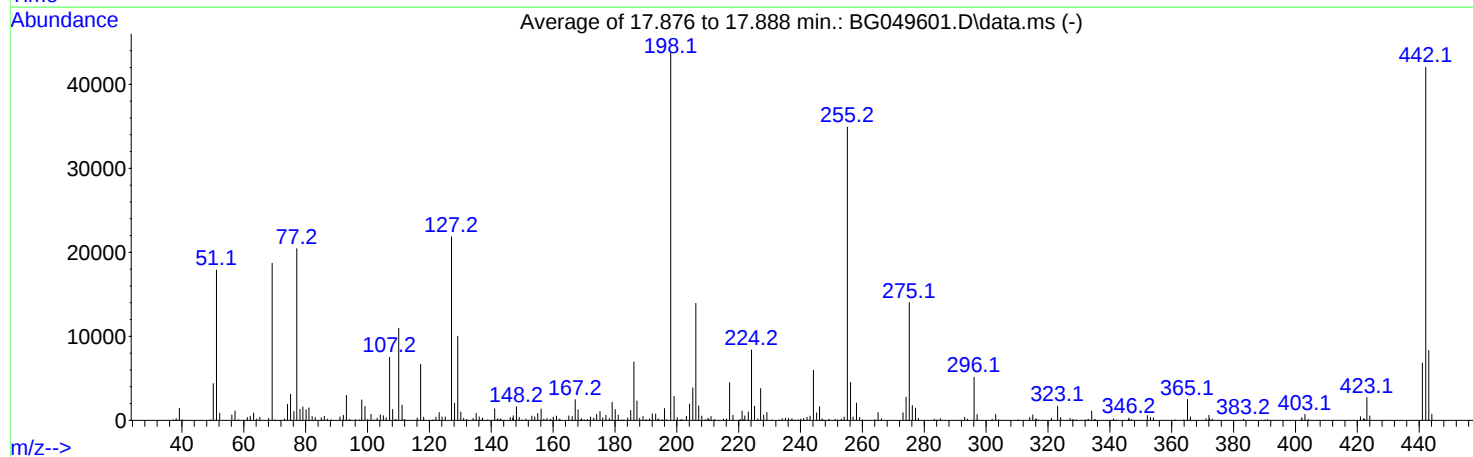


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080221\
 Data File : BG049601.D
 Acq On : 2 Aug 2021 12:15
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 21 16:57:05 2021

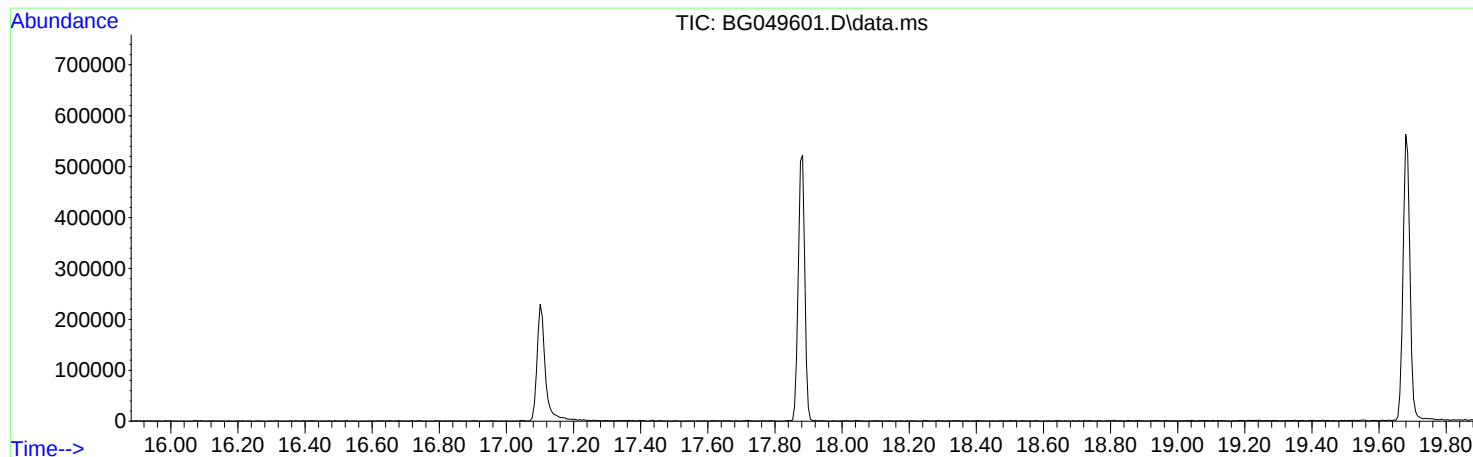




AutoFind: Scans 2526, 2527, 2528; Background Corrected with Scan 2519

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.8	17887	PASS
68	69	0.00	2	1.2	231	PASS
69	198	0.00	100	42.7	18699	PASS
70	69	0.00	2	0.3	55	PASS
127	198	10	80	49.9	21858	PASS
197	198	0.00	2	0.2	100	PASS
198	198	100	100	100.0	43792	PASS
199	198	5	9	6.5	2850	PASS
275	198	10	60	32.0	14023	PASS
365	198	1	100	5.7	2493	PASS
441	198	0.01	100	15.6	6814	PASS
442	442	100	100	100.0	42040	PASS
443	442	15	24	19.8	8325	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080221\
Data File : BG049601.D
Acq On : 2 Aug 2021 12:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 02 14:48:17 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 21 16:57:05 2021
Response via : Initial Calibration

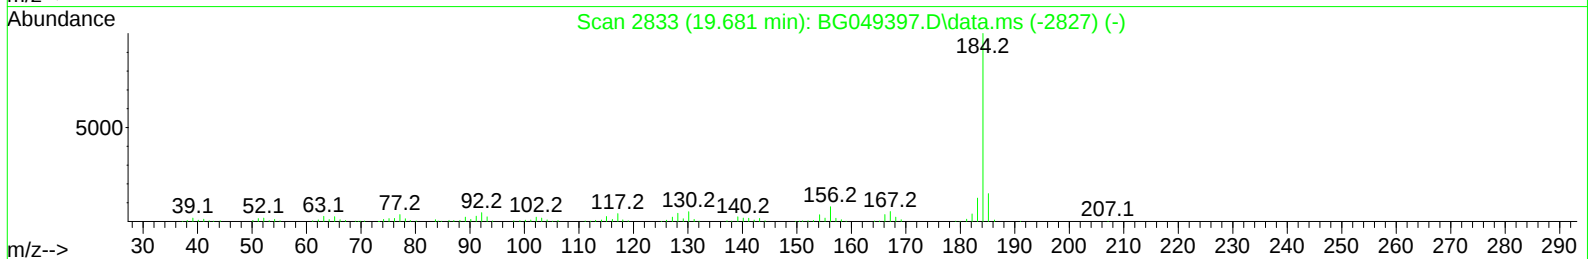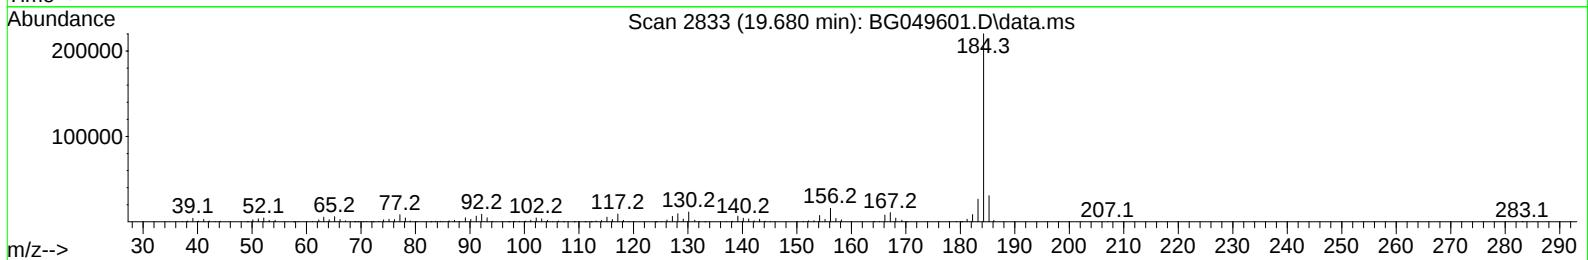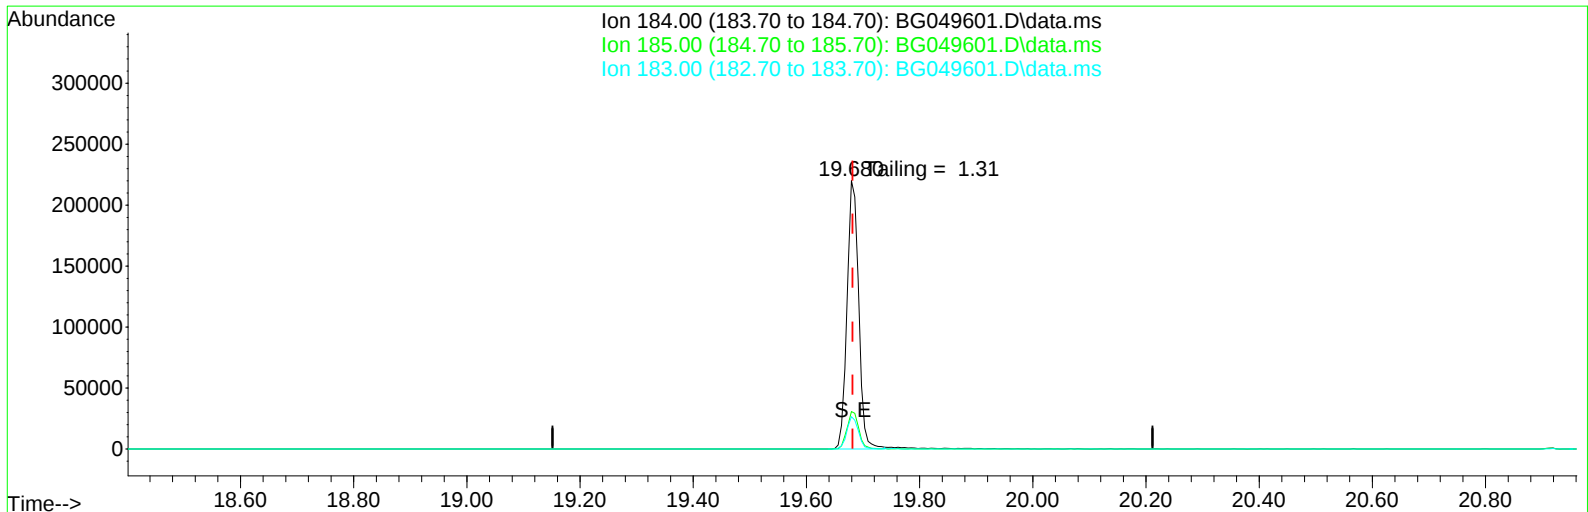

TIC: BG049601.D\data.ms

(77) Benzidine

19.680min (-0.002) 141595.04 ng




response 301756

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	13.96
183.00	11.70	12.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080221\
Data File : BG049601.D
Acq On : 2 Aug 2021 12:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 02 14:48:17 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 21 16:57:05 2021
Response via : Initial Calibration

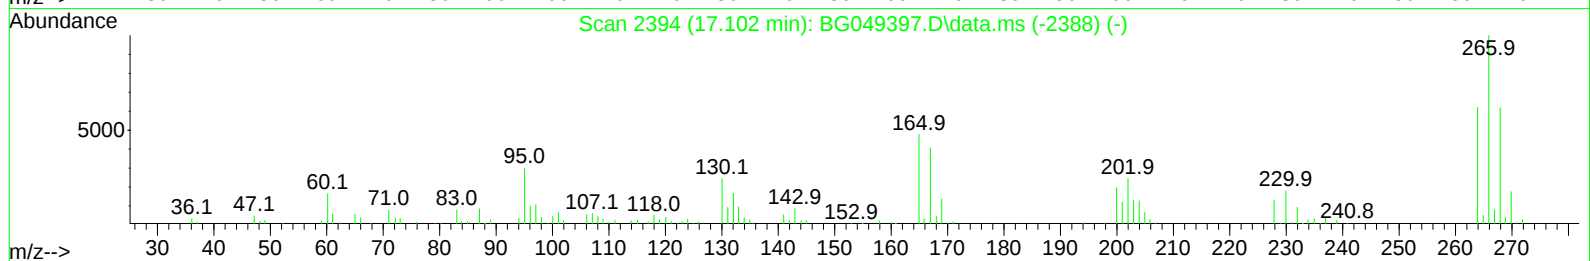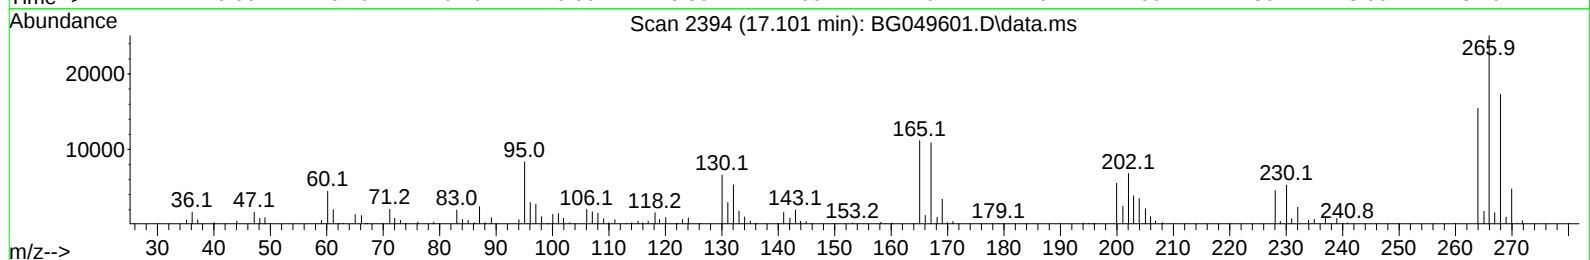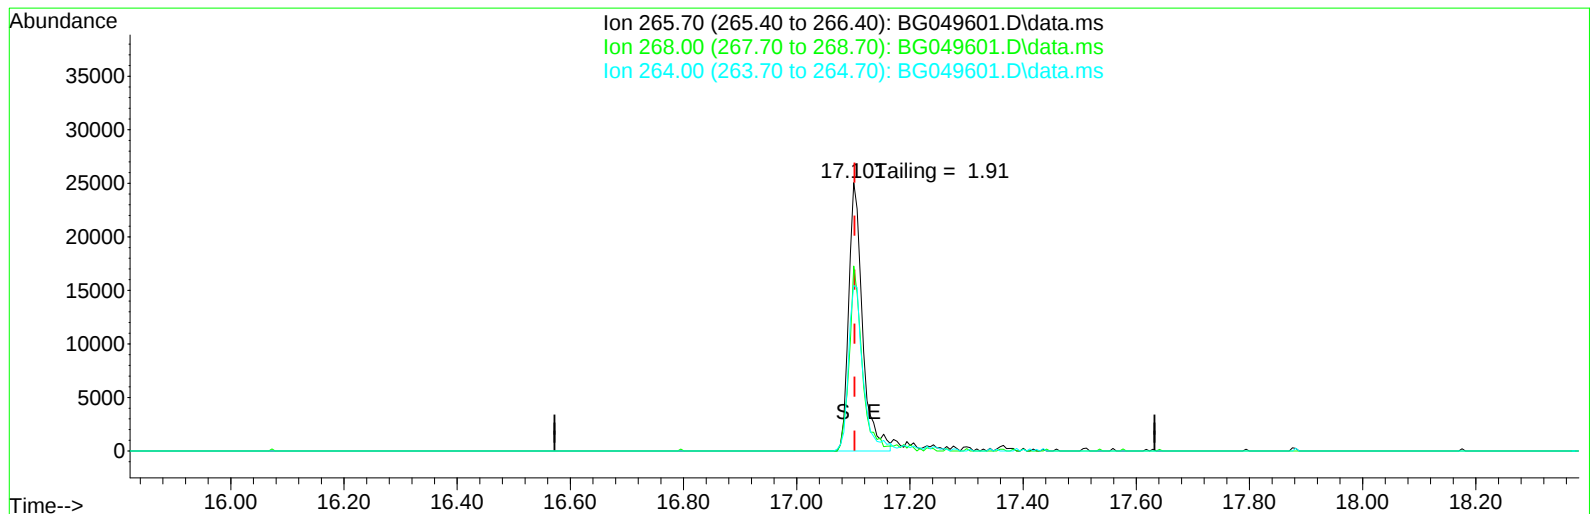

TIC: BG049601.D\data.ms

(70) Pentachlorophenol (C)

17.101min (-0.001) 17946.47 ng

response 42698

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	68.94
264.00	61.30	61.67
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/2/2021	BNA_G	BG049601.D
Compound Name	Response	Retention Time
DDT	168006	20.91
DDD	81	20.47
DDE	421	19.96
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
502	168508	0.30

Instrument :
BNA_G
ClientSampleId :
DFTPP