
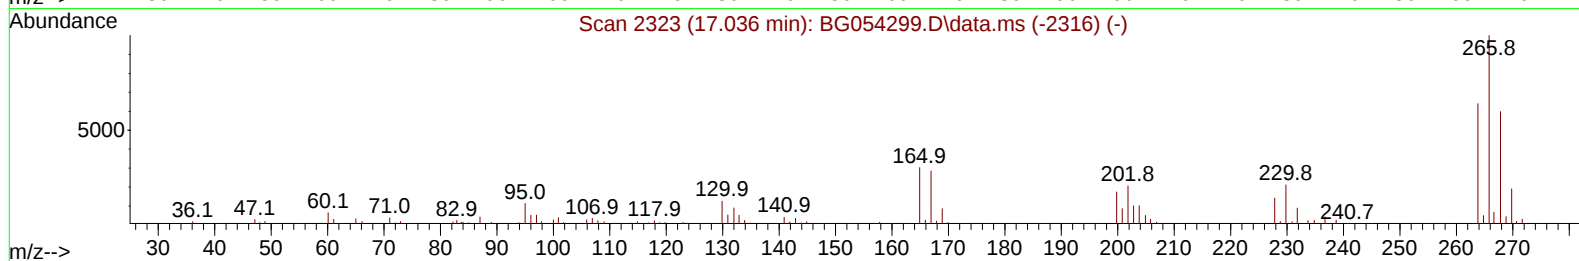
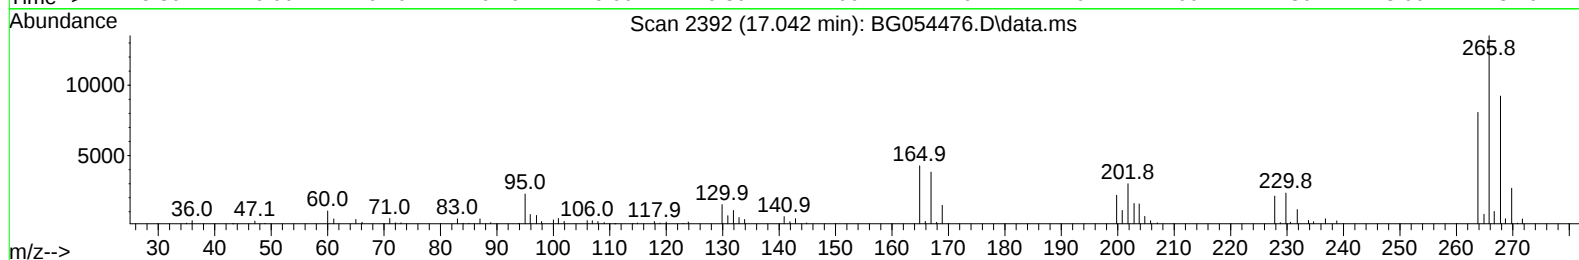


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080222\
Data File : BG054476.D
Acq On : 2 Aug 2022 9:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 06:19:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 04:30:50 2022
Response via : Initial Calibration

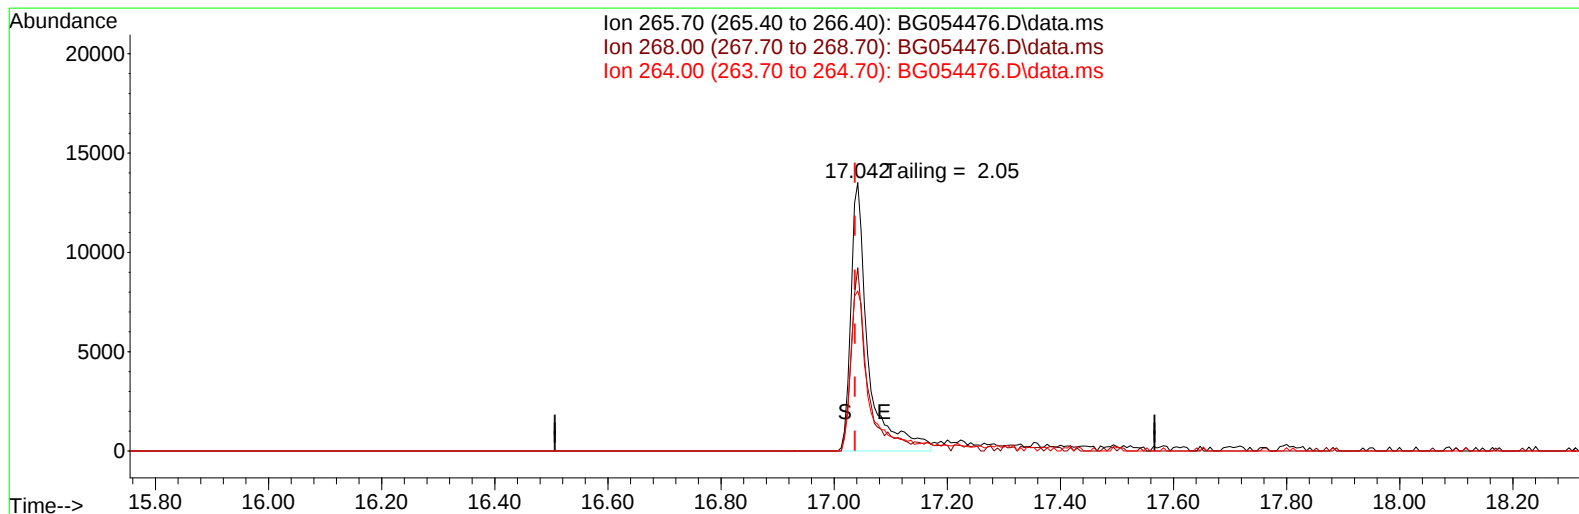

TIC: BG054476.D\data.ms

(70) Pentachlorophenol (C)




17.042min (+ 0.005) 17274.81 ng

response 26646

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	71.98
264.00	66.20	59.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080222\
 Data File : BG054476.D
 Acq On : 2 Aug 2022 9:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 06:19:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 28 04:30:50 2022
 Response via : Initial Calibration

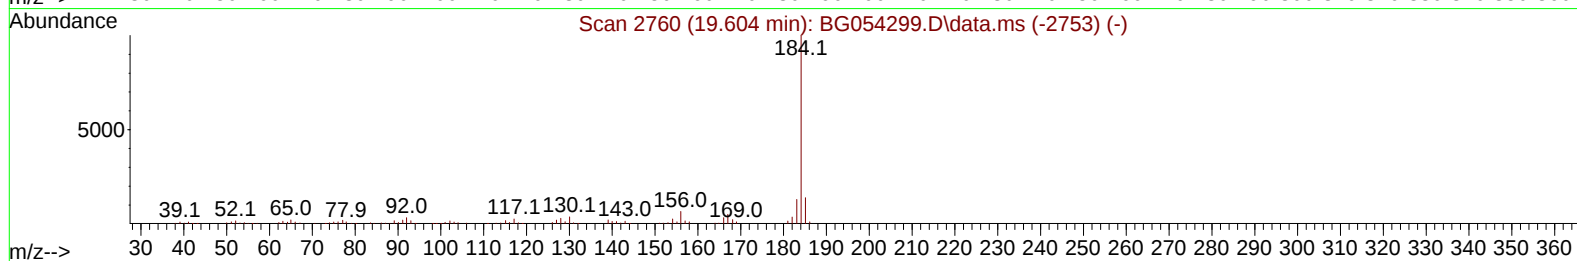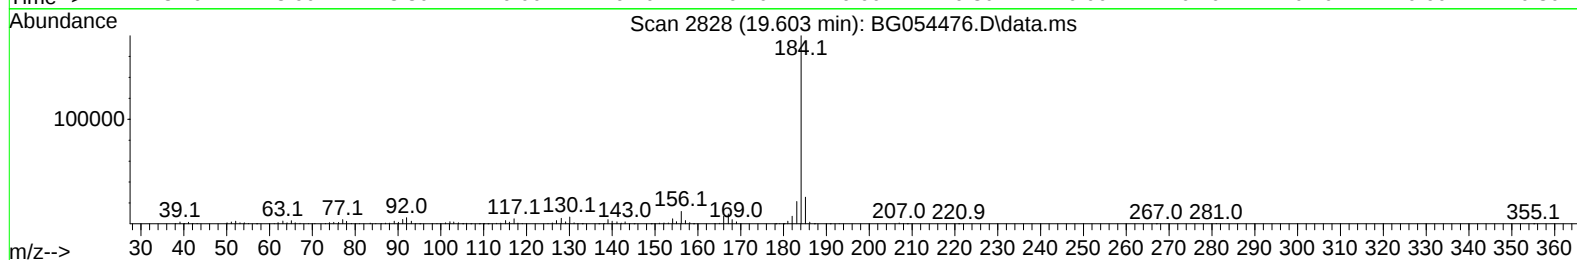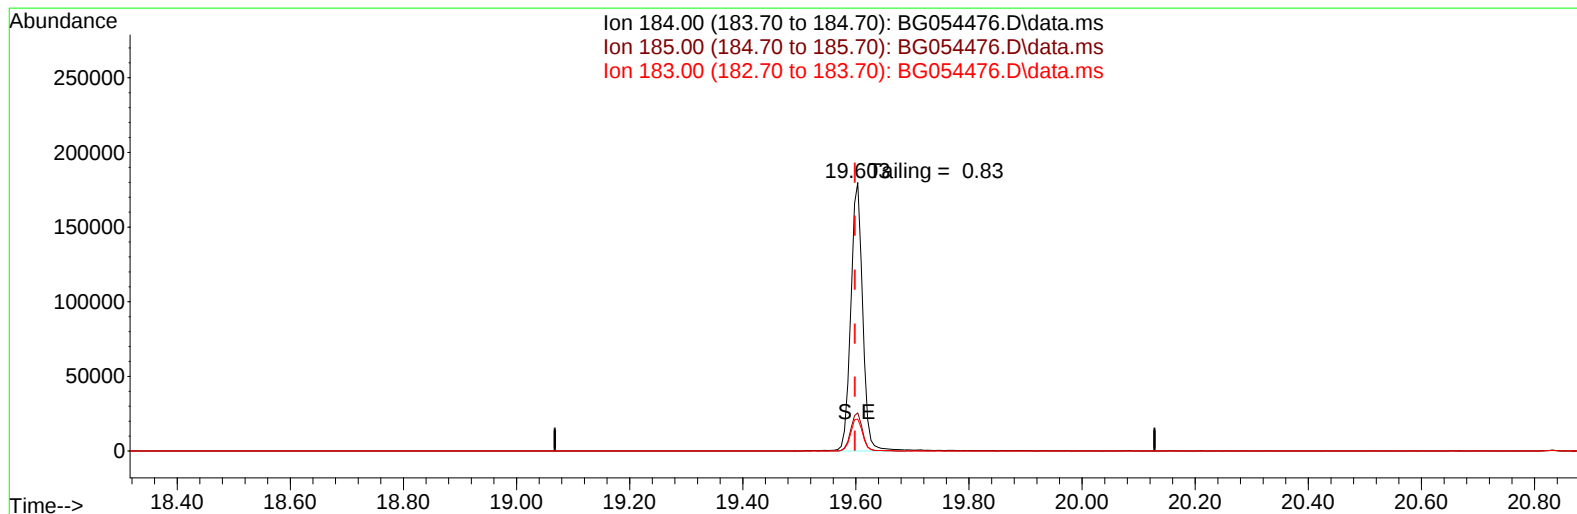

TIC: BG054476.D\data.ms

(77) Benzidine**19.603min (+ 0.005) 0.00 ng****response 260263**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.19
183.00	11.10	11.90
0.00	0.00	0.00