


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080222\
 Data File : BG054476.D
 Acq On : 2 Aug 2022 9:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 28 04:30:50 2022

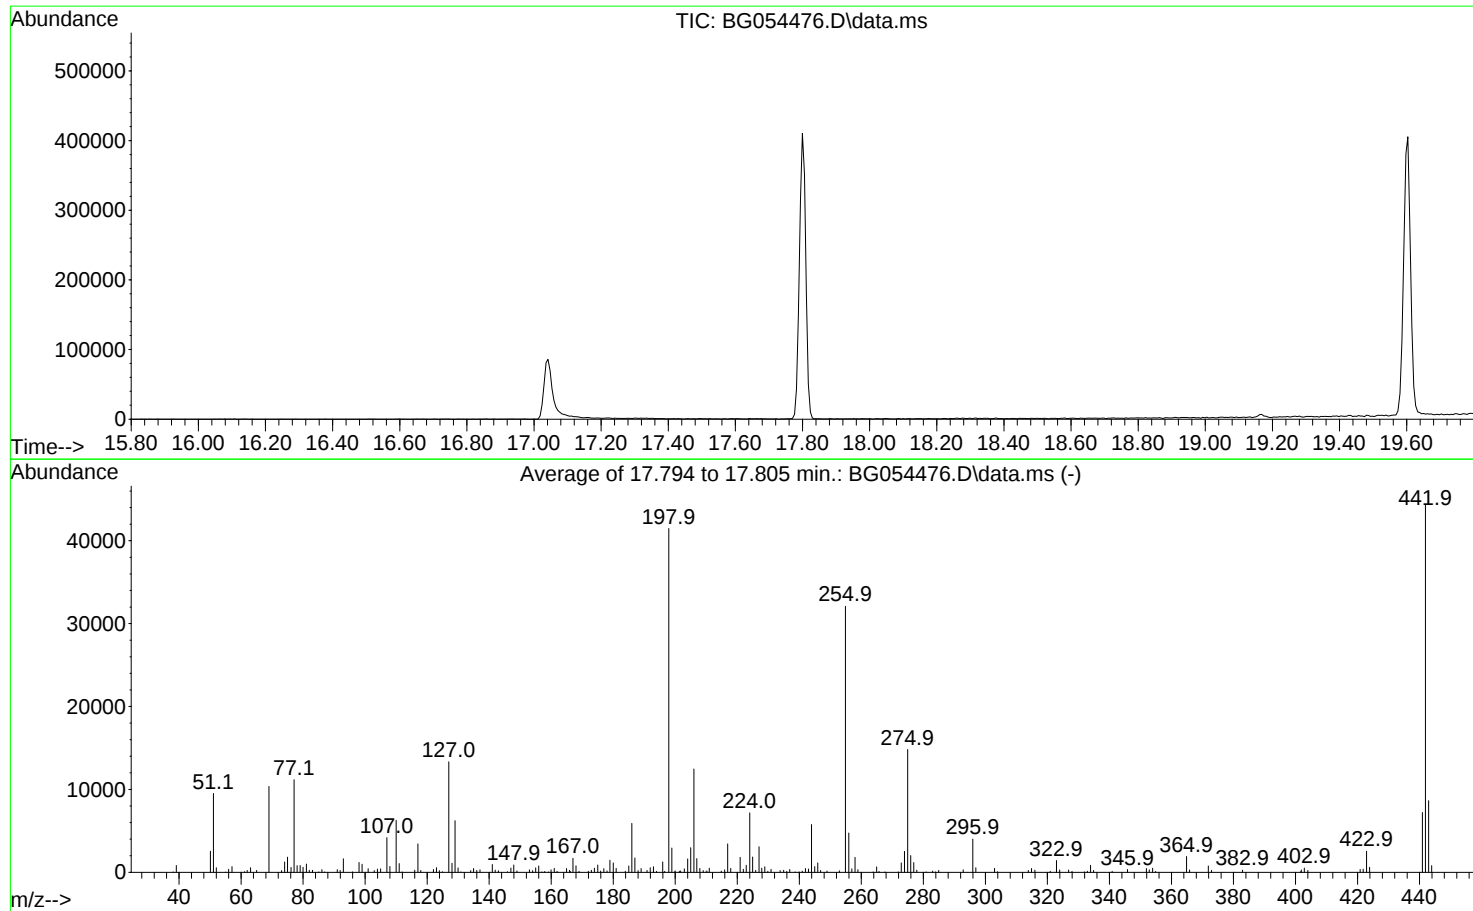




AutoFind: Scans 2520, 2521, 2522; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.9	9511	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	25.0	10357	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	32.1	13331	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	41485	PASS
199	198	5	9	7.1	2933	PASS
275	198	10	60	35.7	14820	PASS
365	198	1	100	4.6	1900	PASS
441	198	0.01	100	17.4	7209	PASS
442	442	50	100	100.0	44381	PASS
443	442	15	24	19.5	8634	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080222\
Data File : BG054476.D
Acq On : 2 Aug 2022 9:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 03 06:19:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 04:30:50 2022
Response via : Initial Calibration

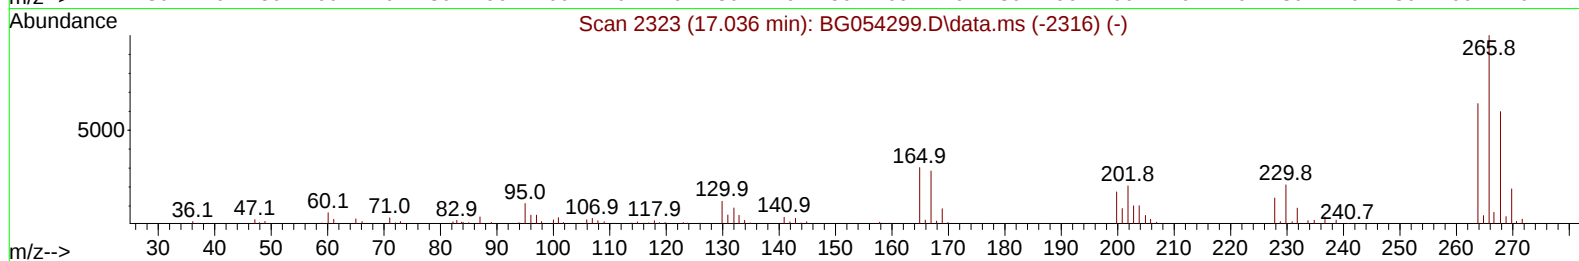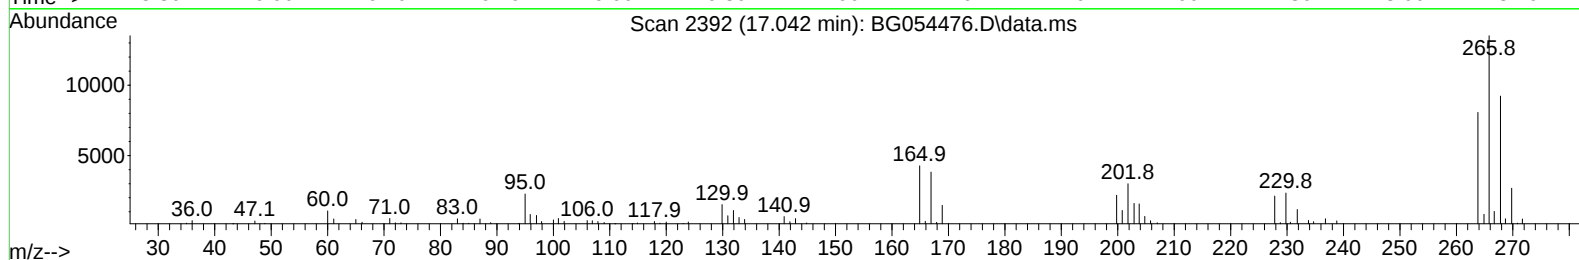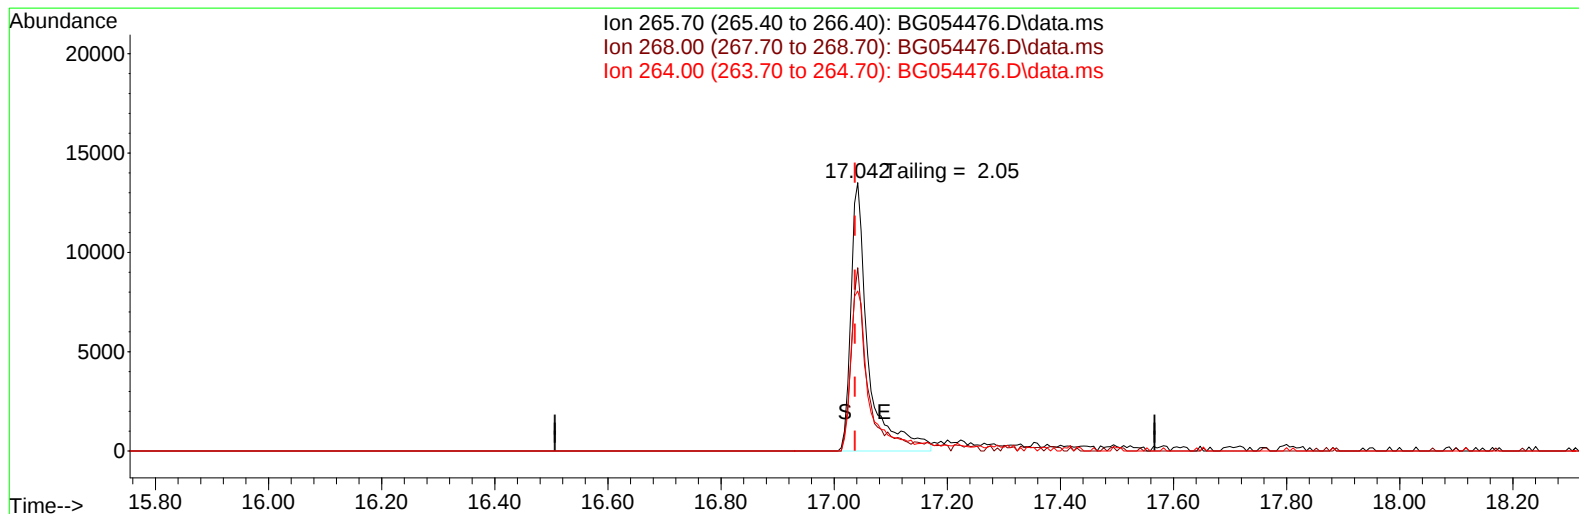

TIC: BG054476.D\data.ms

(70) Pentachlorophenol (C)

17.042min (+ 0.005) 17274.81 ng




response 26646

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	71.98
264.00	66.20	59.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080222\
 Data File : BG054476.D
 Acq On : 2 Aug 2022 9:09
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Aug 03 06:19:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 28 04:30:50 2022
 Response via : Initial Calibration

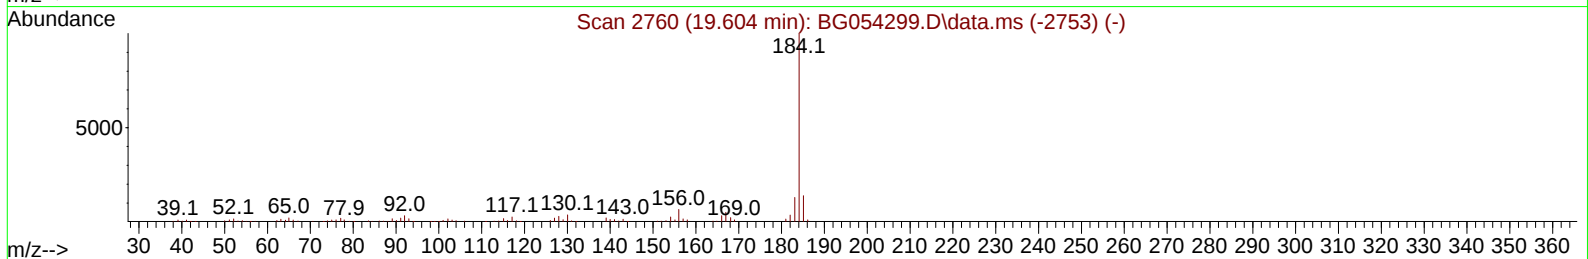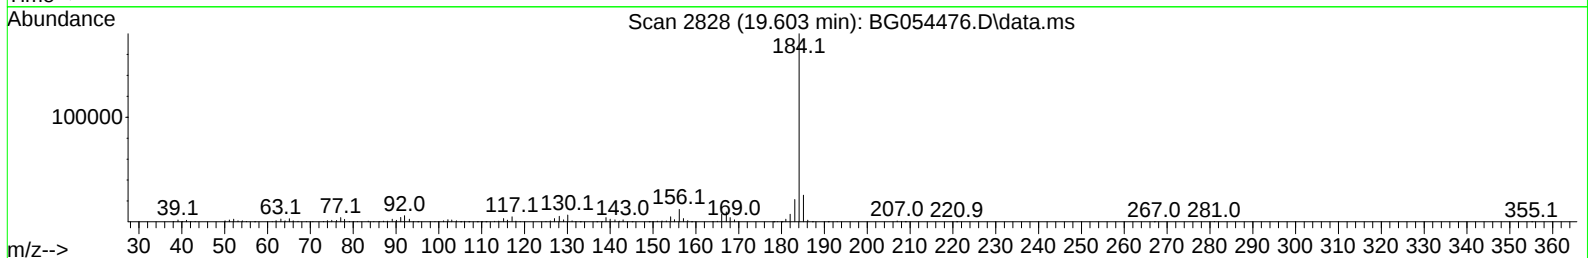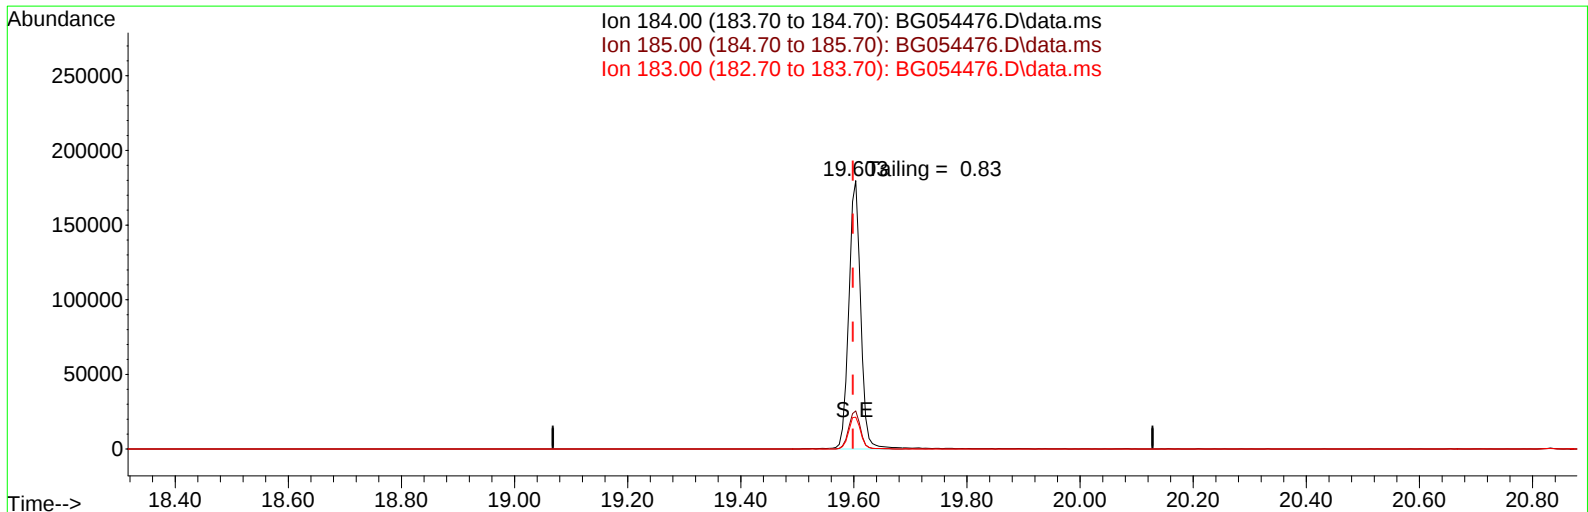

TIC: BG054476.D\data.ms

(77) Benzidine

19.603min (+ 0.005) 0.00 ng

response 260263

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.19
183.00	11.10	11.90
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/2/2022	BNA_G	BG054476.D
Compound Name	Response	Retention Time
DDT	151494	20.831
DDD	4420	20.397
DDE	61	19.891
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4481	155975	2.87

Instrument :
BNA_G
ClientSampleId :
DFTPP