

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080315\
 Data File : BG018243.D
 Acq On : 3 Aug 2015 14:49
 Operator : UM/TP
 Sample : PB84804BL
 Misc : SBLK04
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK04

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG073115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.825	21	23	27	rBV4	3379	3624	0.31%	0.032%
2	2.936	40	42	45	rBV2	6245	7316	0.62%	0.066%
3	3.083	66	67	69	rVB	2858	1966	0.17%	0.018%
4	3.107	69	71	74	rBV3	2476	3438	0.29%	0.031%
5	3.301	101	104	107	rBV4	1819	3125	0.26%	0.028%
6	3.412	120	123	125	rBV3	2820	3137	0.26%	0.028%
7	3.442	127	128	131	rBV	1914	2037	0.17%	0.018%
8	3.489	134	136	141	rVB3	2926	4470	0.38%	0.040%
9	3.595	151	154	155	rBV2	1756	1999	0.17%	0.018%
10	3.700	170	172	175	rBV3	2367	1886	0.16%	0.017%
11	3.759	180	182	183	rBV	2552	1846	0.16%	0.017%
12	4.652	333	334	337	rVB	2477	2118	0.18%	0.019%
13	4.746	349	350	354	rBV2	1809	2245	0.19%	0.020%
14	4.864	368	370	374	rVB2	1810	1797	0.15%	0.016%
15	4.981	389	390	393	rBV2	2117	1853	0.16%	0.017%
16	5.228	430	432	435	rVB2	2079	2379	0.20%	0.021%
17	5.269	435	439	442	rBV3	2009	3498	0.29%	0.031%
18	5.322	444	448	452	rBV	1120	2287	0.19%	0.021%
19	5.563	487	489	493	rVB3	2331	1926	0.16%	0.017%
20	5.674	505	508	509	rBV2	1998	2104	0.18%	0.019%
21	6.497	642	648	651	rBV2	1837	2574	0.22%	0.023%
22	6.662	670	676	684	rBV	170891	259171	21.85%	2.323%
23	6.803	694	700	707	rBV	131144	190642	16.07%	1.709%
24	6.996	727	733	740	rBV	176663	273776	23.08%	2.454%
25	7.455	804	811	819	rVB	129455	206544	17.41%	1.852%
26	7.889	881	885	886	rBV	1777	1781	0.15%	0.016%
27	7.907	886	888	891	rVB	1831	2033	0.17%	0.018%
28	7.936	891	893	897	rBV	1170	1988	0.17%	0.018%
29	8.030	908	909	912	rBV	1940	1990	0.17%	0.018%
30	8.195	930	937	944	rBV	230475	355817	29.99%	3.190%
31	8.612	1002	1008	1016	rBV	172260	277596	23.40%	2.489%
32	9.000	1071	1074	1077	rBV	1978	2198	0.19%	0.020%
33	9.076	1086	1087	1092	rVB	2169	2662	0.22%	0.024%
34	9.335	1123	1131	1139	rBV	171355	275099	23.19%	2.466%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080315\
 Data File : BG018243.D
 Acq On : 3 Aug 2015 14:49
 Operator : UM/TP
 Sample : PB84804BL
 Misc : SBLK04
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK04

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG073115.M
 Title : SVOA CALIBRATION

35	9.881	1218	1224	1234	rVB	246541	383737	32.35%	3.440%
36	10.246	1278	1286	1293	rVB	187805	311653	26.27%	2.794%
37	10.392	1303	1311	1318	rBV	232455	385426	32.49%	3.455%
38	10.504	1328	1330	1334	rBV	1463	2096	0.18%	0.019%
39	10.645	1350	1354	1357	rBV	2109	2080	0.18%	0.019%
40	10.792	1374	1379	1380	rBV	1311	1736	0.15%	0.016%
41	11.092	1421	1430	1431	rBV	1525	2133	0.18%	0.019%
42	11.509	1497	1501	1504	rBV	1444	2533	0.21%	0.023%
43	13.031	1757	1760	1763	rVB	1478	2129	0.18%	0.019%
44	13.095	1767	1771	1774	rBV2	1235	1877	0.16%	0.017%
45	13.224	1789	1793	1796	rBV2	1059	1828	0.15%	0.016%
46	13.377	1814	1819	1822	rVB2	1565	1825	0.15%	0.016%
47	13.418	1822	1826	1830	rBV	1561	2396	0.20%	0.021%
48	13.553	1841	1849	1855	rBV	512330	691150	58.26%	6.196%
49	13.830	1889	1896	1902	rVB	462074	690610	58.22%	6.191%
50	14.141	1941	1949	1955	rVB2	309286	458286	38.63%	4.108%
51	14.388	1985	1991	2001	rBV2	212786	308980	26.05%	2.770%
52	14.734	2046	2050	2054	rVB2	2247	3069	0.26%	0.028%
53	14.905	2077	2079	2082	rBV	1812	2063	0.17%	0.018%
54	15.140	2113	2119	2126	rBV	663663	883192	74.45%	7.917%
55	15.281	2137	2143	2150	rBV	210665	285190	24.04%	2.557%
56	15.375	2156	2159	2166	rVB2	5224	7165	0.60%	0.064%
57	15.545	2185	2188	2191	rVB2	1795	1936	0.16%	0.017%
58	15.580	2191	2194	2196	rBV2	1523	1881	0.16%	0.017%
59	15.851	2237	2240	2243	rBV2	1794	2756	0.23%	0.025%
60	16.009	2264	2267	2270	rBV2	1463	2020	0.17%	0.018%
61	16.092	2279	2281	2283	rBV2	3146	2034	0.17%	0.018%
62	16.180	2294	2296	2298	rVB	1995	1731	0.15%	0.016%
63	16.268	2309	2311	2314	rBV	1974	1808	0.15%	0.016%
64	16.362	2324	2327	2329	rBV2	2170	2011	0.17%	0.018%
65	16.409	2331	2335	2337	rVB	2110	2780	0.23%	0.025%
66	16.585	2363	2365	2369	rVB	3134	3659	0.31%	0.033%
67	16.620	2369	2371	2376	rBV	2400	3744	0.32%	0.034%
68	16.673	2376	2380	2383	rBV3	2825	4942	0.42%	0.044%
69	16.767	2393	2396	2397	rVB2	2888	2223	0.19%	0.020%
70	16.785	2397	2399	2401	rBV2	2169	2105	0.18%	0.019%
71	16.897	2409	2418	2423	rBV	457012	618895	52.17%	5.548%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080315\
Data File : BG018243.D
Acq On : 3 Aug 2015 14:49
Operator : UM/TP
Sample : PB84804BL
Misc : SBLK04
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK04

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG073115.M
Title : SVOA CALIBRATION

72	16.996	2428	2435	2440	rVV	753592	1067712	90.00%	9.572%
73	17.032	2440	2441	2444	rVB	2826	2079	0.18%	0.019%
74	17.055	2444	2445	2449	rBV	2398	2235	0.19%	0.020%
75	17.085	2449	2450	2454	rBV2	1324	1796	0.15%	0.016%
76	17.179	2464	2466	2467	rBV	3795	2167	0.18%	0.019%
77	17.390	2498	2502	2503	rBV2	1615	2290	0.19%	0.021%
78	17.431	2506	2509	2510	rBV3	2264	2305	0.19%	0.021%
79	17.531	2525	2526	2529	rBV2	2124	2043	0.17%	0.018%
80	17.672	2548	2550	2551	rBV	2465	2487	0.21%	0.022%
81	17.825	2574	2576	2580	rVB2	2501	2270	0.19%	0.020%
82	17.884	2584	2586	2589	rVB3	2447	2397	0.20%	0.021%
83	17.984	2601	2603	2610	rBV2	2697	5363	0.45%	0.048%
84	18.177	2633	2636	2638	rBV2	3437	4299	0.36%	0.039%
85	18.459	2682	2684	2685	rBV2	2944	1864	0.16%	0.017%
86	18.501	2689	2691	2694	rBV3	2983	3162	0.27%	0.028%
87	18.571	2701	2703	2706	rVB4	3152	2333	0.20%	0.021%
88	19.305	2822	2828	2834	rBV	889759	1186294	100.00%	10.635%
89	21.103	3129	3134	3138	rBV	499347	626192	52.79%	5.614%
90	23.136	3474	3480	3488	rVB	461484	816589	68.84%	7.320%
91	23.271	3497	3503	3509	rVB2	238762	424606	35.79%	3.806%


Sum of corrected areas: 11155084

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080315\
Data File : BG018243.D
Acq On : 3 Aug 2015 14:49
Operator : UM/TP
Sample : PB84804BL
Misc : SBLK04
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK04

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG073115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

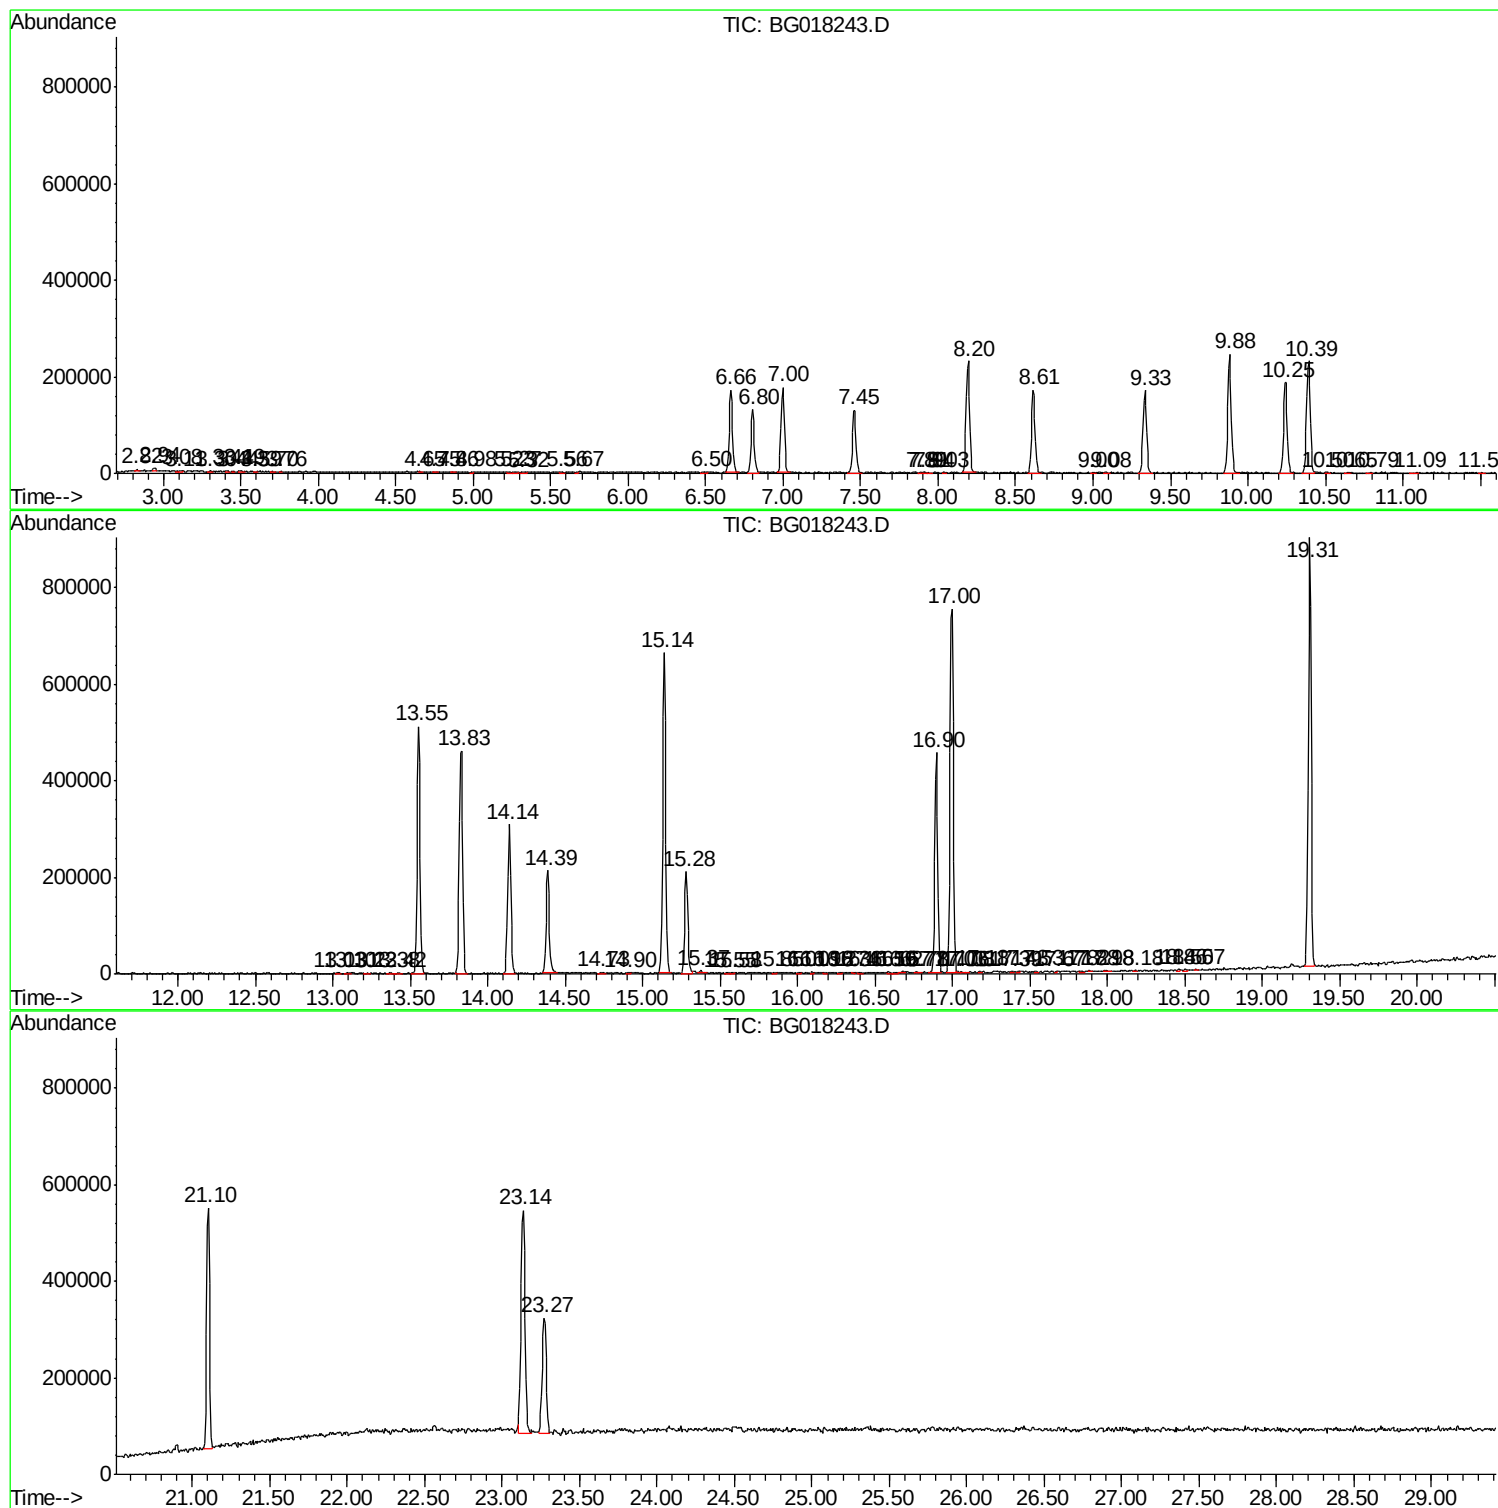

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080315\
Data File : BG018243.D
Acq On : 3 Aug 2015 14:49
Operator : UM/TP
Sample : PB84804BL
Misc : SBLK04
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK04

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG073115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080315\
Data File : BG018243.D
Acq On : 3 Aug 2015 14:49
Operator : UM/TP
Sample : PB84804BL
Misc : SBLK04
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK04

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG073115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc