


Data Path : Z:\HPCHEM1\BNA_G\Data\BG080315\
Data File : BG018241.D
Acq On : 3 Aug 2015 13:33
Operator : UM/TP
Sample : DFTPP24
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP24

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG073115.M
Title : SVOA CALIBRATION
Last Update : Tue Aug 04 02:54:30 2015

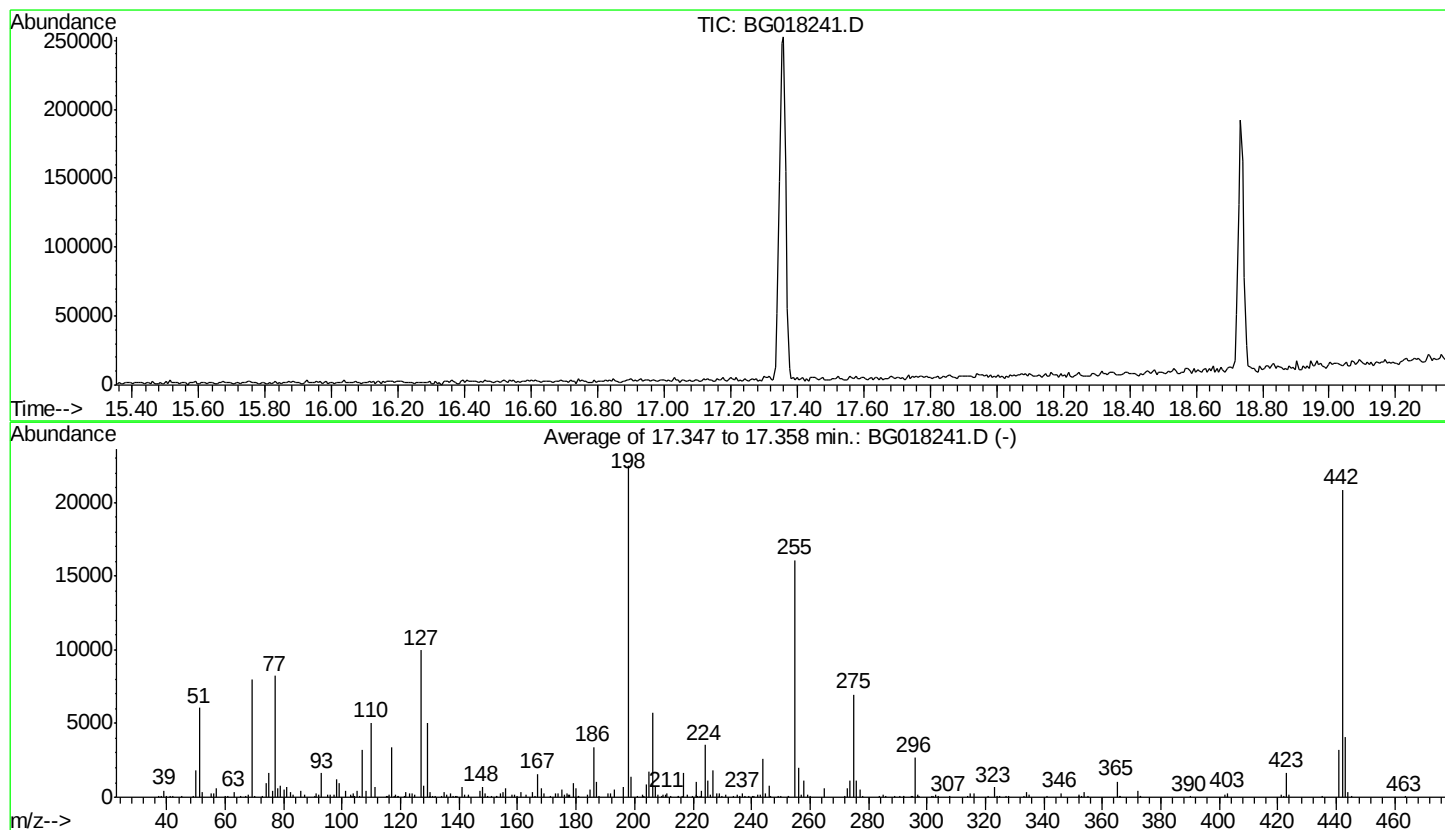

AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.0	6077	PASS
68	69	0.00	2	1.7	136	PASS
69	198	0.00	100	35.5	7985	PASS
70	69	0.00	2	0.8	63	PASS
127	198	10	80	44.3	9958	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	22502	PASS
199	198	5	9	6.2	1393	PASS
275	198	10	60	30.9	6955	PASS
365	198	1	100	4.8	1080	PASS
441	442	0.01	24	15.3	3183	PASS
442	198	50	100	92.7	20864	PASS
443	442	15	24	19.6	4091	PASS

m/z	Abundance
39.10	292.0
40.00	311.0
41.10	294.0
43.10	218.0
45.00	322.0
50.00	1579.0
51.00	4002.0
51.90	231.0
55.00	187.0
56.00	168.0
57.00	467.0
62.90	335.0
66.90	177.0
67.90	216.0
68.90	6610.0
73.10	243.0
74.00	1009.0
75.00	1560.0
76.00	324.0
77.00	6167.0
78.00	535.0
79.00	501.0
79.90	486.0
81.00	675.0
82.10	385.0
86.10	444.0
86.90	277.0
90.80	225.0
92.90	1025.0
95.00	279.0
97.20	195.0
98.00	733.0
99.00	813.0
100.90	440.0
102.80	373.0
104.30	222.0
105.00	453.0
107.00	2492.0
107.90	419.0
110.00	4303.0
111.00	577.0
115.00	246.0
117.00	2616.0
118.10	353.0
118.90	201.0
121.80	319.0
122.90	322.0
123.90	196.0
127.00	7310.0
128.00	786.0
128.90	4160.0
129.90	294.0
134.90	397.0
135.90	425.0
137.10	276.0
138.60	165.0
141.00	871.0
142.10	176.0
143.10	177.0
147.00	204.0
147.90	441.0
148.90	323.0
153.90	305.0
154.90	331.0
156.00	261.0
157.80	252.0
161.00	448.0
165.00	269.0
165.90	172.0
167.00	1192.0
167.90	536.0
168.90	190.0
173.00	383.0
174.00	400.0
175.00	288.0
176.90	422.0
177.90	161.0
178.90	911.0
180.00	580.0
185.00	261.0
186.00	1693.0
187.00	590.0
189.10	267.0
191.00	233.0
192.90	255.0
196.00	321.0
197.90	16098.0
198.90	836.0
202.80	231.0
203.90	866.0
205.00	997.0

Instrument :
BNA_G
ClientSampleId :
DFTPP24

206.10	3564.0
207.00	1193.0
208.00	352.0
211.10	253.0
214.80	172.0
216.80	1017.0
217.90	241.0
220.90	581.0
221.20	557.0
222.80	383.0
224.00	2552.0
225.00	956.0
225.80	170.0
227.00	1377.0
228.80	235.0
237.00	257.0
237.90	175.0
244.00	1748.0
245.90	455.0
246.70	185.0
255.00	10336.0
256.00	1531.0
257.90	885.0
265.00	675.0
272.10	203.0
273.00	391.0
273.80	502.0
275.00	4516.0
276.10	409.0
277.00	220.0
289.00	164.0
296.00	1544.0
296.80	183.0
314.90	247.0
323.00	513.0
333.90	288.0
346.00	262.0
353.10	207.0
354.10	194.0
355.20	159.0
365.00	538.0
372.10	230.0
402.70	191.0
423.00	729.0
441.10	2029.0
442.00	10672.0
443.00	1950.0
444.00	330.0
463.50	230.0

Instrument :
BNA_G
ClientSampleId :
DFTPP24

m/z	Abundance
39.00	635.0
39.70	308.0
43.10	166.0
43.90	189.0
49.10	204.0
50.00	2122.0
51.00	7372.0
52.00	630.0
55.00	239.0
55.90	328.0
57.00	873.0
63.00	492.0
65.10	171.0
68.90	9405.0
70.20	191.0
73.00	192.0
74.00	977.0
75.00	1666.0
76.00	512.0
77.00	10243.0
78.00	757.0
79.00	903.0
79.90	577.0
81.00	676.0
82.10	478.0
83.00	347.0
85.90	472.0
86.90	310.0
91.00	589.0
91.90	446.0
93.00	2130.0
95.00	258.0
97.20	384.0
98.00	1500.0
98.90	1088.0
100.90	427.0
102.90	195.0
103.90	418.0
105.00	453.0
107.00	3124.0
108.00	643.0
110.00	5742.0
111.00	944.0
115.60	392.0
116.90	3621.0
118.10	162.0
119.10	159.0
121.10	313.0
121.80	231.0
123.00	551.0
124.00	201.0
125.00	230.0
127.00	10912.0
128.00	822.0
129.00	5627.0
130.10	434.0
131.80	151.0
133.80	297.0
134.80	283.0
137.00	291.0
137.90	167.0
140.90	593.0
141.90	297.0
143.30	179.0
147.10	392.0
147.80	847.0
148.80	249.0
149.70	173.0
151.00	260.0
152.80	196.0
154.00	283.0
154.90	481.0
156.00	670.0
159.00	254.0
161.10	157.0
162.90	199.0
164.90	439.0
167.00	1624.0
168.00	586.0
168.90	187.0
171.10	239.0
173.00	474.0
174.00	204.0
175.00	504.0
176.00	490.0
177.10	441.0
178.00	253.0
178.90	758.0
180.00	463.0
180.80	259.0
183.90	241.0

Instrument :
BNA_G
ClientSampleId :
DFTPP24

184.90	608.0
186.00	4323.0
186.90	1037.0
188.00	221.0
188.90	417.0
191.10	303.0
191.90	579.0
193.00	662.0
196.00	974.0
197.90	25808.0
198.90	1618.0
200.90	226.0
202.80	208.0
203.90	787.0
205.00	2156.0
206.00	6681.0
207.00	1155.0
208.00	347.0
209.20	227.0
210.70	417.0
216.10	187.0
216.90	1884.0
217.80	273.0
221.00	1060.0
222.90	519.0
224.00	4335.0
225.00	1218.0
225.90	310.0
226.90	1740.0
227.90	421.0
229.10	382.0
229.90	193.0
230.90	282.0
233.70	231.0
235.00	347.0
236.90	260.0
239.00	343.0
240.30	153.0
242.10	174.0
244.00	3049.0
244.90	303.0
246.00	746.0
249.00	299.0
252.60	249.0
255.00	19568.0
256.00	2142.0
257.10	380.0
258.00	1079.0
260.10	159.0
265.00	692.0
272.80	814.0
273.90	1304.0
275.00	8550.0
276.00	1353.0
277.00	581.0
278.00	190.0
283.00	261.0
284.90	211.0
285.90	175.0
291.90	175.0
295.90	3168.0
296.90	465.0
301.70	152.0
302.90	374.0
303.90	163.0
307.60	190.0
314.90	339.0
316.00	359.0
321.10	201.0
323.10	682.0
323.90	164.0
324.80	171.0
333.90	343.0
345.80	333.0
351.90	170.0
353.90	517.0
365.00	1123.0
366.20	290.0
372.20	509.0
372.90	305.0
402.00	173.0
403.00	533.0
421.10	198.0
422.00	256.0
423.00	1955.0
423.90	189.0
435.10	183.0
441.00	3305.0
442.00	24072.0
443.10	4632.0
444.10	284.0

Instrument :
BNA_G
ClientSampleId :
DFTPP24

m/z	Abundance
37.00	171.0
38.00	215.0
39.10	414.0
42.10	151.0
50.00	1654.0
51.00	6857.0
51.90	242.0
55.10	239.0
55.90	260.0
57.00	464.0
60.10	183.0
61.00	156.0
63.00	256.0
67.00	203.0
67.80	193.0
69.00	8490.0
72.70	210.0
74.00	980.0
75.00	1809.0
76.10	580.0
77.00	9083.0
78.00	433.0
79.00	861.0
79.90	426.0
81.00	794.0
82.10	247.0
82.80	174.0
86.00	307.0
90.90	295.0
91.90	161.0
93.00	1684.0
96.00	421.0
98.00	1494.0
98.90	907.0
100.90	370.0
103.10	206.0
103.90	332.0
105.00	411.0
106.00	319.0
107.00	3952.0
108.00	349.0
108.90	266.0
110.00	5188.0
111.00	654.0
116.10	403.0
117.00	4007.0
117.80	338.0
121.90	466.0
123.00	753.0
123.90	328.0
124.80	354.0
127.00	11653.0
128.00	834.0
128.90	5294.0
130.00	634.0
130.80	187.0
135.00	488.0
135.90	165.0
137.20	178.0
139.00	213.0
140.90	641.0
142.90	318.0
147.00	796.0
148.00	914.0
149.00	303.0
152.10	163.0
153.00	221.0
154.00	195.0
155.00	355.0
155.90	909.0
157.90	280.0
159.00	185.0
160.00	309.0
161.00	350.0
162.90	229.0
164.90	384.0
166.90	1888.0
167.90	815.0
169.00	414.0
173.90	316.0
175.00	714.0
176.90	483.0
178.90	1111.0
179.90	875.0
181.00	316.0
183.90	269.0
185.00	662.0
186.00	4171.0
187.00	1468.0
188.80	237.0
191.10	314.0

Instrument :
BNA_G
ClientSampleId :
DFTPP24

192.00	340.0
193.10	571.0
196.00	797.0
197.90	25600.0
199.00	1726.0
202.70	203.0
203.10	278.0
203.90	1069.0
205.00	2169.0
206.00	6840.0
207.00	1204.0
207.90	315.0
209.90	417.0
211.00	605.0
212.20	179.0
215.10	161.0
217.00	2006.0
219.60	213.0
220.90	1483.0
221.60	193.0
222.20	168.0
222.90	506.0
224.00	3778.0
225.00	1238.0
227.00	2413.0
228.00	340.0
229.00	385.0
231.00	231.0
235.00	295.0
235.90	156.0
237.00	341.0
241.00	223.0
242.00	425.0
243.20	603.0
244.00	2974.0
245.00	607.0
246.00	1138.0
249.80	163.0
252.80	233.0
255.00	18392.0
256.00	2433.0
257.20	197.0
257.90	1324.0
259.00	406.0
264.90	370.0
273.00	546.0
273.90	1507.0
275.00	7800.0
276.00	1743.0
277.00	685.0
283.90	289.0
285.00	299.0
290.90	154.0
292.10	203.0
294.50	160.0
295.00	190.0
296.00	3263.0
297.10	238.0
302.30	205.0
303.00	153.0
314.10	208.0
314.80	154.0
315.90	321.0
320.90	189.0
323.10	780.0
324.00	177.0
326.90	168.0
328.10	181.0
333.00	271.0
334.00	415.0
334.90	445.0
341.00	162.0
345.90	295.0
352.10	520.0
354.00	309.0
364.90	1581.0
365.90	341.0
372.00	508.0
373.10	160.0
390.00	157.0
402.10	363.0
402.90	318.0
421.00	389.0
423.10	2312.0
423.90	279.0
441.10	4216.0
442.00	27848.0
443.10	5693.0
444.00	456.0
445.10	152.0

Instrument :
BNA_G
ClientSampleId :
DFTPP24

Scan 2491 (17.323 min): BG018241.D
DFTPP24

m/z	Abundance
39.90	188.0
43.10	286.0
44.00	152.0
69.00	183.0
70.90	187.0
72.90	184.0
76.90	258.0
109.00	176.0
122.90	321.0
152.00	240.0
156.90	257.0
170.80	164.0
189.00	310.0
207.10	463.0
208.00	173.0
283.20	167.0

Instrument :
BNA_G
ClientSampleId :
DFTPP24