
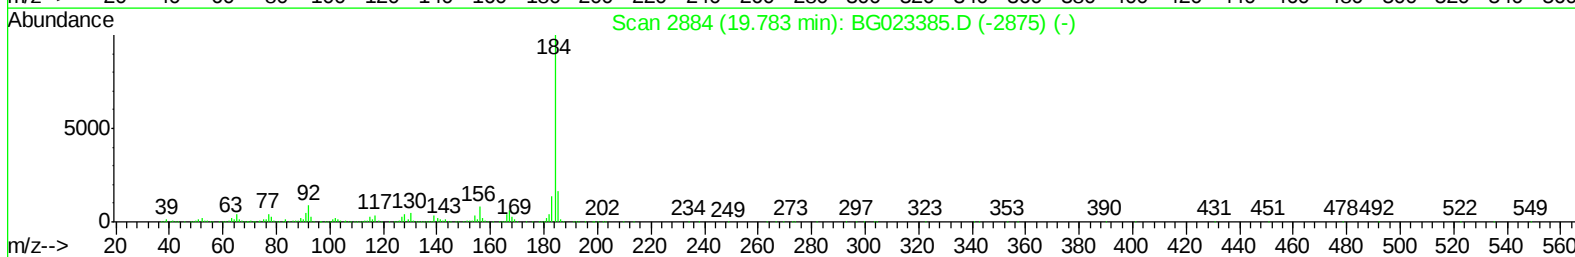
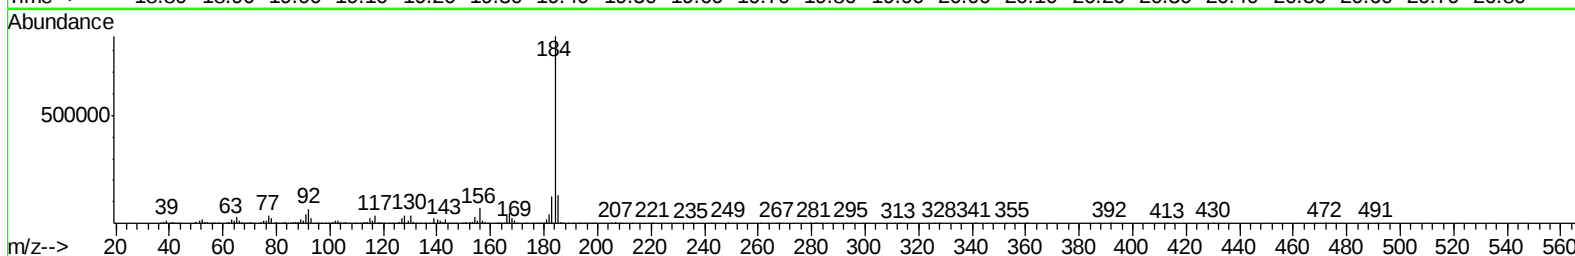


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080316\
Data File : BG023419.D
Acq On : 3 Aug 2016 9:17
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 04 07:36:08 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 01 19:22:14 2016
Response via : Initial Calibration

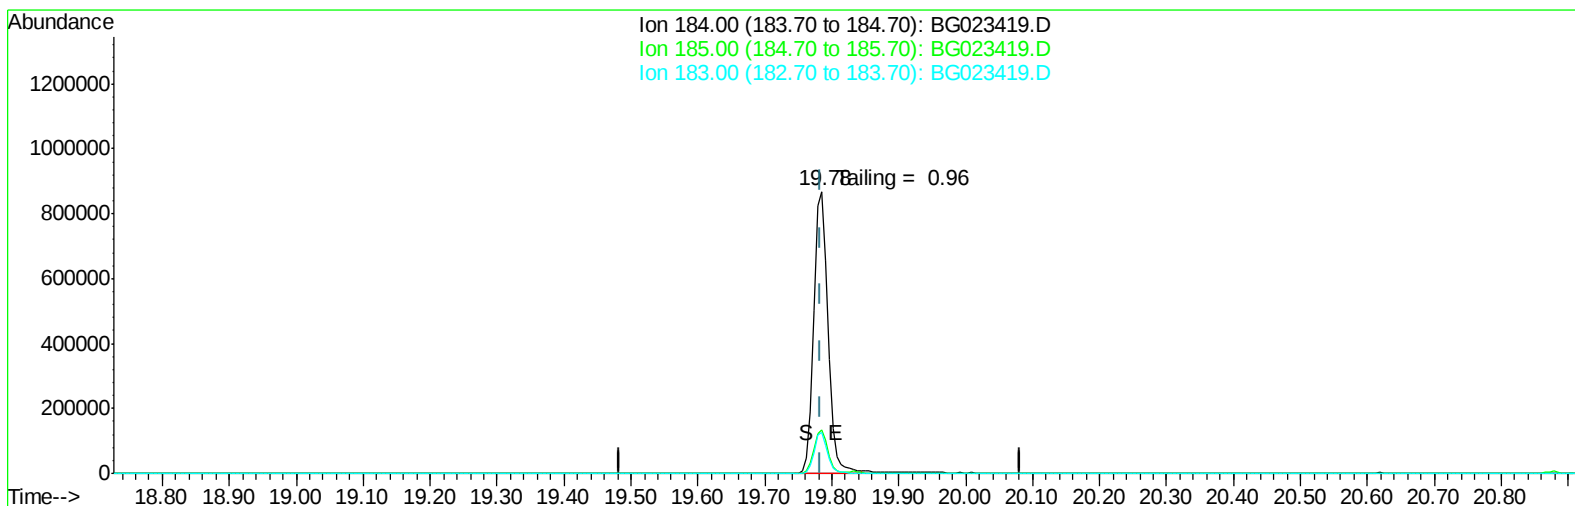

TIC: BG023419.D

(76) Benzidine




19.785min (+0.002) 564648.30ng

response 1334196

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	15.39
183.00	13.40	14.63
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080316\
Data File : BG023419.D
Acq On : 3 Aug 2016 9:17
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 04 07:36:08 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 01 19:22:14 2016
Response via : Initial Calibration

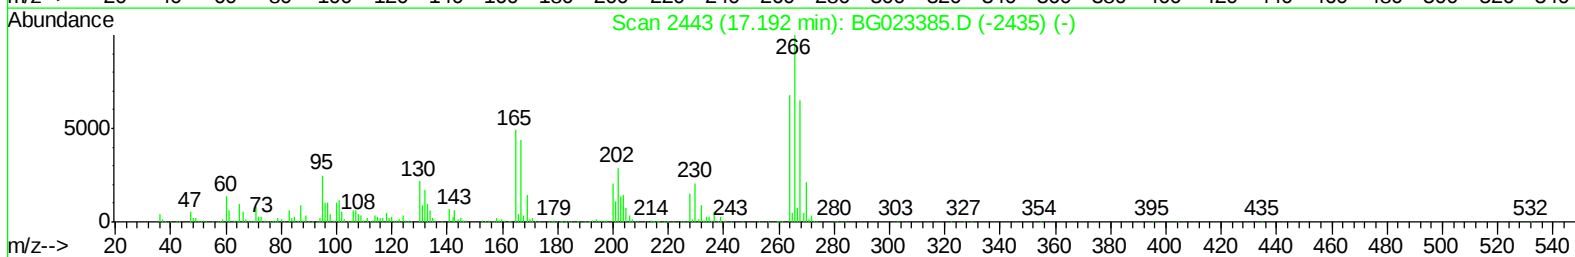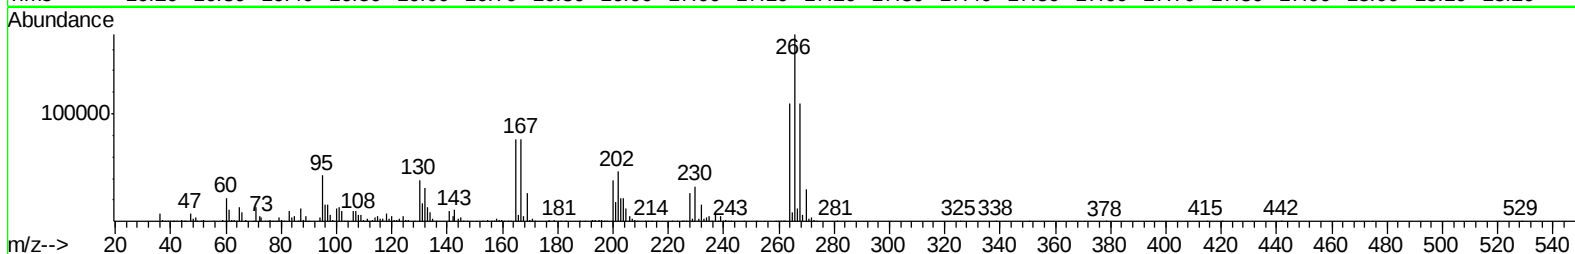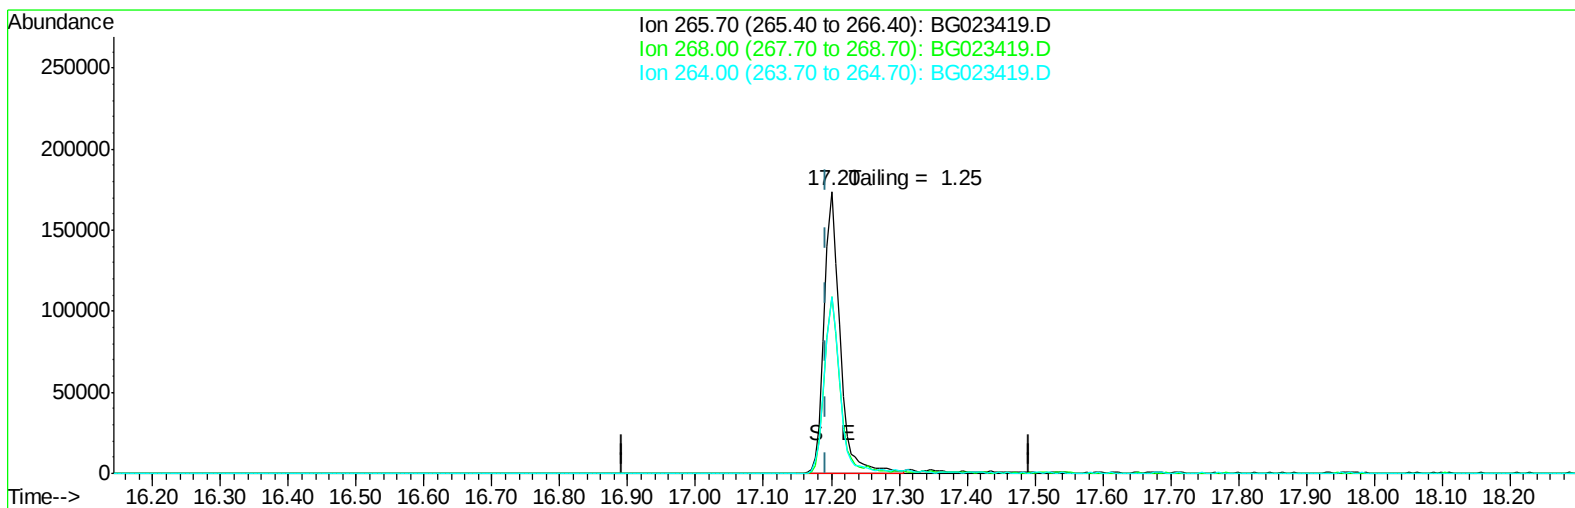

TIC: BG023419.D

(69) Pentachlorophenol (C)

17.200min (+0.008) 134609.04ng

response 278187

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	62.83
264.00	63.20	62.73
0.00	0.00	0.00