
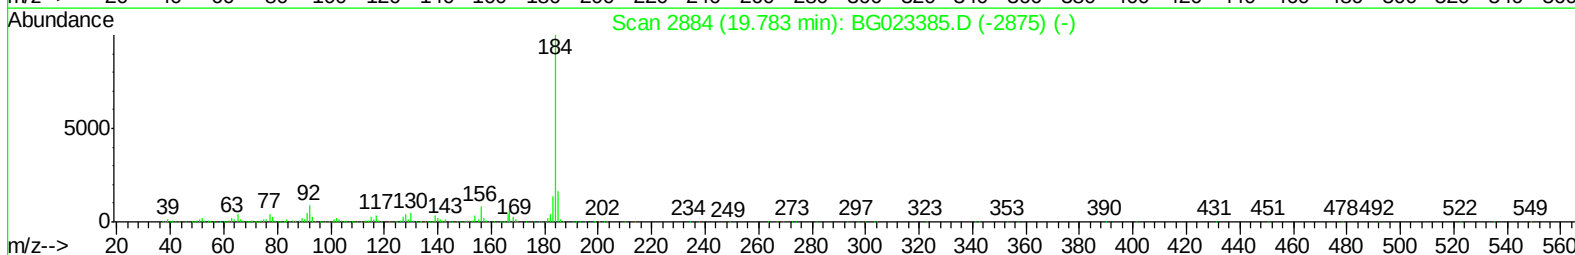
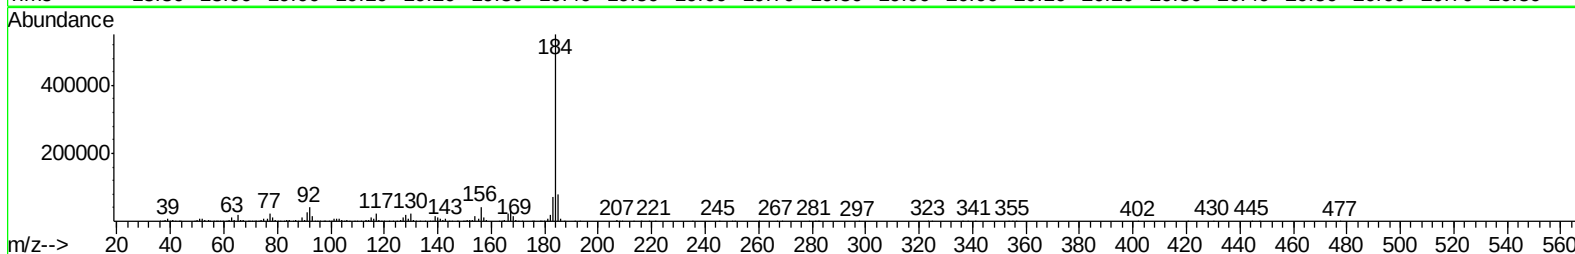


Data Path : Z:\HPCHEM1\BNA\_G\DATA\BG080316\  
 Data File : BG023428.D  
 Acq On : 3 Aug 2016 16:36  
 Operator : UM/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 04 07:37:37 2016  
 Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG080116.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Aug 01 19:22:14 2016  
 Response via : Initial Calibration

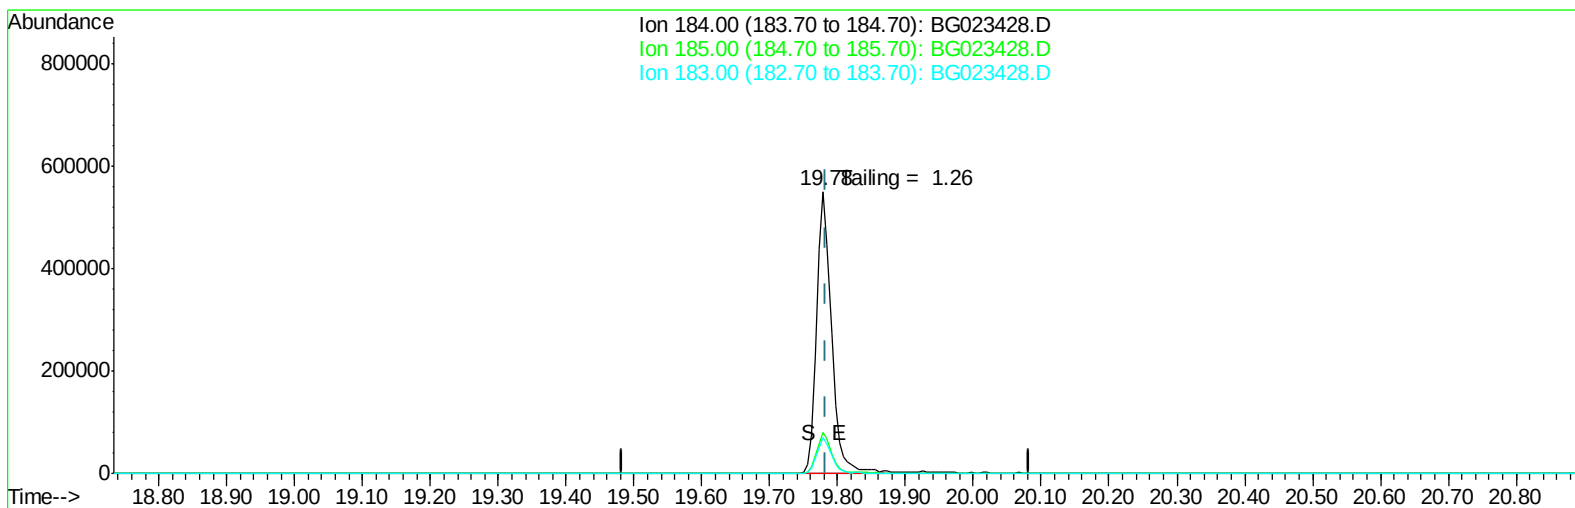

TIC: BG023428.D

(76) Benzidine




19.779min (-0.004) 246018.25ng

response 834353

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.80 | 14.63 |
| 183.00 | 13.40 | 12.82 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_G\DATA\BG080316\  
Data File : BG023428.D  
Acq On : 3 Aug 2016 16:36  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 04 07:37:37 2016  
Quant Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG080116.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 01 19:22:14 2016  
Response via : Initial Calibration

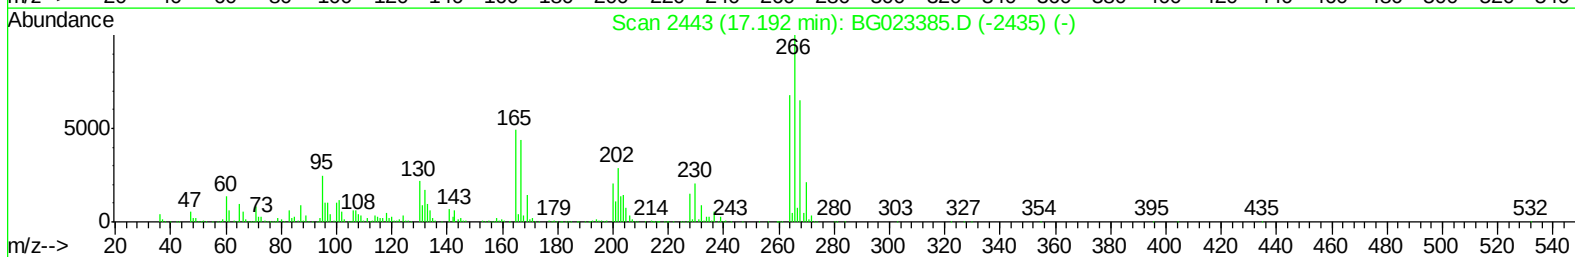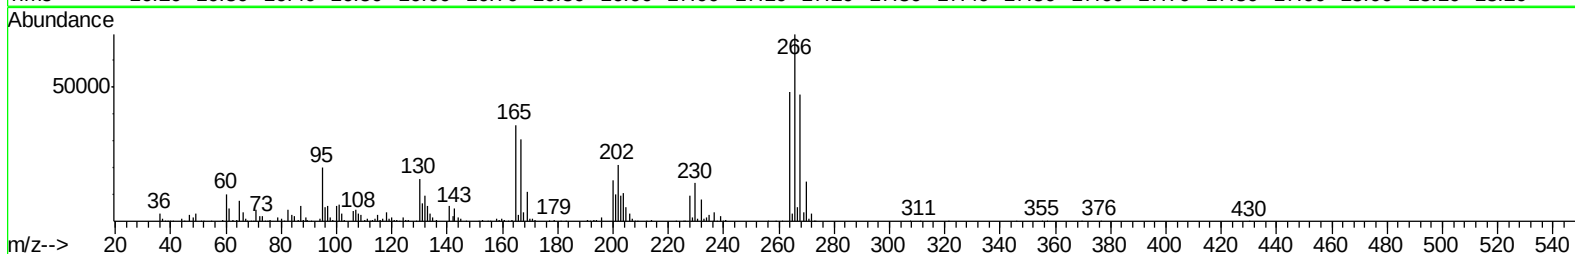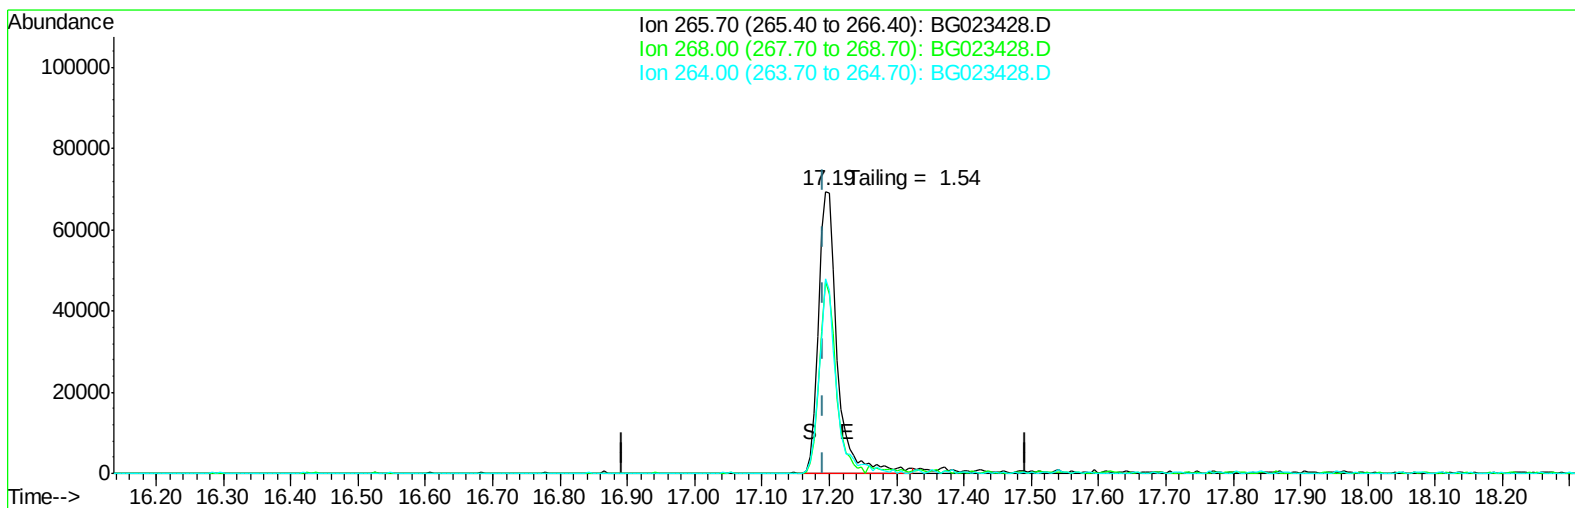

TIC: BG023428.D

(69) Pentachlorophenol (C)

17.194min (+0.002) 259656.81ng

response 137049

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 64.90 | 68.12 |
| 264.00 | 63.20 | 69.29 |
| 0.00   | 0.00  | 0.00  |