


Data Path : Z:\HPCHEM1\BNA G\DATA\BG080316\
 Data File : BG023419.D
 Acq On : 3 Aug 2016 9:17
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 01 19:22:14 2016

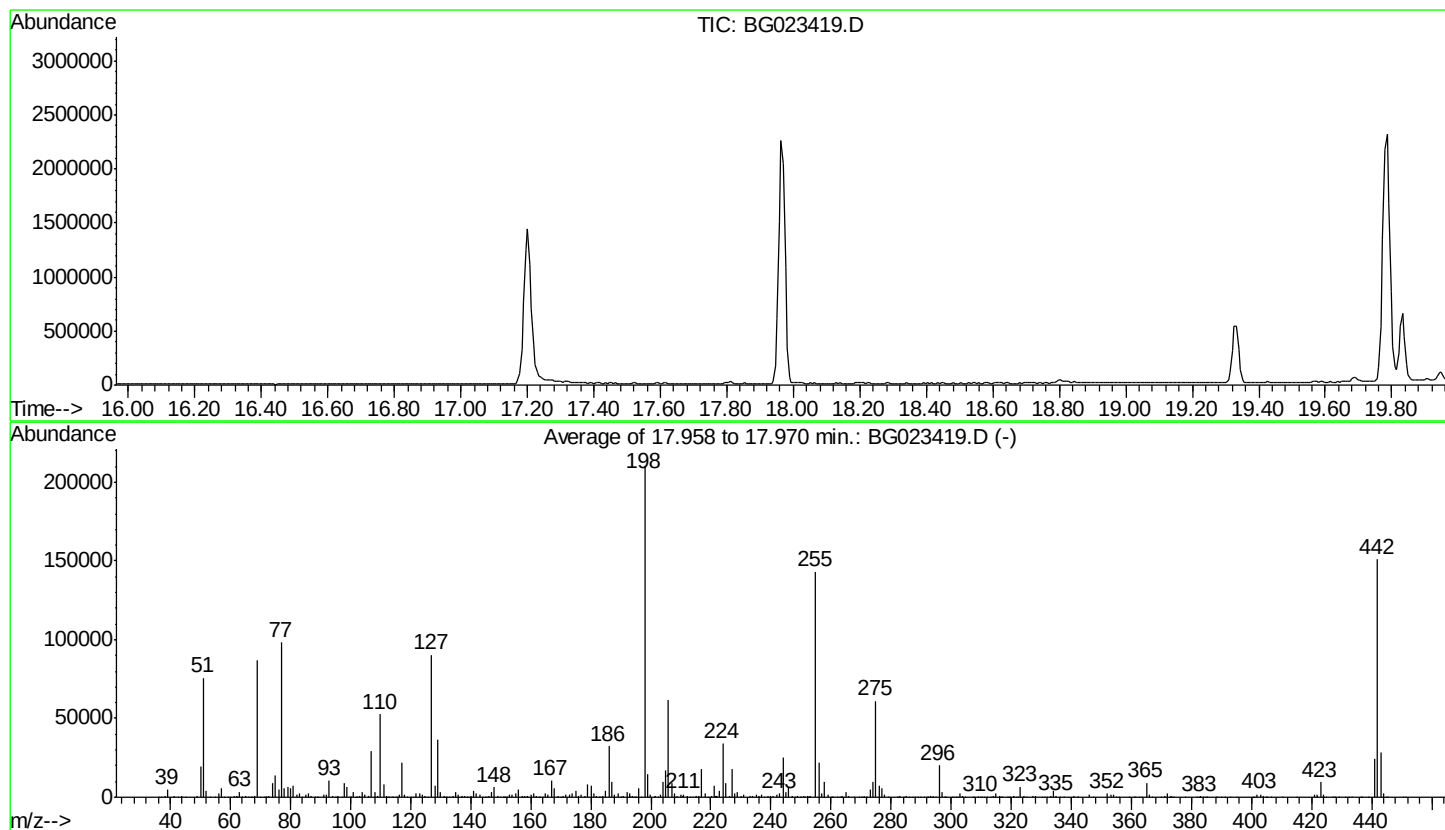

AutoFind: Scans 2574, 2575, 2576; Background Corrected with Scan 2567

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	75836	PASS
68	69	0.00	2	1.4	1193	PASS
69	198	0.00	100	41.4	87090	PASS
70	69	0.00	2	0.4	375	PASS
127	198	10	80	43.0	90573	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	210496	PASS
199	198	5	9	6.9	14420	PASS
275	198	10	60	29.0	61005	PASS
365	198	1	100	4.4	9217	PASS
441	442	0.01	24	16.0	24128	PASS
442	198	50	100	71.7	150856	PASS
443	442	15	24	18.7	28272	PASS