


Data Path : Z:\HPCHEM1\BNA G\DATA\BG080316\
Data File : BG023428.D
Acq On : 3 Aug 2016 16:36
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG080116.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 01 19:22:14 2016

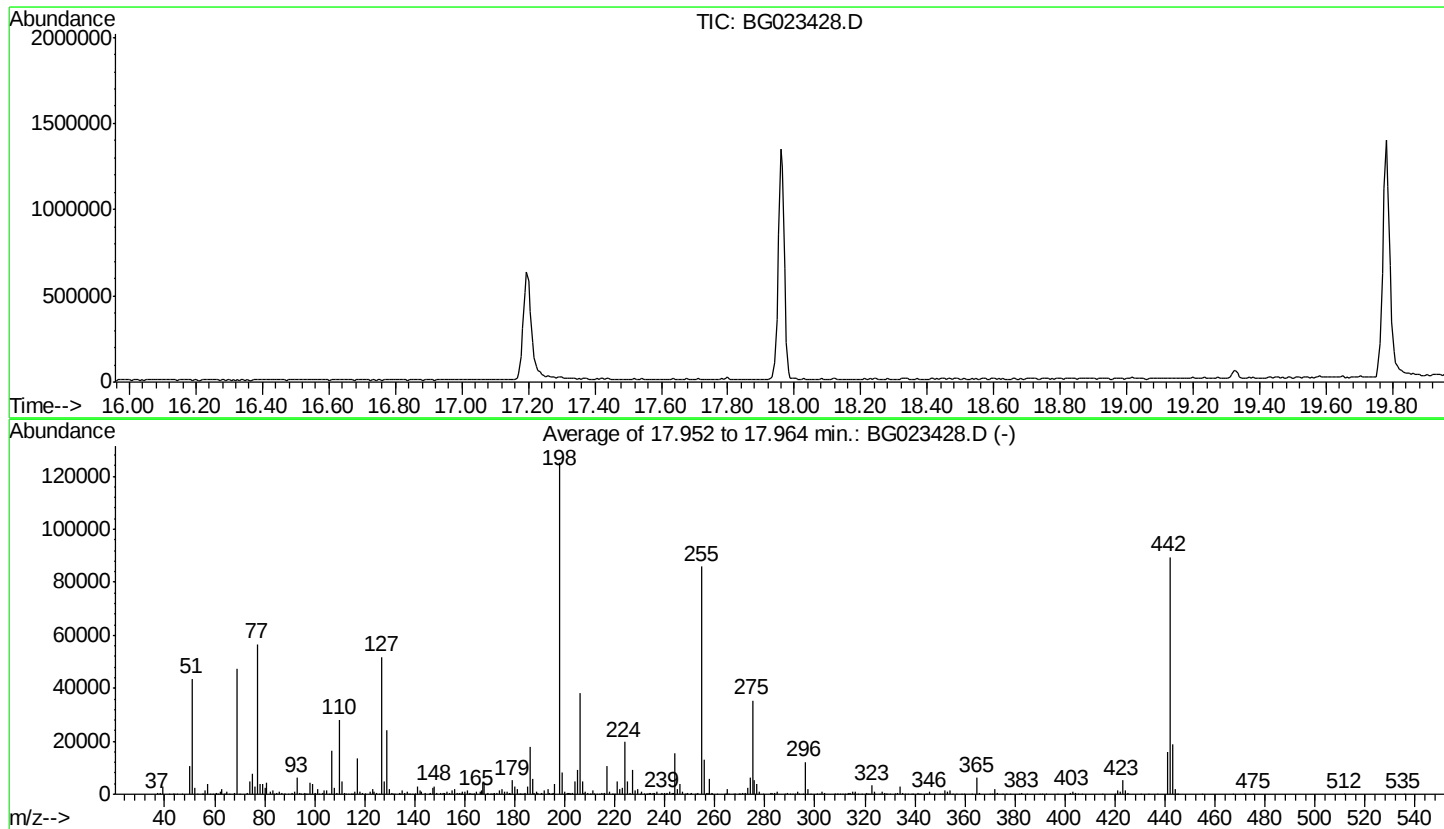

AutoFind: Scans 2573, 2574, 2575; Background Corrected with Scan 2567

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	43647	PASS
68	69	0.00	2	1.0	457	PASS
69	198	0.00	100	37.9	47445	PASS
70	69	0.00	2	0.4	213	PASS
127	198	10	80	41.3	51738	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	125160	PASS
199	198	5	9	6.7	8444	PASS
275	198	10	60	28.3	35381	PASS
365	198	1	100	4.9	6160	PASS
441	442	0.01	24	18.0	16153	PASS
442	198	50	100	71.5	89546	PASS
443	442	15	24	21.0	18828	PASS