
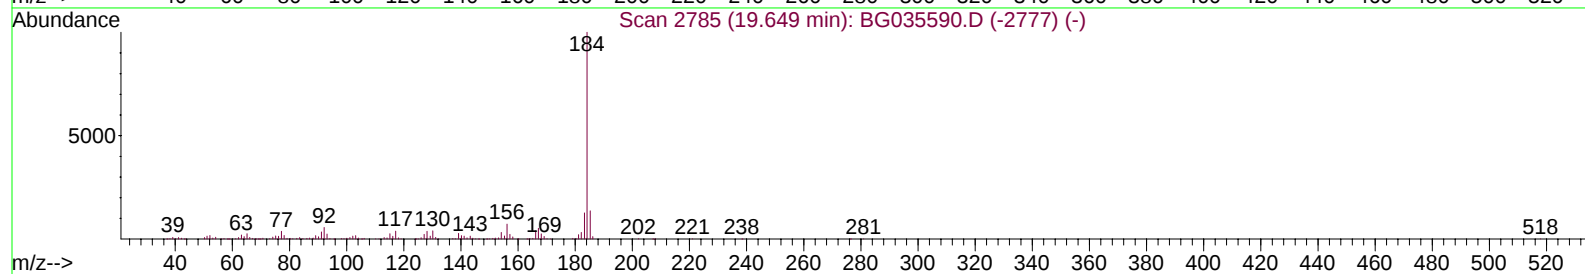
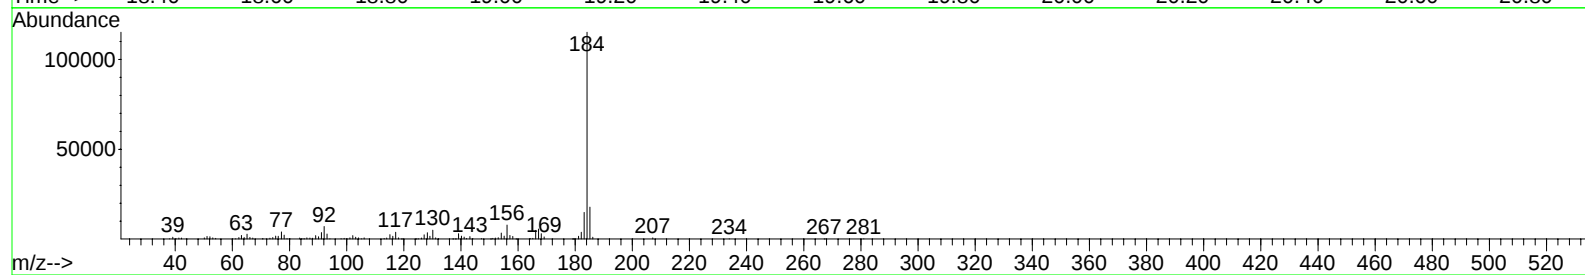


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080318\
Data File : BG036088.D
Acq On : 3 Aug 2018 11:05
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 18:35:34 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

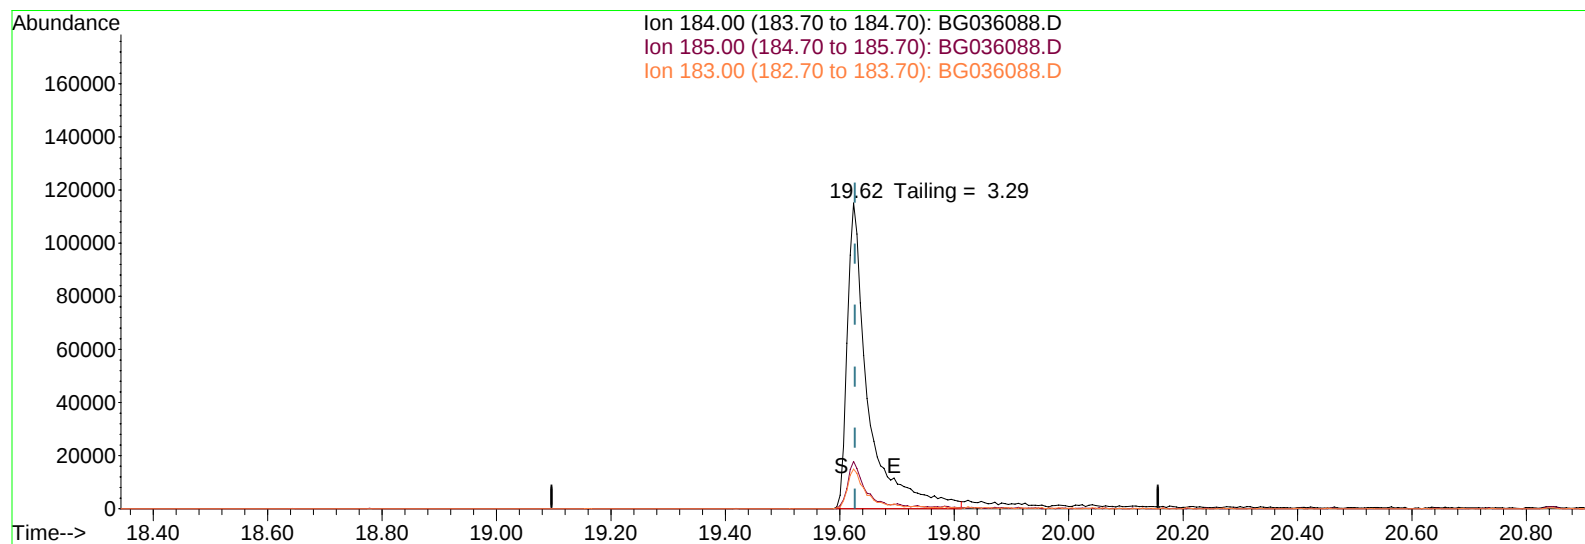

(76) Benzidine




19.624min (-0.002) 67106.73ng

response 292866

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.50
183.00	13.30	12.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080318\
Data File : BG036088.D
Acq On : 3 Aug 2018 11:05
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 18:35:34 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

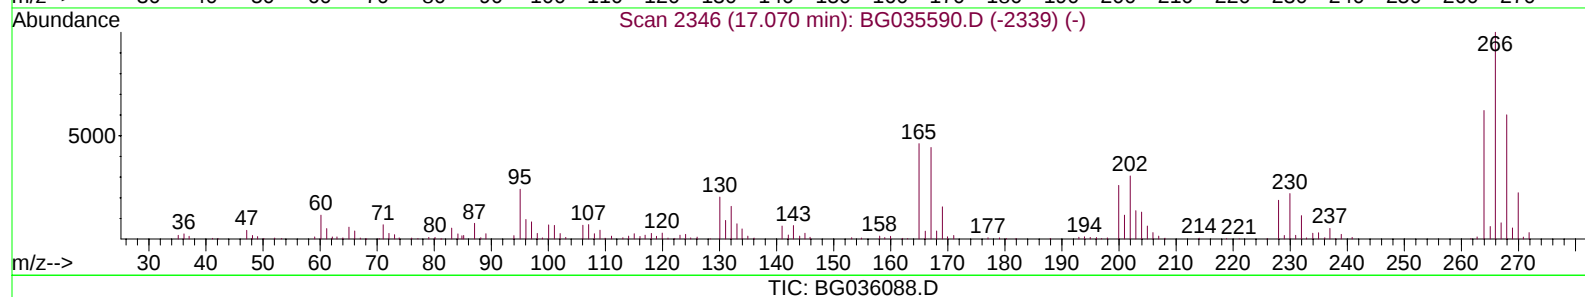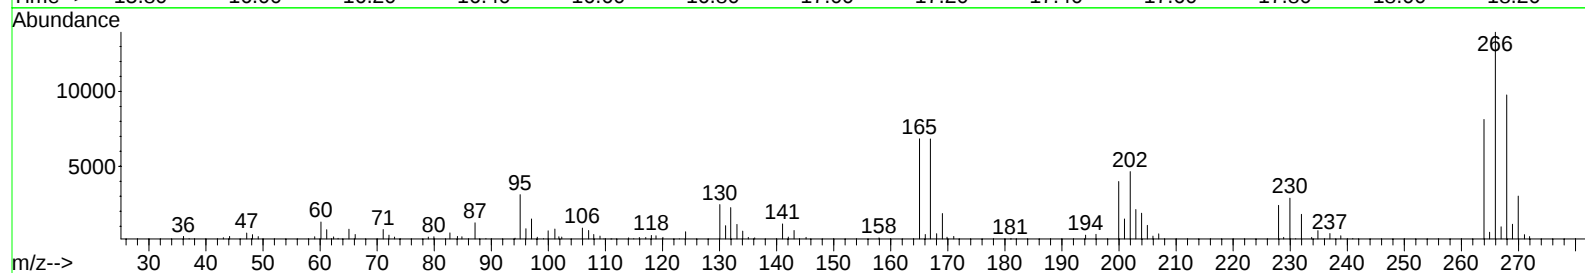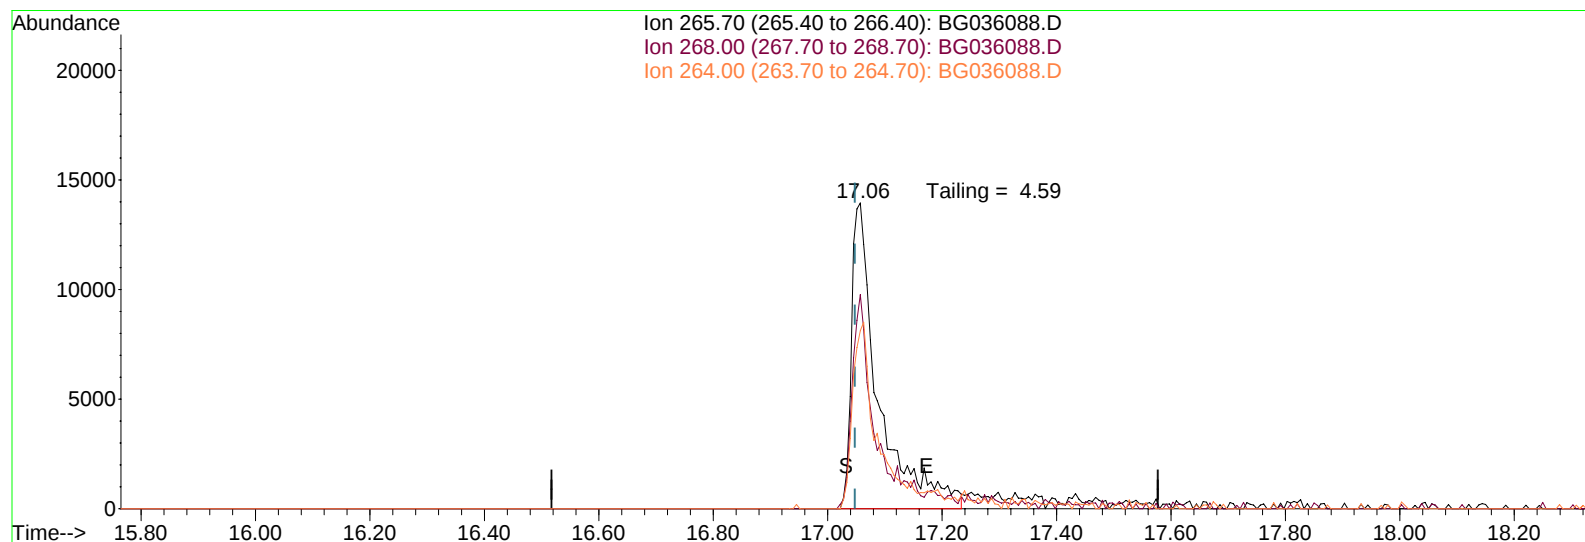

(69) Pentachlorophenol (C)

17.057min (+0.010) 42003.79ng

response 38820

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	70.02
264.00	62.00	58.25
0.00	0.00	0.00