
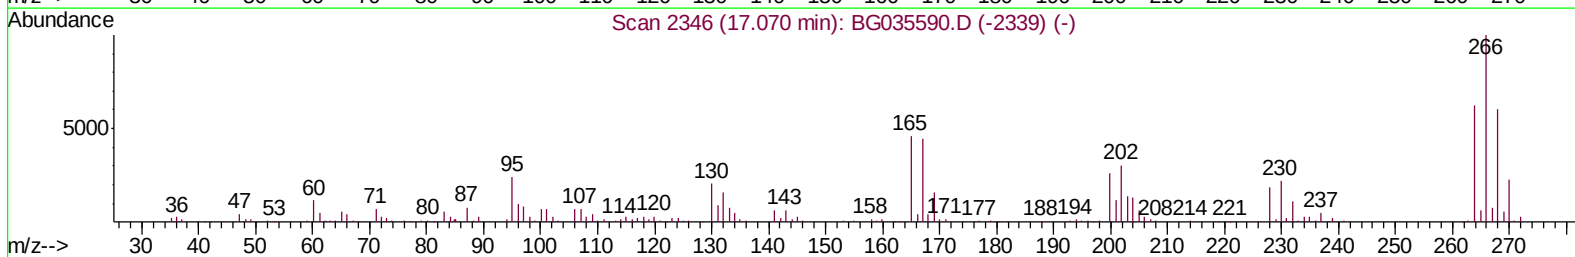
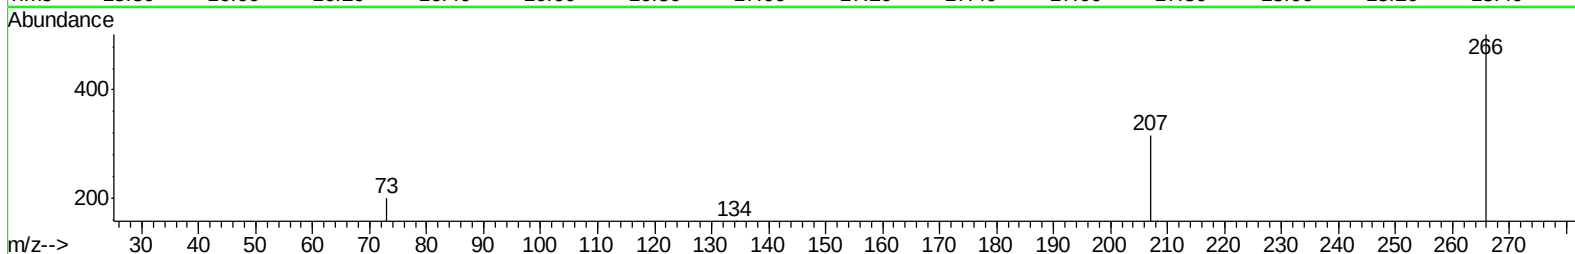


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_G\DATA\BG080318\  
Data File : BG036107.D  
Acq On : 4 Aug 2018 00:07  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 01:47:27 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG071218.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jul 31 12:30:06 2018  
Response via : Initial Calibration

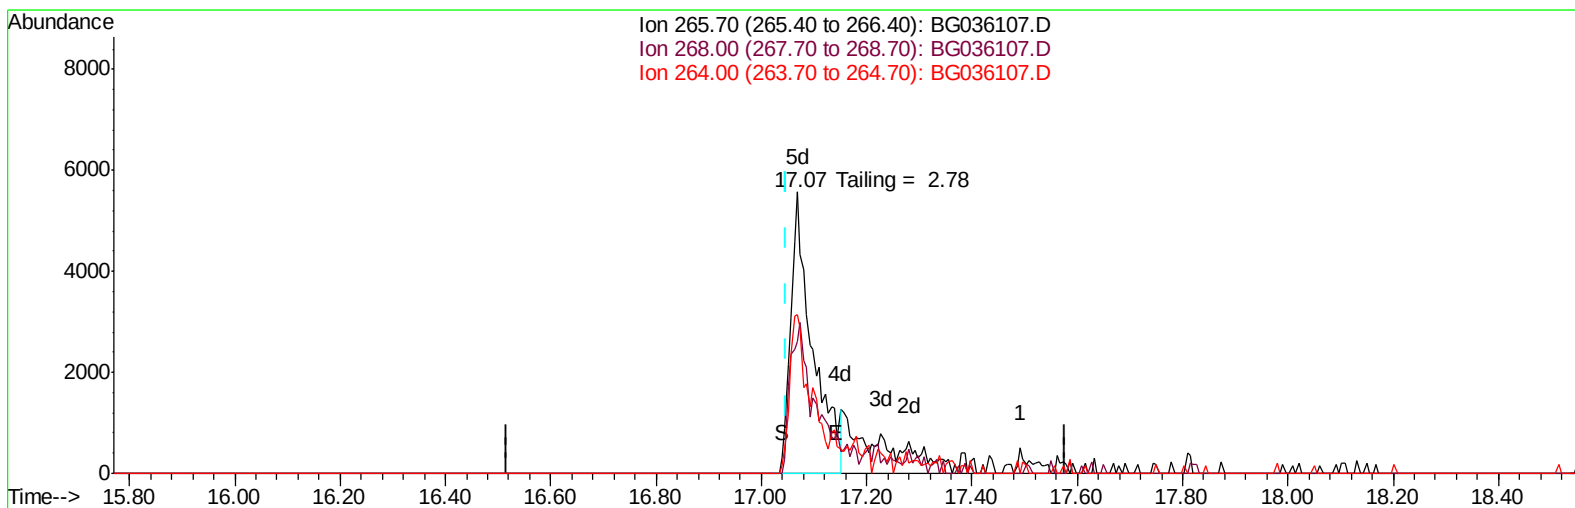

TIC: BG036107.D

(69) Pentachlorophenol (C)




17.491min (+0.444) 1278.11ng

response 865

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 0.00# |
| 264.00 | 62.00 | 0.00# |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_G\DATA\BG080318\  
Data File : BG036107.D  
Acq On : 4 Aug 2018 00:07  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 01:47:27 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG071218.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jul 31 12:30:06 2018  
Response via : Initial Calibration

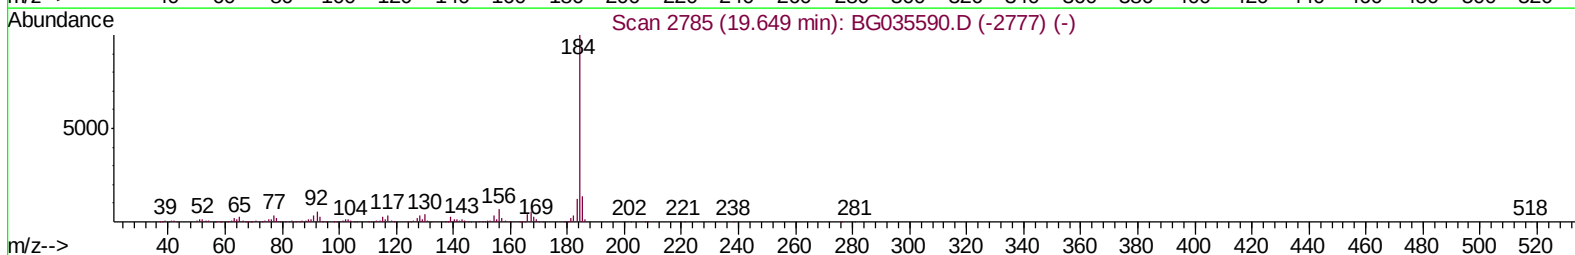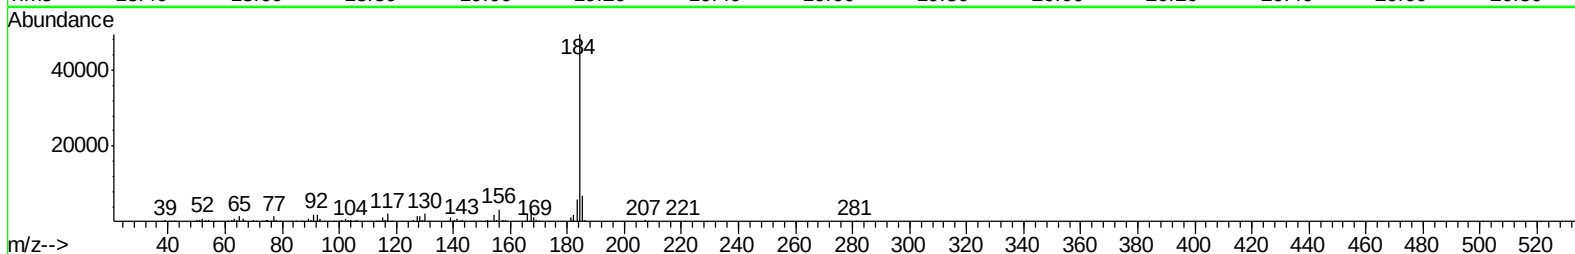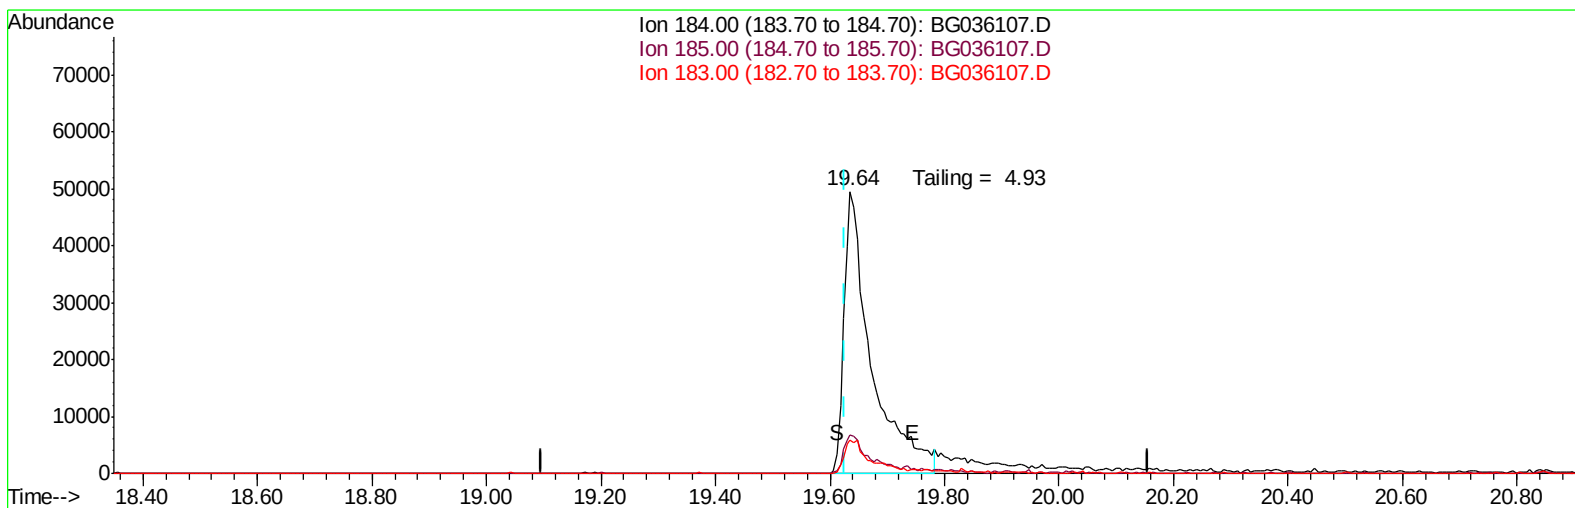

TIC: BG036107.D

(76) Benzidine

19.636min (+0.009) 114548.14ng

response 162621

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 13.90 | 13.74 |
| 183.00 | 13.30 | 11.96 |
| 0.00   | 0.00  | 0.00  |