
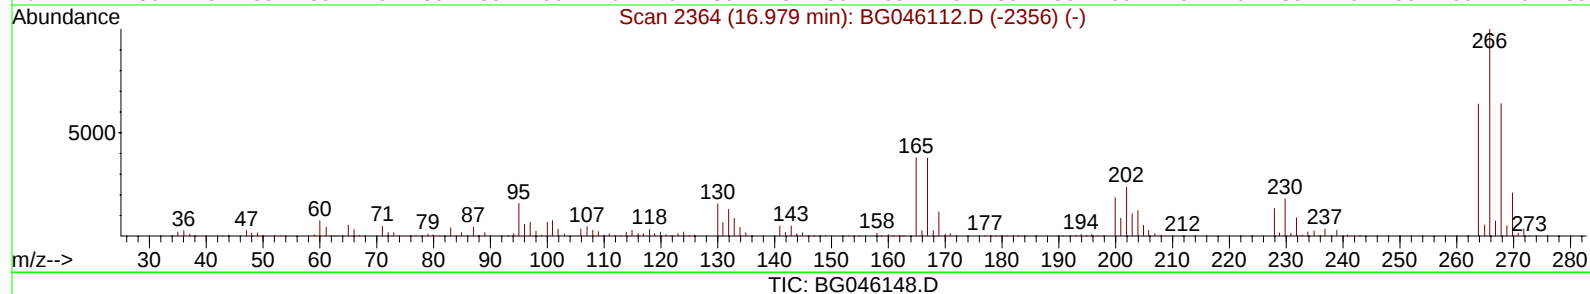
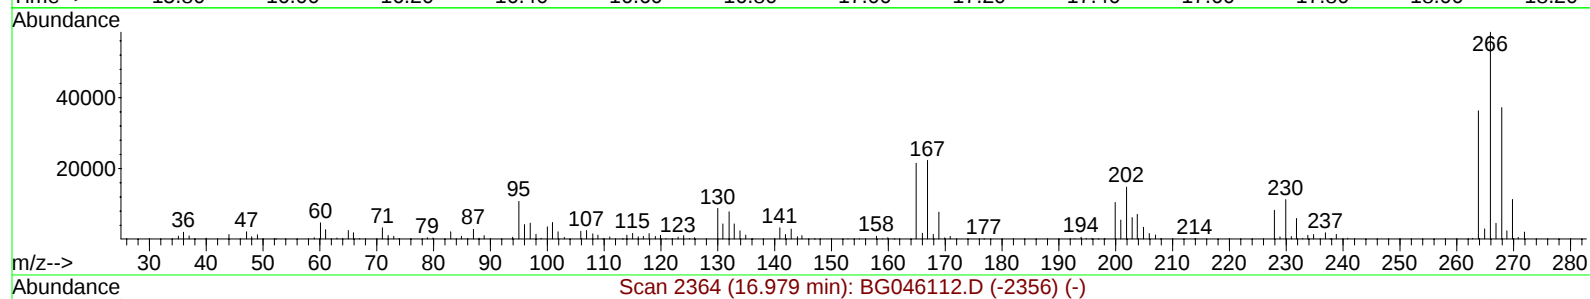


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG080320\
Data File : BG046148.D
Acq On : 3 Aug 2020 10:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 19:00:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 30 18:43:49 2020
Response via : Initial Calibration

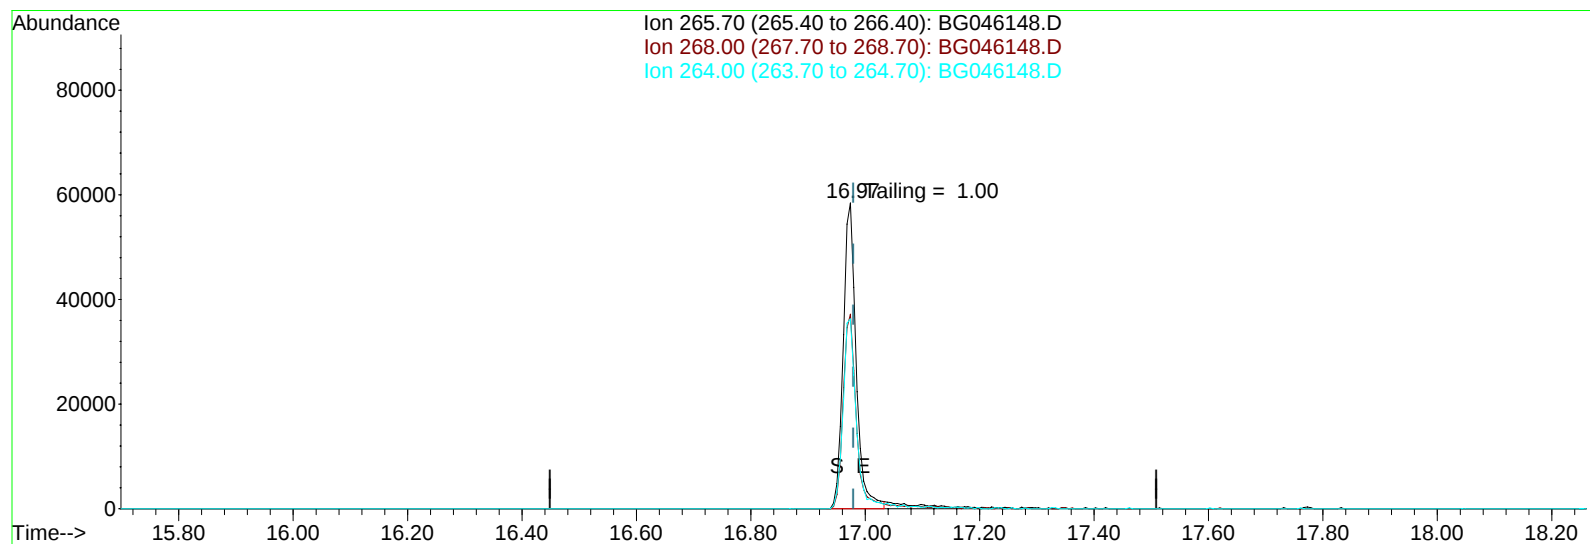

(70) Pentachlorophenol (C)




16.974min (-0.005) 37659.98ng

response 95119

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	63.62
264.00	63.90	62.07
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG080320\
 Data File : BG046148.D
 Acq On : 3 Aug 2020 10:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 19:00:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 30 18:43:49 2020
 Response via : Initial Calibration

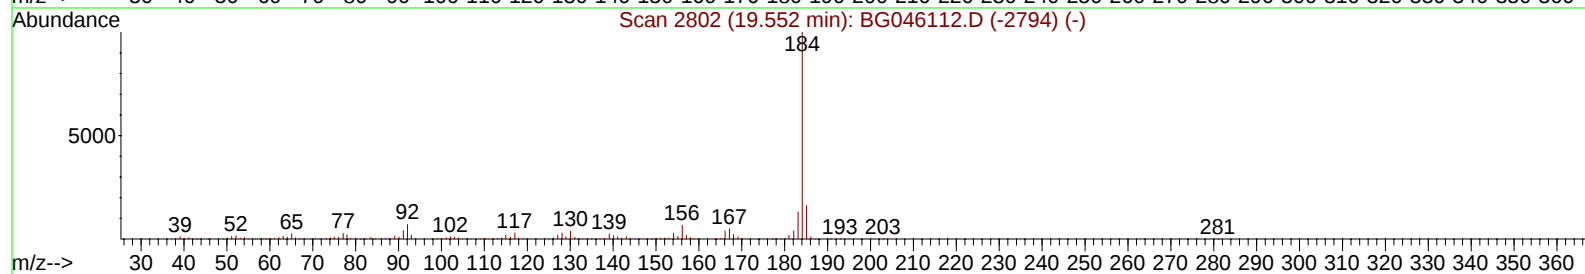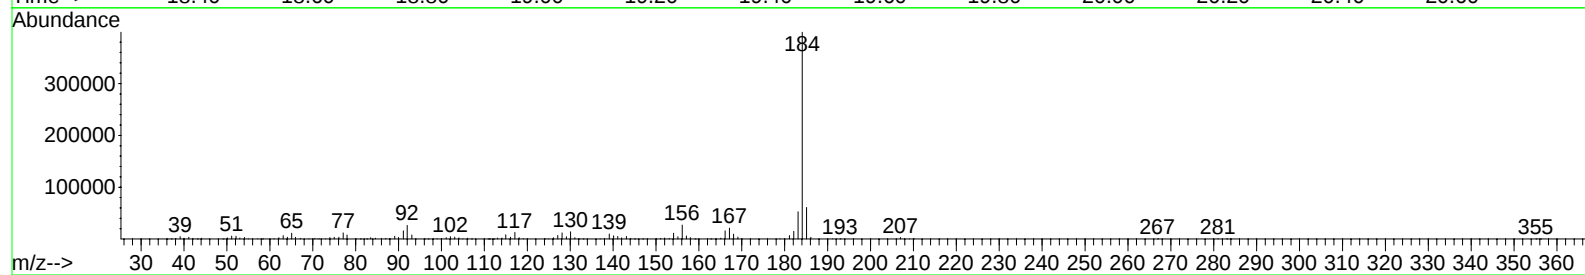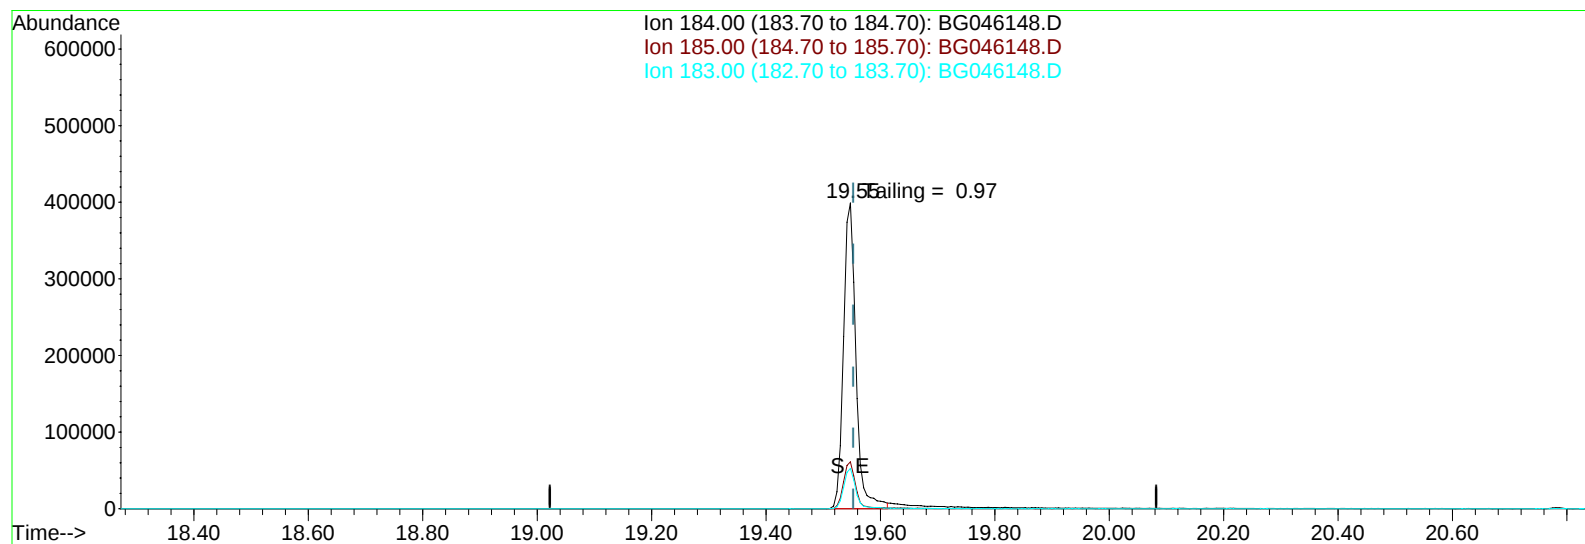

TIC: BG046148.D

(77) Benzidine

19.547min (-0.005) 0.00ng

response 630717

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	15.31
183.00	13.10	13.17
0.00	0.00	0.00