


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080320\
 Data File : BG046148.D
 Acq On : 3 Aug 2020 10:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG073020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 30 18:43:49 2020

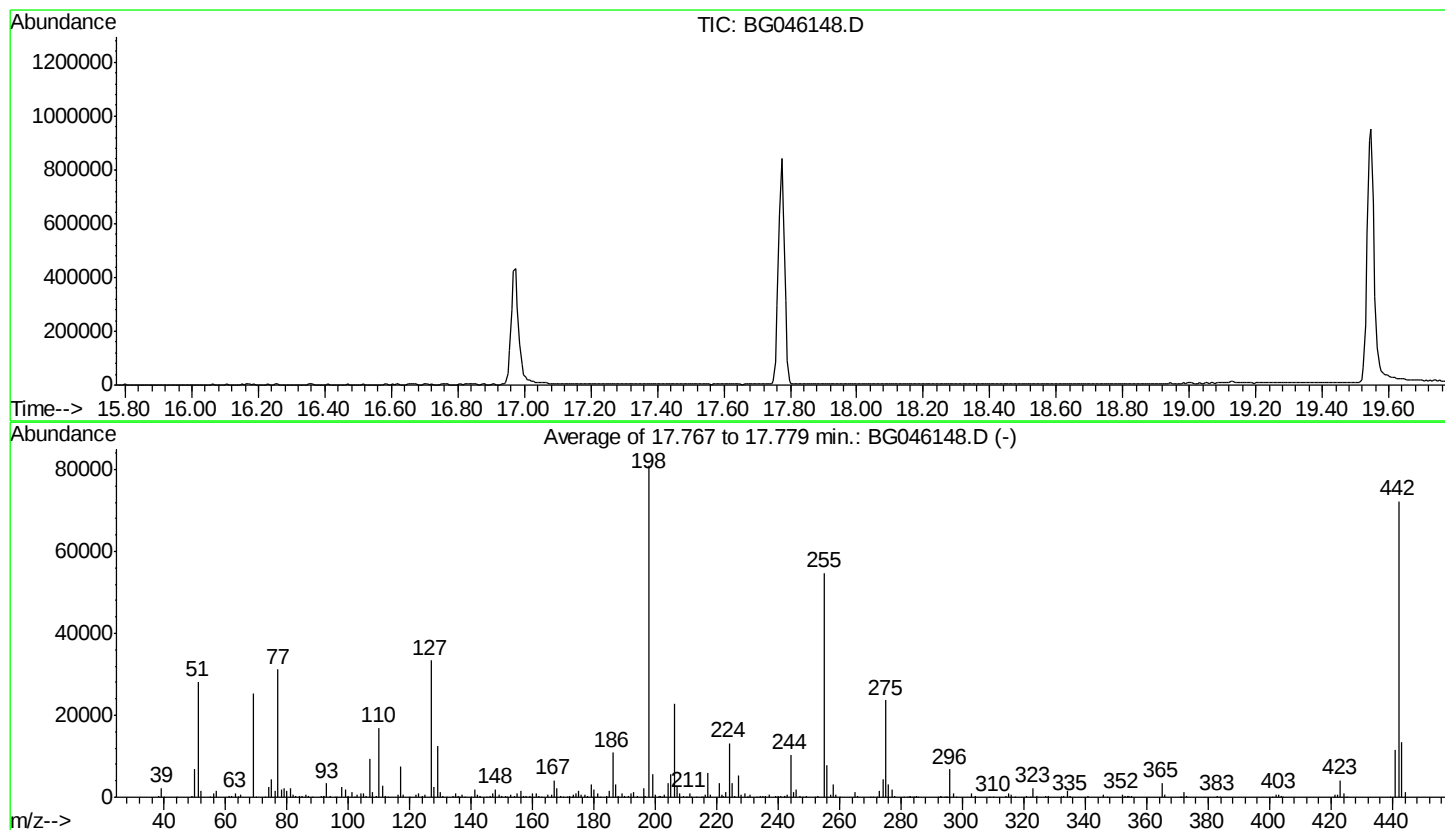

AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	28189	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.5	25456	PASS
70	69	0.00	2	0.6	157	PASS
127	198	10	80	41.2	33322	PASS
197	198	0.00	2	0.4	284	PASS
198	198	100	100	100.0	80922	PASS
199	198	5	9	7.1	5706	PASS
275	198	10	60	29.3	23672	PASS
365	198	1	100	4.3	3460	PASS
441	198	0.01	100	14.1	11440	PASS
442	198	50	100	89.2	72178	PASS
443	442	15	24	18.7	13493	PASS