
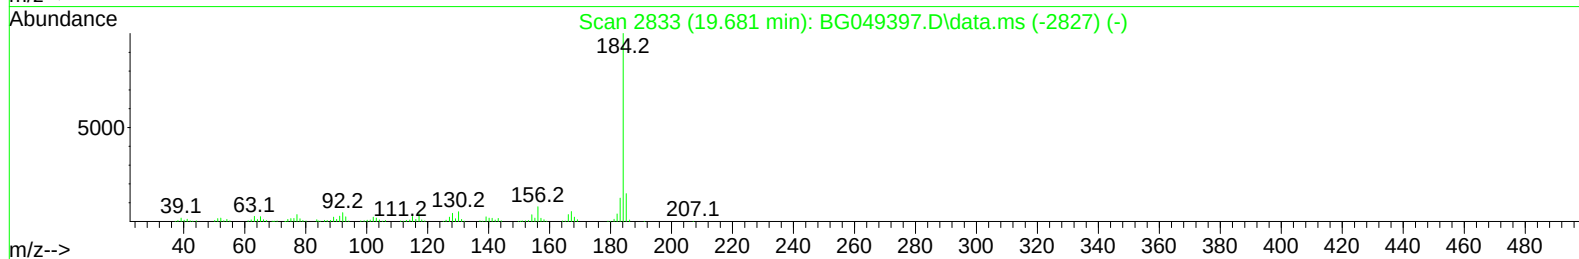
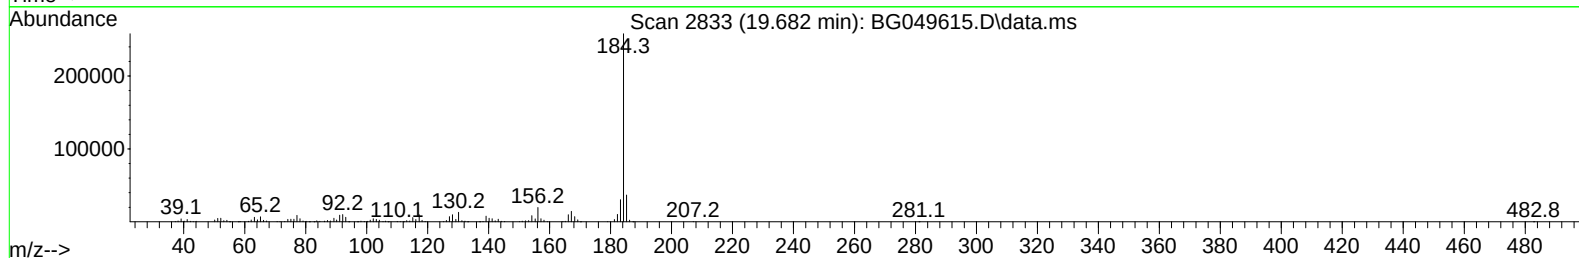


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080321\
Data File : BG049615.D
Acq On : 3 Aug 2021 8:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 11:39:33 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 11:30:48 2021
Response via : Initial Calibration

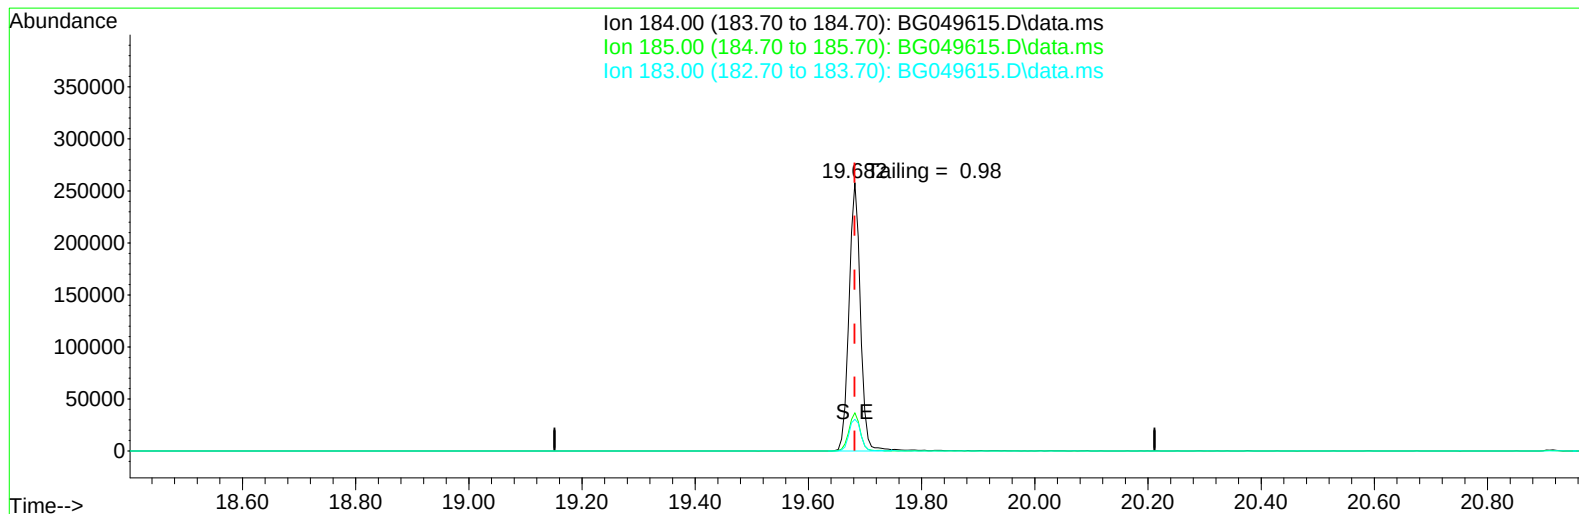

TIC: BG049615.D\data.ms

(77) Benzidine




19.682min (+ 0.001) 6567.26 ng

response 360069

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.25
183.00	11.70	11.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080321\
Data File : BG049615.D
Acq On : 3 Aug 2021 8:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 11:39:33 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 11:30:48 2021
Response via : Initial Calibration

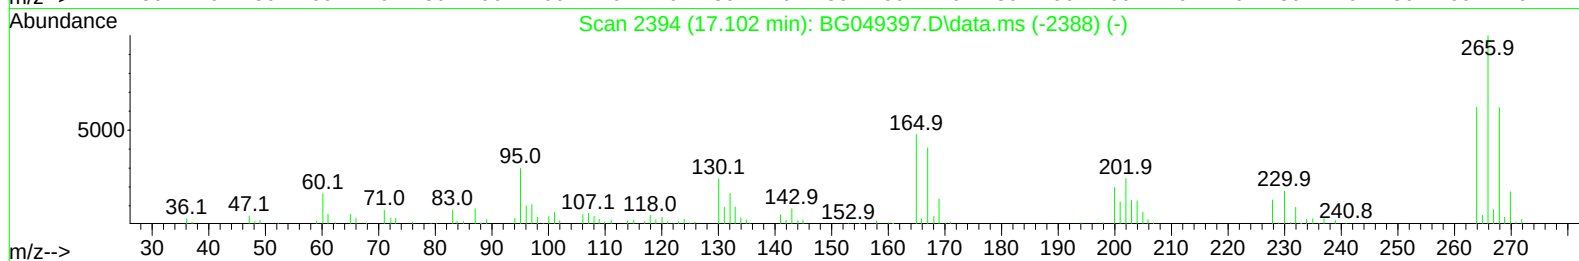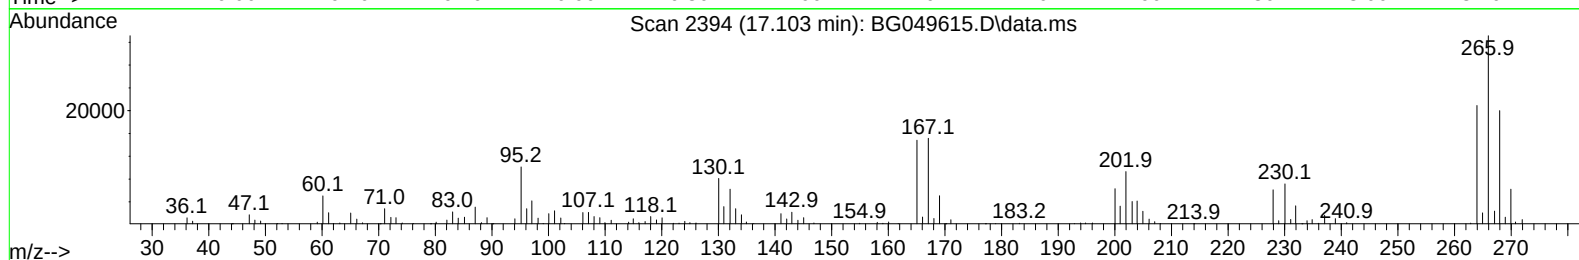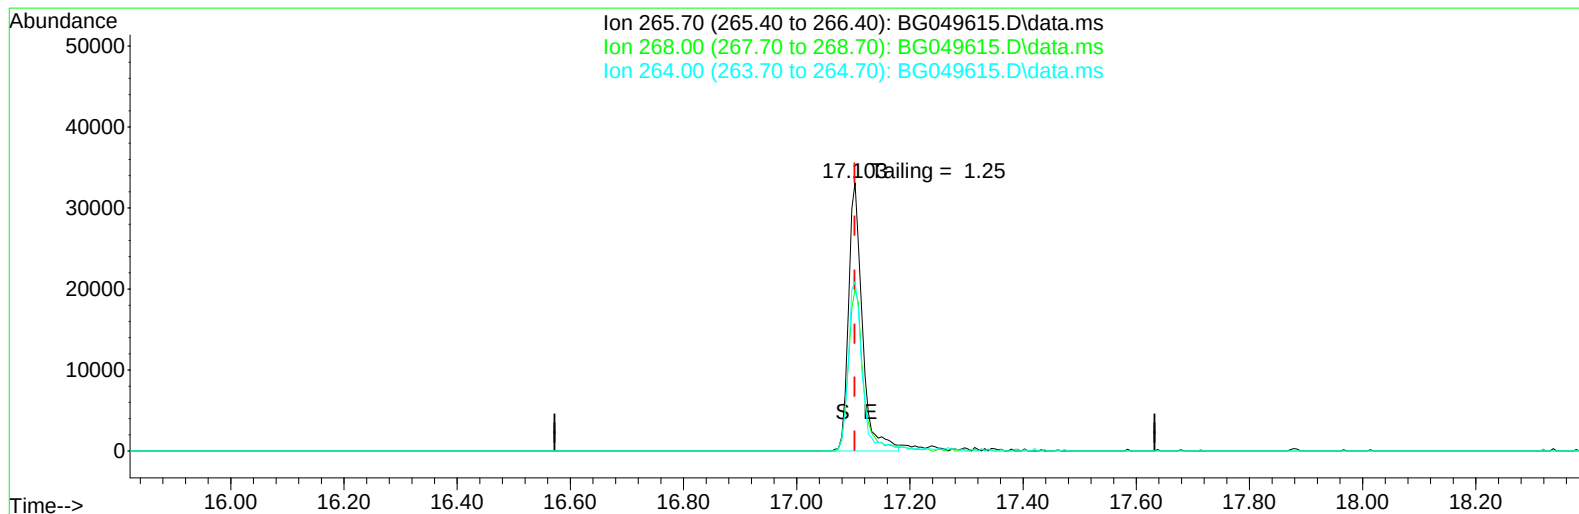

TIC: BG049615.D\data.ms

(70) Pentachlorophenol (C)

17.103min (+ 0.001) 0.00 ng

response 57919

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	60.36
264.00	61.30	63.04
0.00	0.00	0.00