
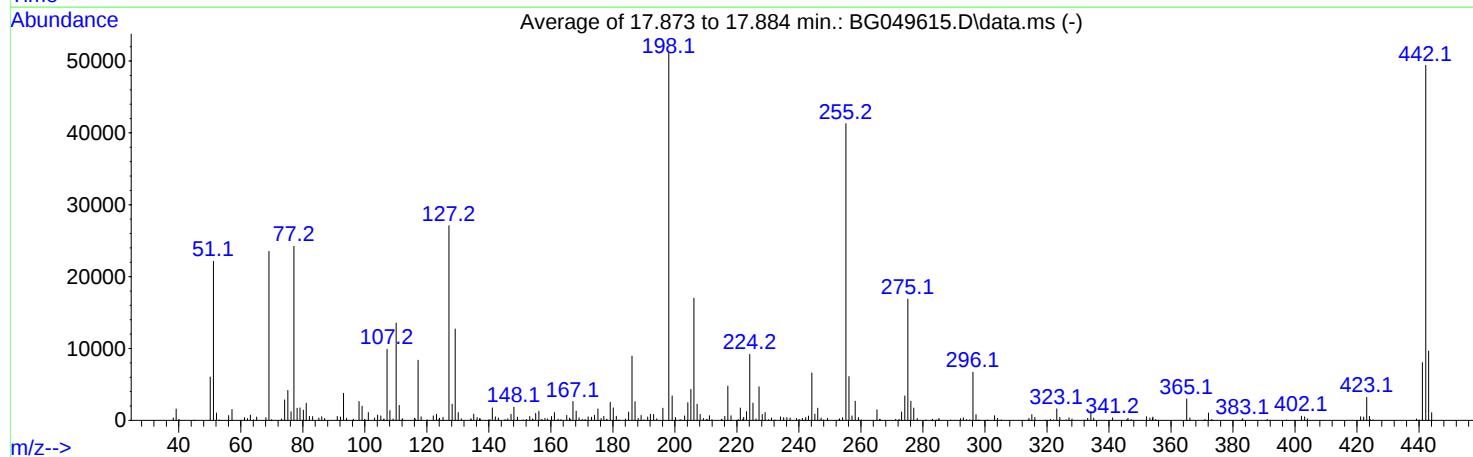


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080321\
 Data File : BG049615.D
 Acq On : 3 Aug 2021 8:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 03 15:15:33 2021

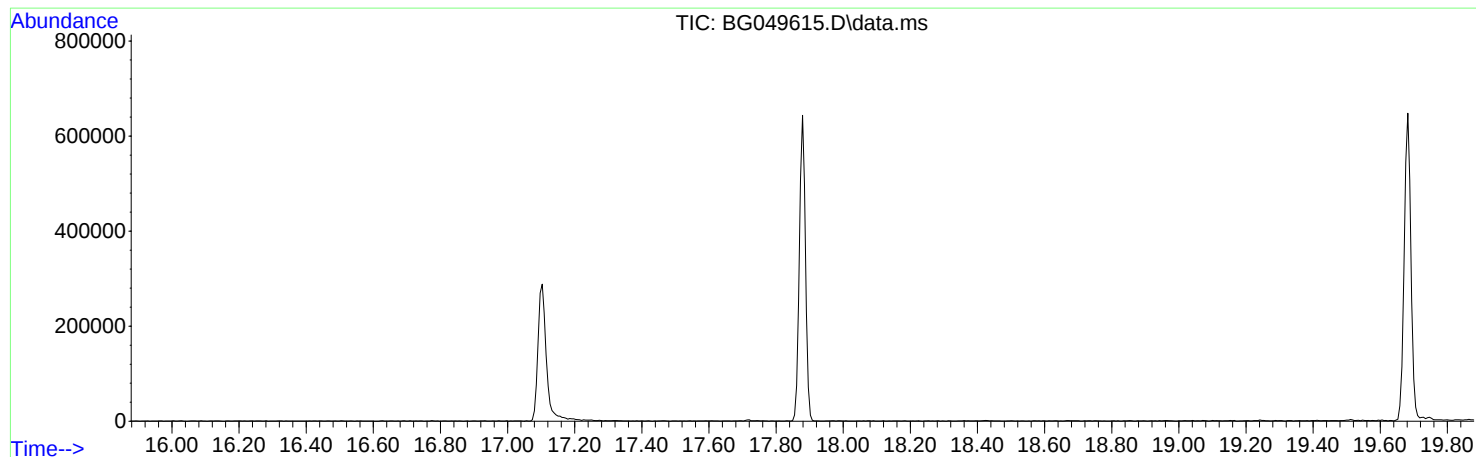




AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2519

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.2	22133	PASS
68	69	0.00	2	1.7	391	PASS
69	198	0.00	100	45.9	23517	PASS
70	69	0.00	2	0.5	116	PASS
127	198	10	80	53.0	27109	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51189	PASS
199	198	5	9	6.7	3417	PASS
275	198	10	60	33.0	16878	PASS
365	198	1	100	5.8	2983	PASS
441	198	0.01	100	15.7	8049	PASS
442	442	100	100	100.0	49403	PASS
443	442	15	24	19.5	9653	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080321\
Data File : BG049615.D
Acq On : 3 Aug 2021 8:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 03 11:39:33 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 11:30:48 2021
Response via : Initial Calibration

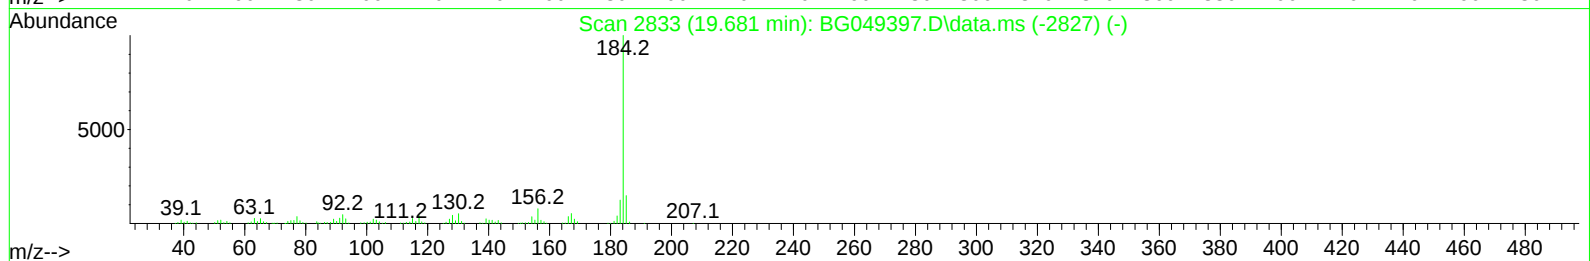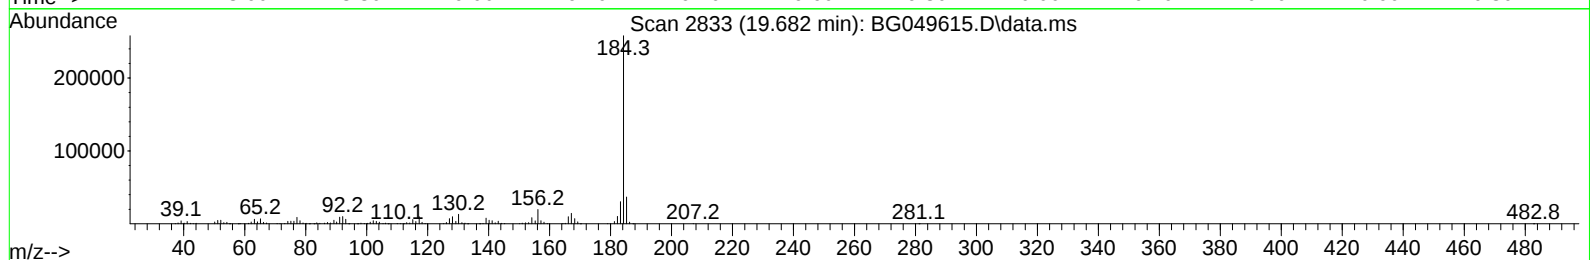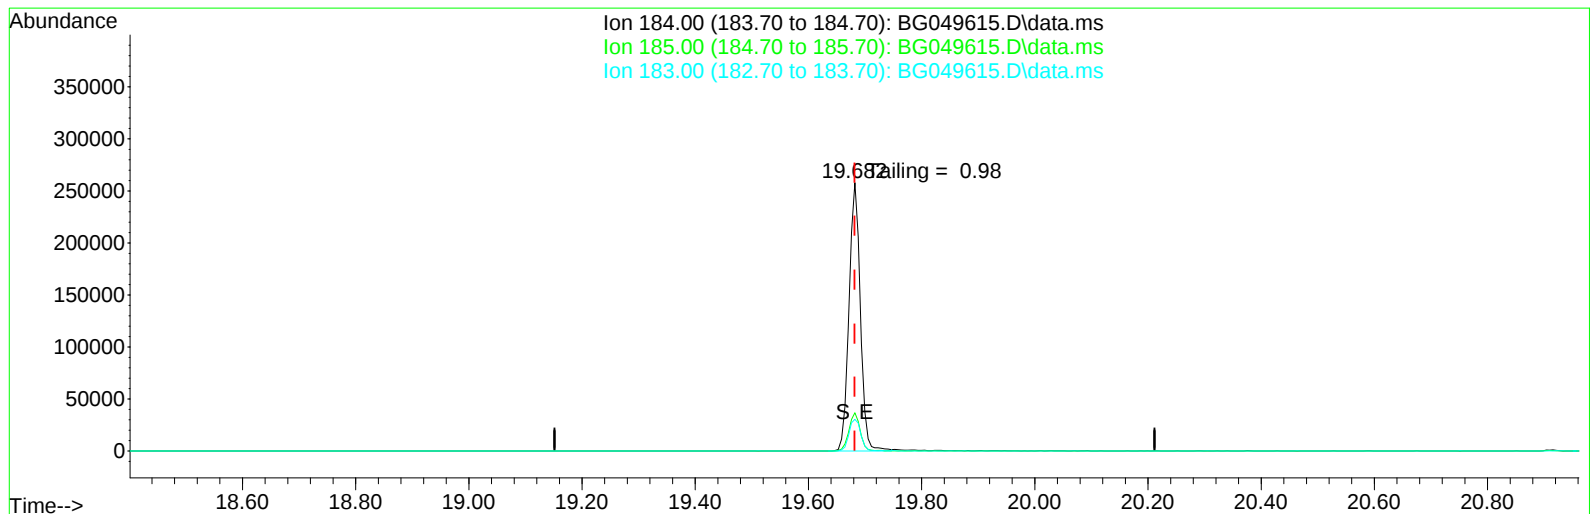

TIC: BG049615.D\data.ms

(77) Benzidine

19.682min (+ 0.001) 6567.26 ng




response 360069

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.25
183.00	11.70	11.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080321\
Data File : BG049615.D
Acq On : 3 Aug 2021 8:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 03 11:39:33 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG080321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 03 11:30:48 2021
Response via : Initial Calibration

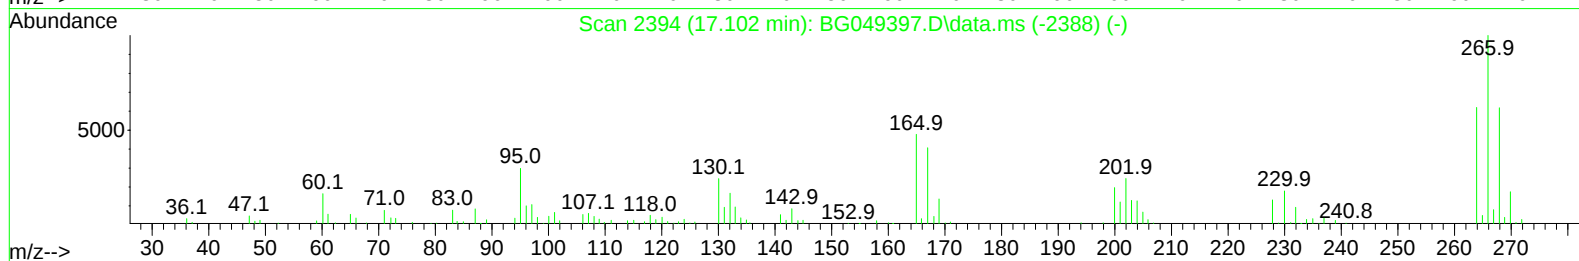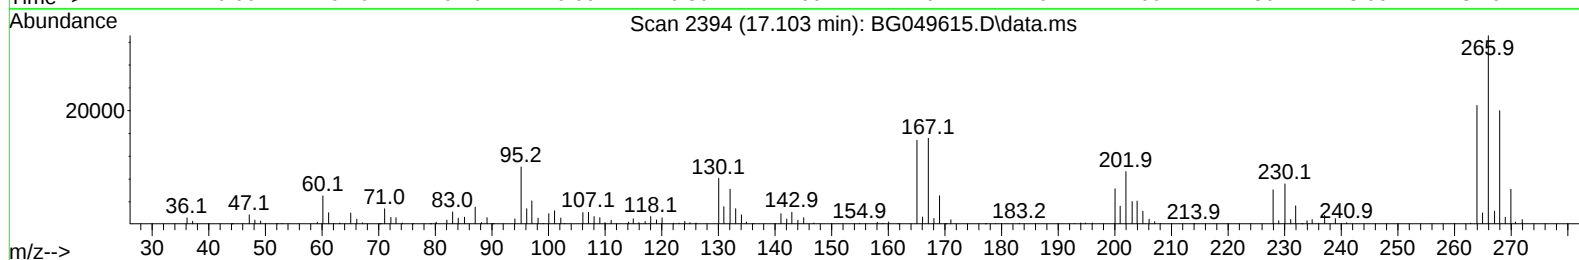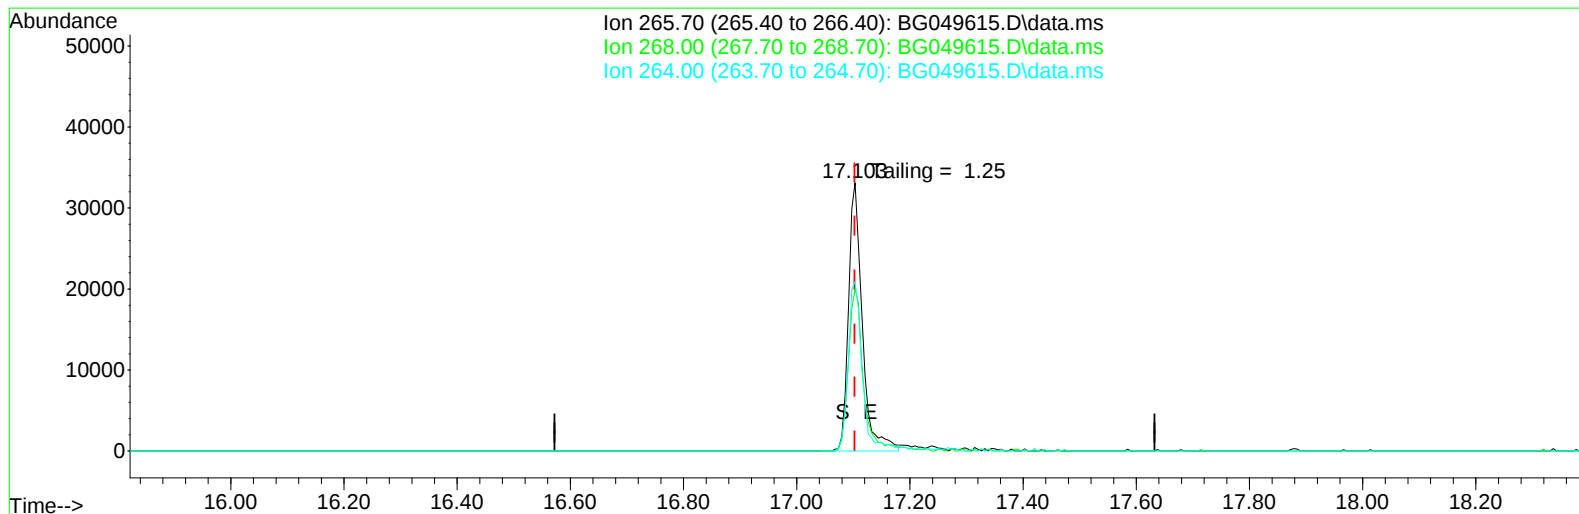

TIC: BG049615.D\data.ms

(70) Pentachlorophenol (C)

17.103min (+ 0.001) 0.00 ng

response 57919

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	60.36
264.00	61.30	63.04
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/3/2021	BNA_G	BG049615.D
Compound Name	Response	Retention Time
DDT	199159	20.91
DDD	1543	20.46
DDE	242	19.97
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1785	200944	0.89