
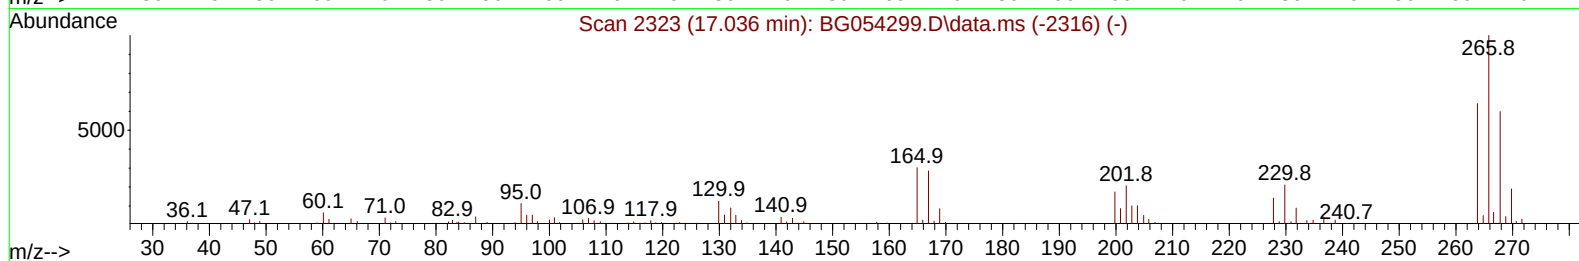
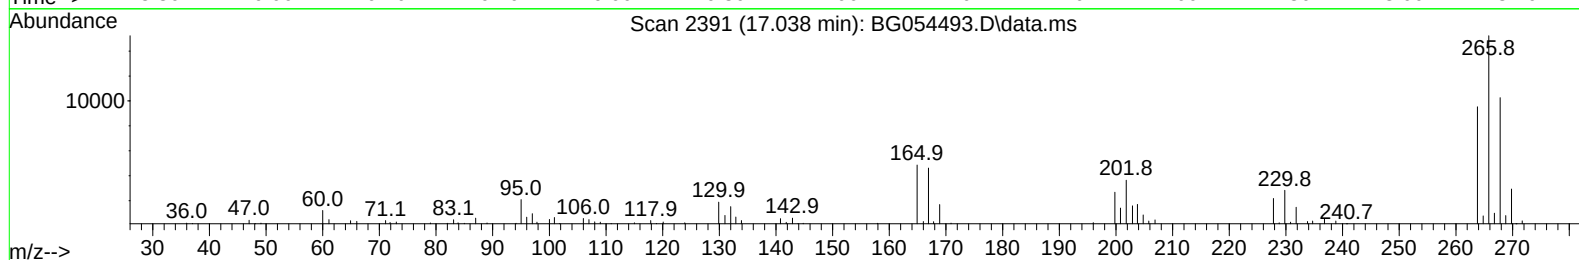


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080322\
Data File : BG054493.D
Acq On : 3 Aug 2022 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 04 04:39:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 04:30:50 2022
Response via : Initial Calibration

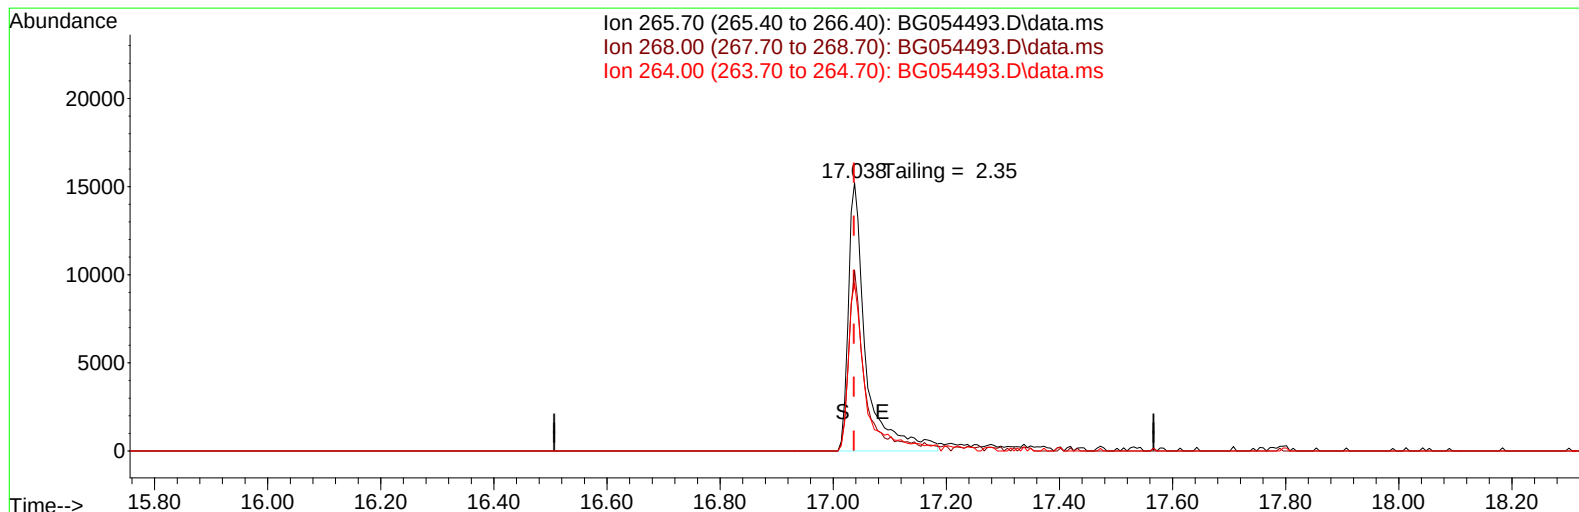

TIC: BG054493.D\data.ms

(70) Pentachlorophenol (C)




17.038min (+ 0.001) 19038.22 ng

response 32011

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	67.35
264.00	66.20	62.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080322\
Data File : BG054493.D
Acq On : 3 Aug 2022 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 04 04:39:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 04:30:50 2022
Response via : Initial Calibration

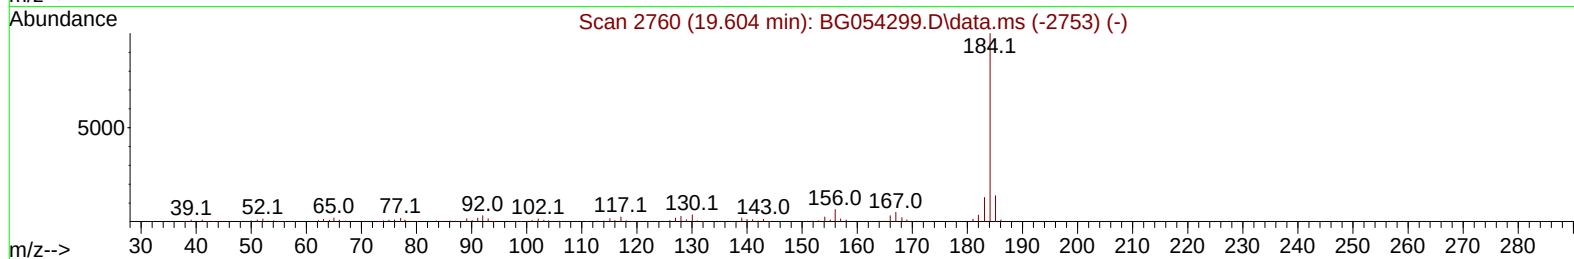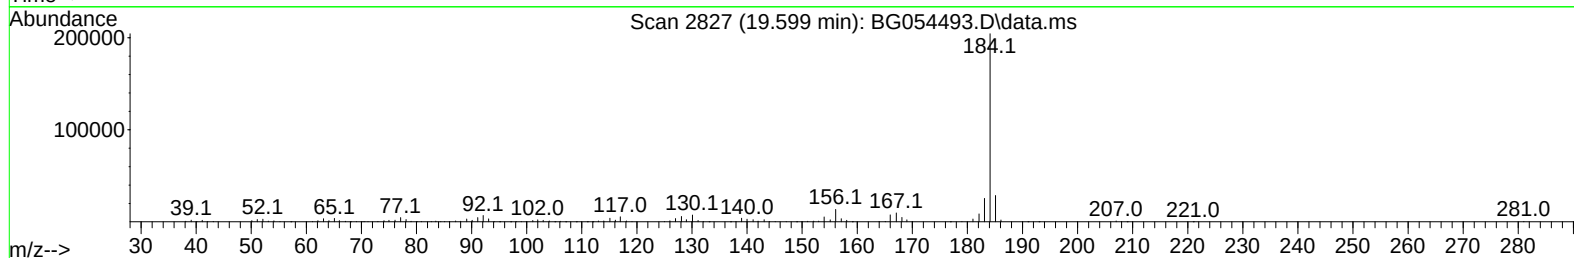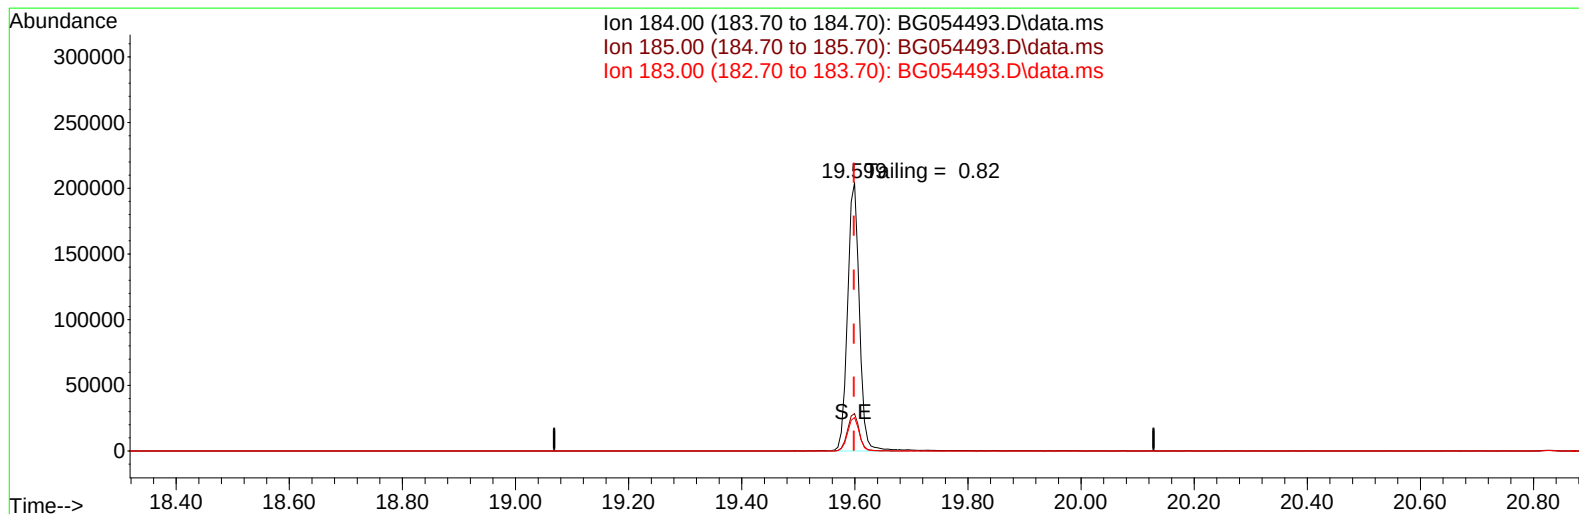

TIC: BG054493.D\data.ms

(77) Benzidine**19.599min (+ 0.001) 298778.70 ng****response 297611**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.98
183.00	11.10	12.50
0.00	0.00	0.00