


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080322\
 Data File : BG054493.D
 Acq On : 3 Aug 2022 10:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 28 04:30:50 2022

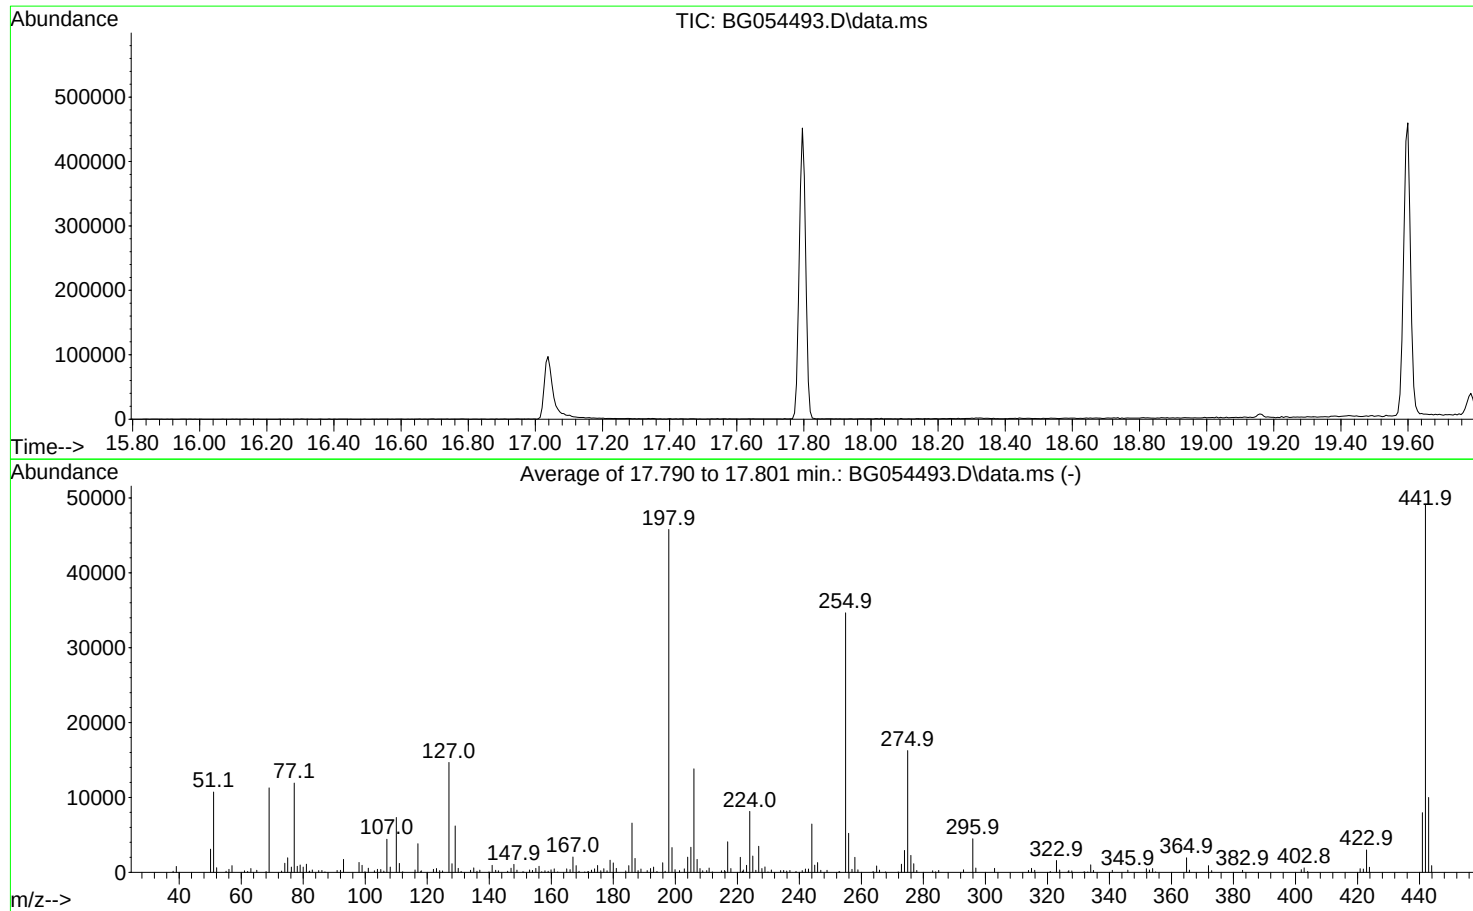




AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.4	10726	PASS
68	69	0.00	2	0.8	91	PASS
69	198	0.00	100	24.6	11278	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	32.0	14674	PASS
197	198	0.00	2	0.3	137	PASS
198	198	100	100	100.0	45789	PASS
199	198	5	9	7.2	3305	PASS
275	198	10	60	35.5	16257	PASS
365	198	1	100	4.2	1935	PASS
441	198	0.01	100	17.4	7954	PASS
442	442	50	100	100.0	49136	PASS
443	442	15	24	20.4	10003	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080322\
Data File : BG054493.D
Acq On : 3 Aug 2022 10:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 04 04:39:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 04:30:50 2022
Response via : Initial Calibration

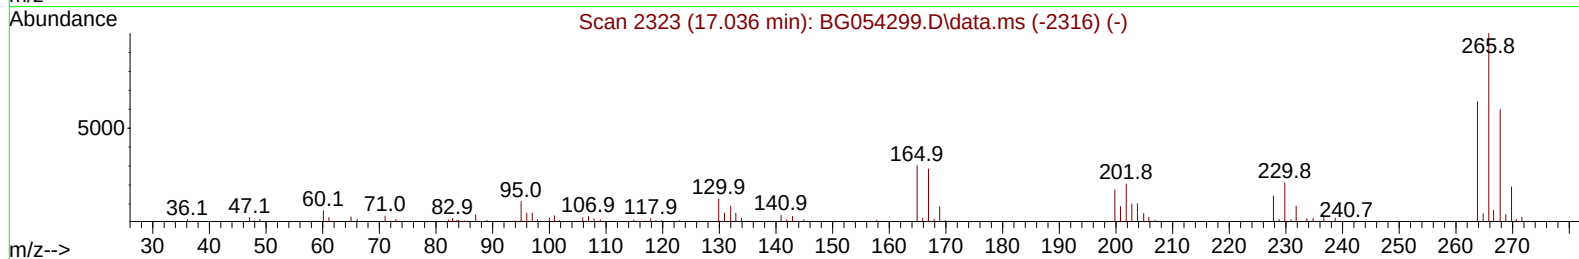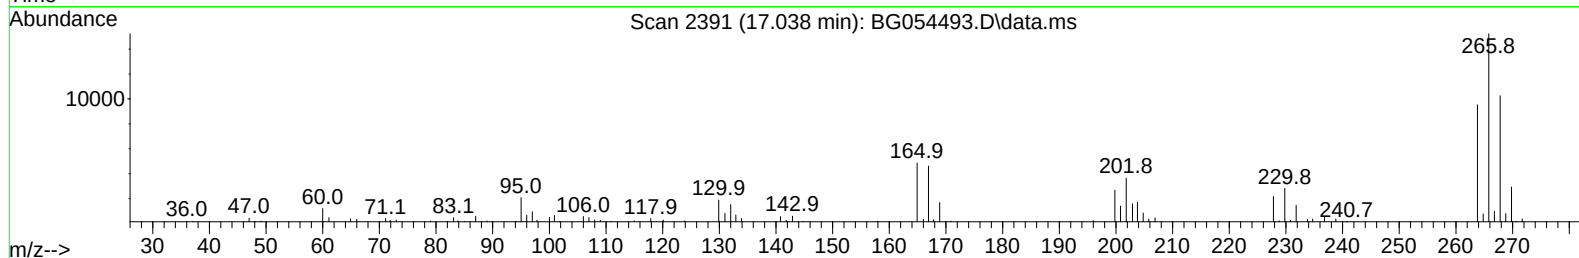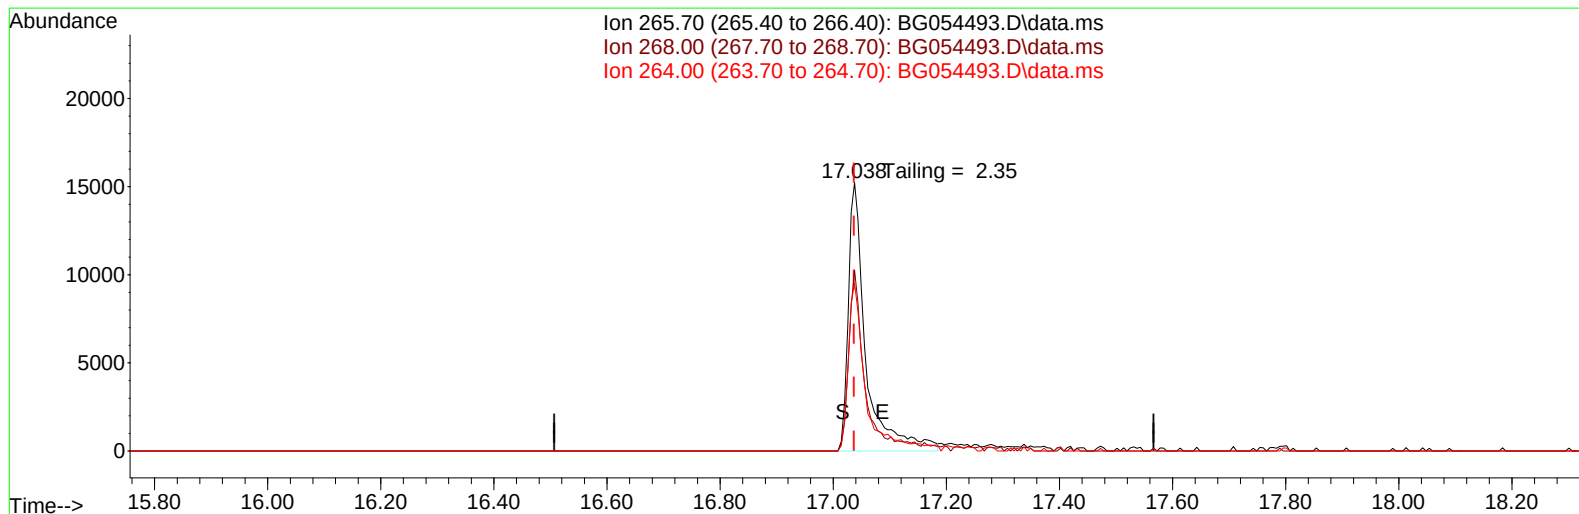

TIC: BG054493.D\data.ms

(70) Pentachlorophenol (C)

17.038min (+ 0.001) 19038.22 ng




response 32011

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	67.35
264.00	66.20	62.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080322\
 Data File : BG054493.D
 Acq On : 3 Aug 2022 10:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Aug 04 04:39:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG071522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 28 04:30:50 2022
 Response via : Initial Calibration

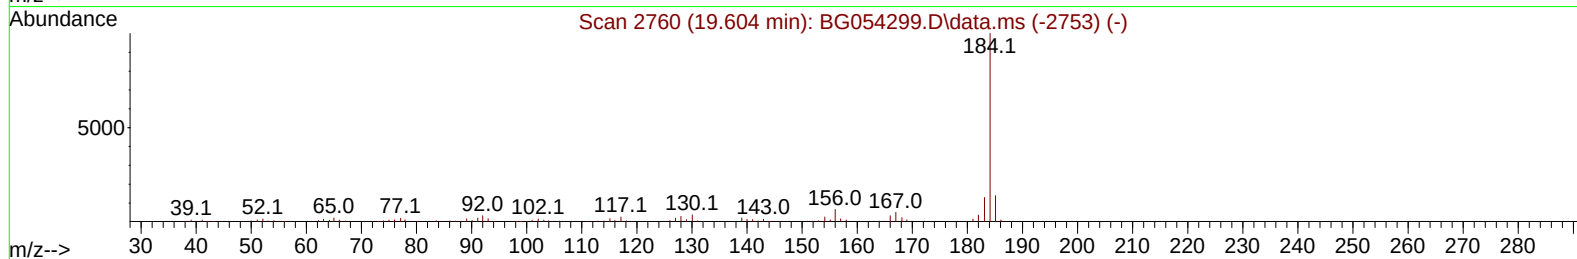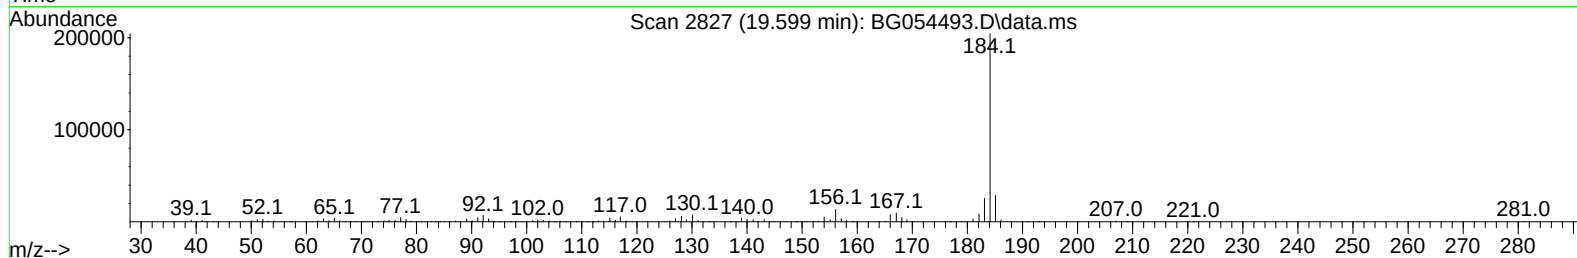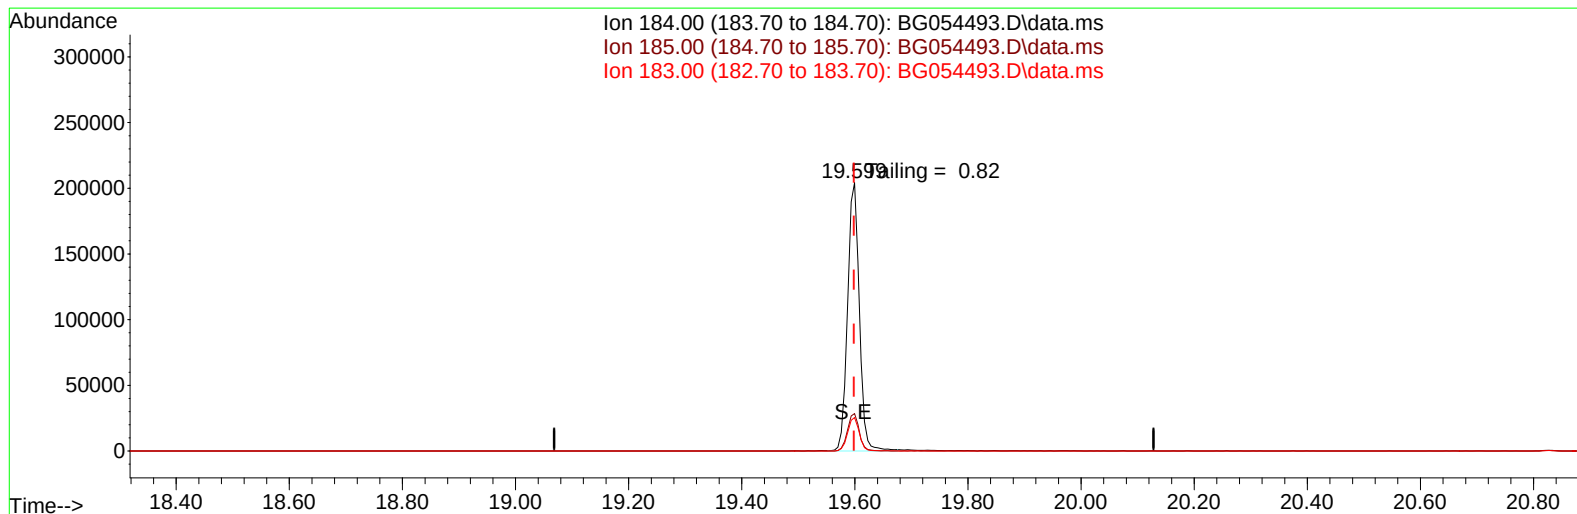

TIC: BG054493.D\data.ms

(77) Benzidine**19.599min (+ 0.001) 298778.70 ng****response 297611**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.98
183.00	11.10	12.50
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/3/2022	BNA_G	BG054493.D
Compound Name	Response	Retention Time
DDT	170233	20.827
DDD	5869	20.392
DDE	664	19.887
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6533	176766	3.70

Instrument :
BNA_G
ClientSampleId :
DFTPP