

Data Path : Z:\HPCHEM1\BNA G\DATA\BG080416\
 Data File : BG023457.D
 Acq On : 4 Aug 2016 18:27
 Operator : UM/SJ
 Sample : H4208-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDJJ1

Manual Integrations
 APPROVED

sohil
 8/5/2016 6:59:59 PM

Quant Time: Aug 05 03:15:00 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 05 02:31:20 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	85153	20.00	ng/ul	0.00
18) Naphthalene-d8	10.95	136	424693	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.78	164	349513	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.54	188	969530	20.00	ng/ul	0.00
75) Chrysene-d12	21.86	240	970189	20.00	ng/ul	0.00
83) Perylene-d12	25.23	264	959508	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.48	96	4325	2.16	ng/uL	0.00
5) Phenol-d5	7.27	99	166570	19.42	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.43	67	117380	21.36	ng/ul	0.00
9) 2-Chlorophenol-d4	7.65	132	118751	20.29	ng/ul	0.00
13) 4-Methylphenol-d8	8.83	113	132530	19.79	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	63986	19.11	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	69850	18.17	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.57	165	135850	18.73	ng/ul	0.00
29) 4-Chloroaniline-d4	11.09	131	177982	20.92	ng/ul	0.00
43) Dimethylphthalate-d6	14.17	166	595959	20.83	ng/ul	0.00
46) Acenaphthylene-d8	14.47	160	641920	19.93	ng/ul	0.00
51) 4-Nitrophenol-d4	15.00	143	54887m	11.24	ng/ul	0.01
57) Fluorene-d10	15.78	176	559128	21.15	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	66342	10.67	ng/ul	0.00
70) Anthracene-d10	17.64	188	959436	21.96	ng/ul	0.00
76) Pyrene-d10	19.93	212	1123744	22.88	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.00	264	972001	22.38	ng/ul	0.00

Target Compounds

						Ovalue
44) Dimethylphthalate	14.22	163	332714	11.74	ng/ul	98
89) Indeno(1,2,3-cd)pyrene	29.08	276	135118m	2.18	ng/ul	
90) Dibenzo(a,h)anthracene	29.17	278	114704m	2.17	ng/ul	
91) Benzo(a,h,i)perylene	30.29	276	152378	2.97	ng/ul#	78

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG080416\
Data File : BG023457.D
Acq On : 4 Aug 2016 18:27
Operator : UM/SJ
Sample : H4208-02
Misc :
ALS Vial : 4 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
BDJJ1

Manual Integrations
APPROVED

sohil
8/5/2016 6:59:59 PM

Quant Time: Aug 05 03:15:00 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 05 02:31:20 2016
Response via : Initial Calibration

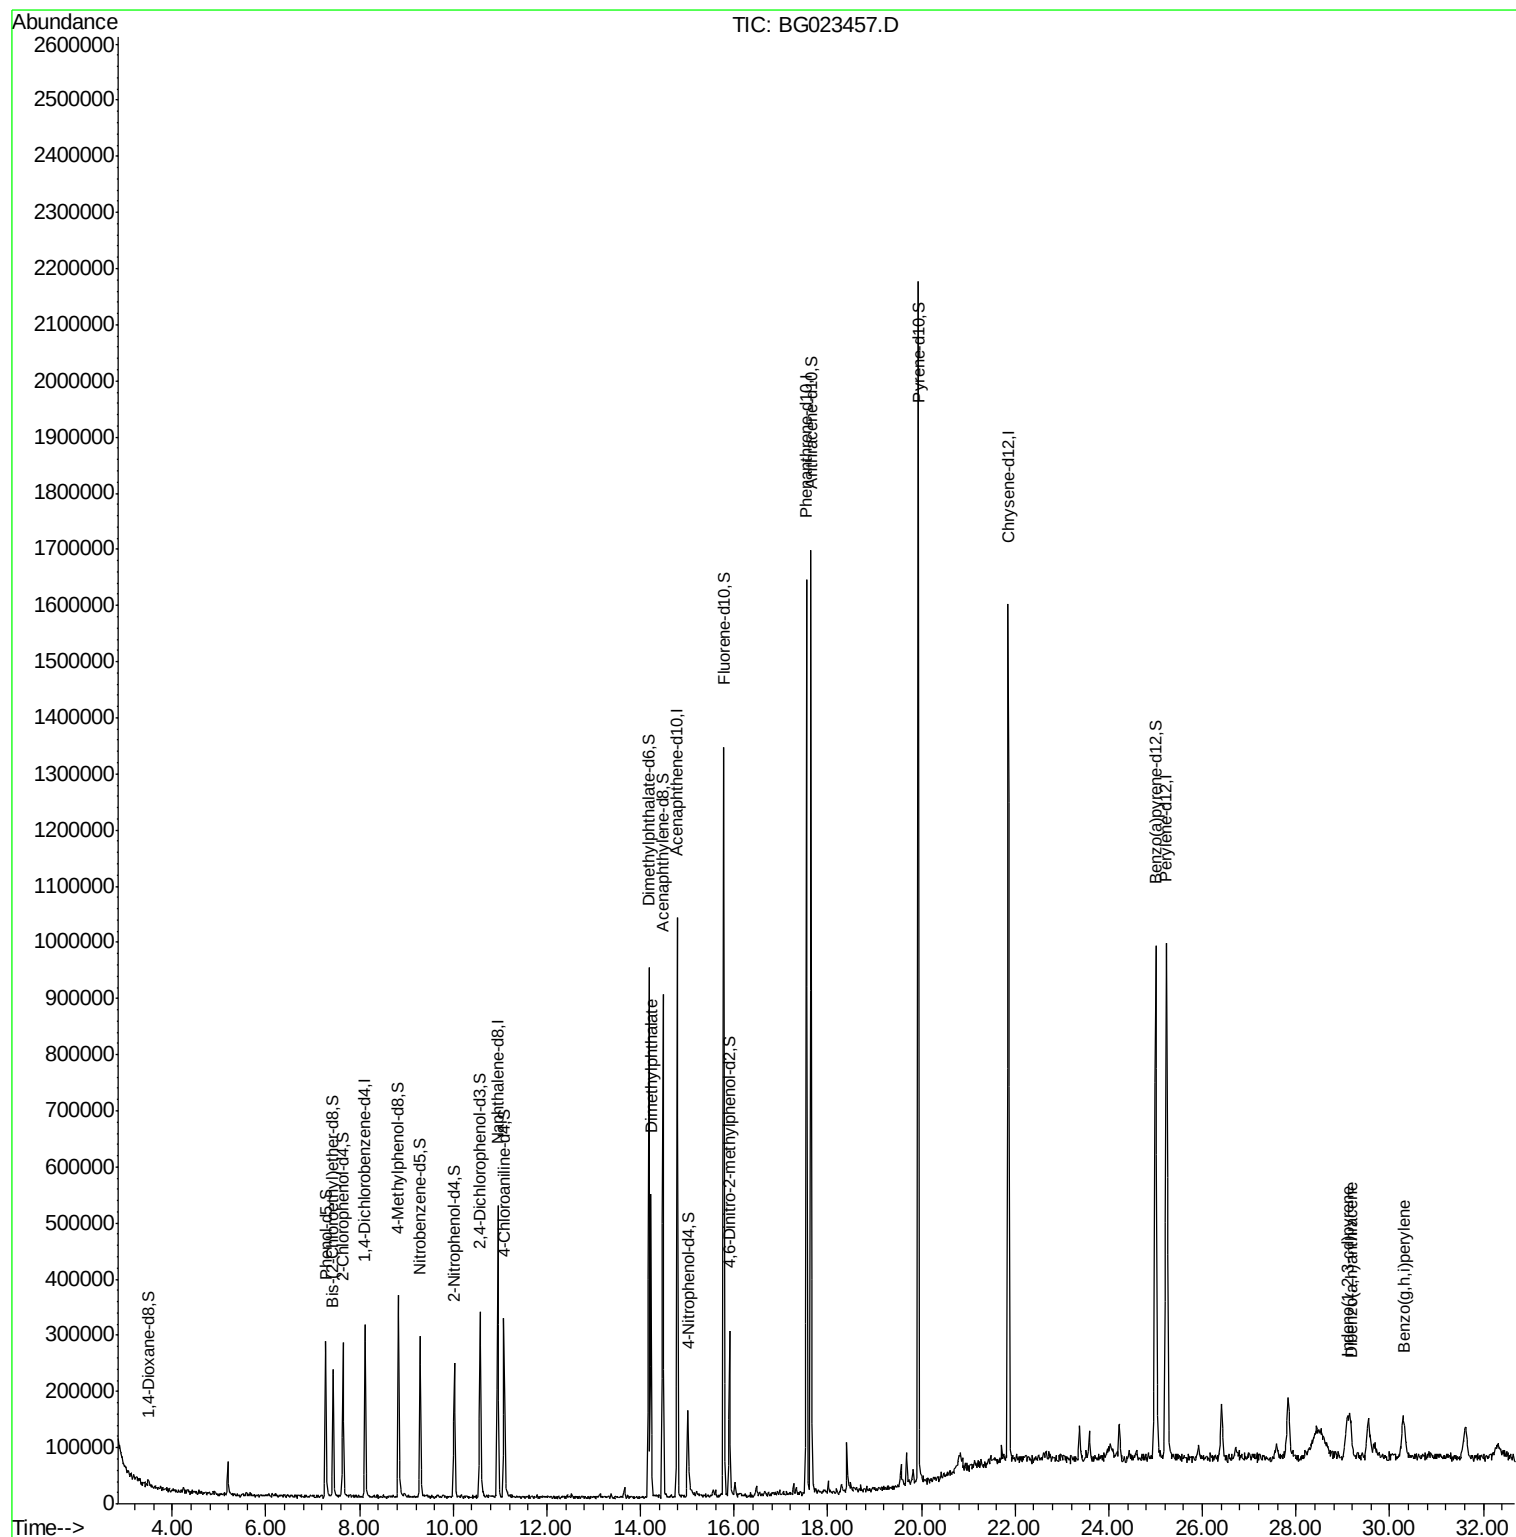

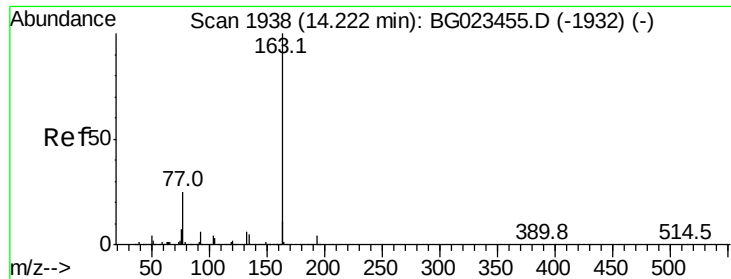





#44
Dimethylphthalate
Concen: 11.74 ng/ul
RT: 14.22 min Scan# 1938
Delta R.T. -0.00 min
Lab File: BG023457.D
Acq: 4 Aug 2016 18:27

Instrument :
BNA_G
ClientSampleId :
BDJJ1

Tot Ion	Ratio	Lower	Upper
163	100		
194	3.9	3.4	5.2
164	10.1	8.8	13.2




Manual Integrations
APPROVED


sohil
8/5/2016 6:59:59 PM

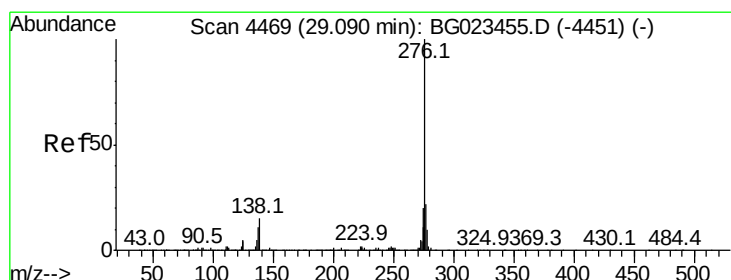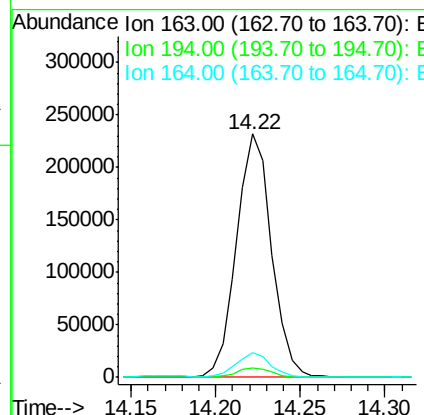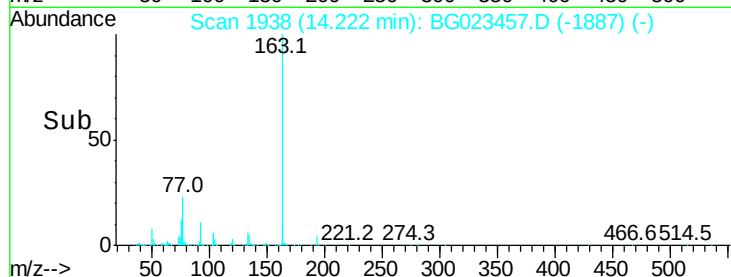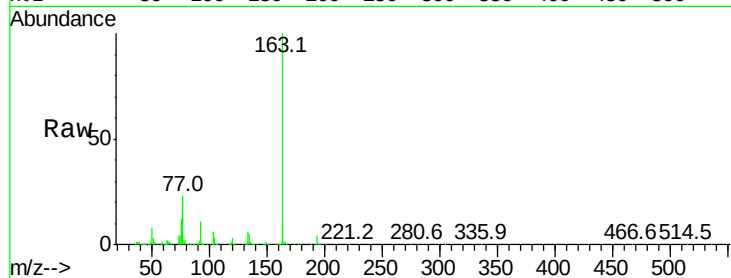

#89
Indeno(1,2,3-cd)pyrene
Concen: 2.18 ng/ul m
RT: 29.08 min Scan# 4468
Delta R.T. -0.01 min
Lab File: BG023457.D
Acq: 4 Aug 2016 18:27

Tgt Ion	Ratio	Lower	Upper
276	100		
138	11.9	20.8	31.2#
277	20.3	17.6	26.4

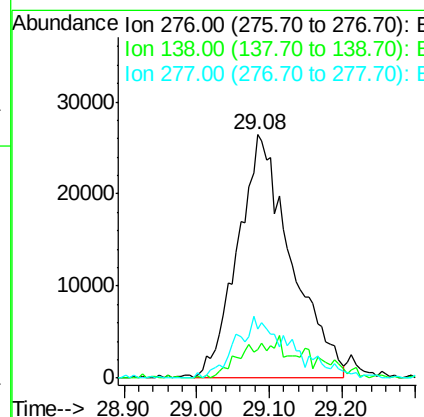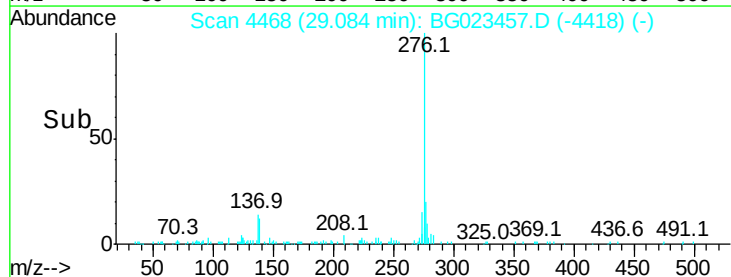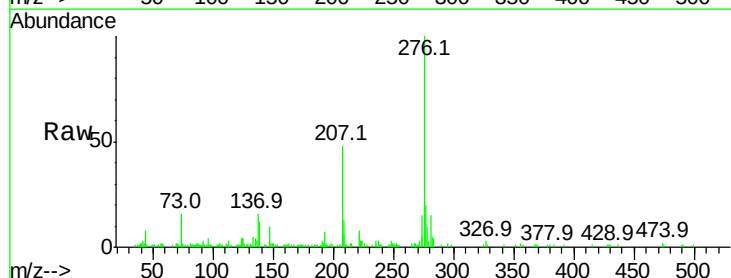

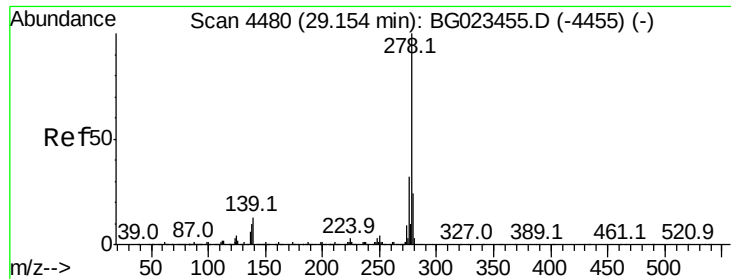

#90

Dibenzo(a,h)anthracene

Concen: 2.17 ng/ul m

RT: 29.17 min Scan# 4482

Delta R.T. 0.01 min

Lab File: BG023457.D

Acq: 4 Aug 2016 18:27

Instrument :

BNA_G


ClientSampleId :

BDJJ1




Tot Ion:	278	Resp:	114704
Ion Ratio	Lower	Upper	
278	100		
139	7.5	16.3	24.5#
279	23.8	19.1	28.7

Manual Integrations
APPROVED

sohil
8/5/2016 6:59:59 PM

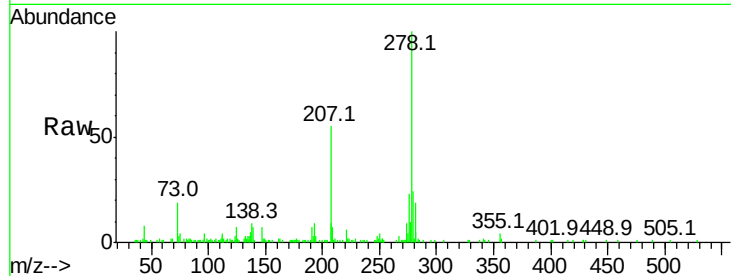

Abundance Ion 278.00 (277.70 to 278.70): E
Ion 139.00 (138.70 to 139.70): E
Ion 279.00 (278.70 to 279.70): E

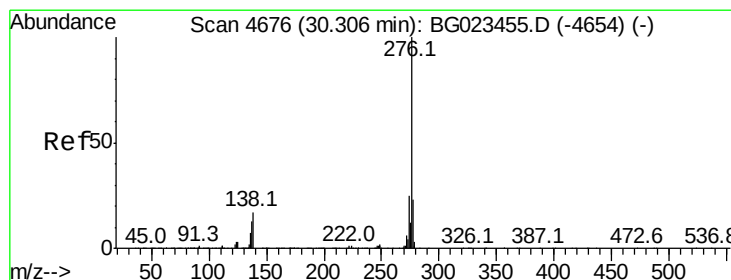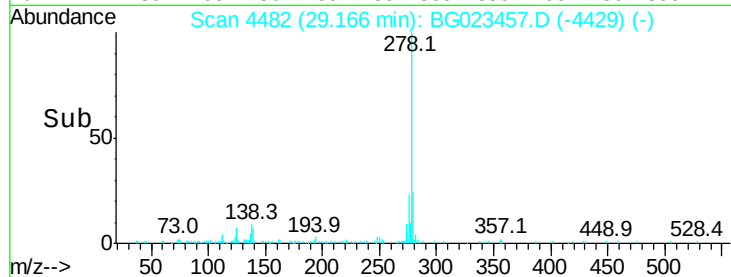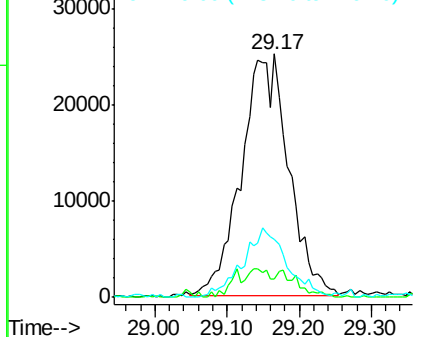

#91

Benzo(g,h,i)perylene

Concen: 2.97 ng/ul

RT: 30.29 min Scan# 4674

Delta R.T. -0.01 min

Lab File: BG023457.D

Acq: 4 Aug 2016 18:27

Tgt Ion:	276	Resp:	152378
Ion Ratio	Lower	Upper	
276	100		
138	9.9	22.1	33.1#
277	24.5	17.0	25.4

Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E

