

Data Path : Z:\HPCHEM1\BNA G\DATA\BG080416\
 Data File : BG023474.D
 Acq On : 5 Aug 2016 5:46
 Operator : UM/SJ
 Sample : H4208-18
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDJK7

Quant Time: Aug 05 06:48:55 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 05 03:48:01 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	142704	20.00	ng/ul	0.00
18) Naphthalene-d8	10.95	136	661905	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.78	164	492678	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.54	188	1191195	20.00	ng/ul	0.00
75) Chrysene-d12	21.86	240	1223932	20.00	ng/ul	0.00
83) Perylene-d12	25.23	264	1185660	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.49	96	5851	1.74	ng/uL	0.00
5) Phenol-d5	7.27	99	259970	18.08	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.43	67	192302	20.88	ng/ul	0.00
9) 2-Chlorophenol-d4	7.65	132	185365	18.90	ng/ul	0.00
13) 4-Methylphenol-d8	8.83	113	211212	18.82	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	105767	20.27	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	118249	19.73	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.57	165	212560	18.81	ng/ul	0.00
29) 4-Chloroaniline-d4	11.09	131	287908	21.71	ng/ul	0.00
43) Dimethylphthalate-d6	14.18	166	853794	21.17	ng/ul	0.00
46) Acenaphthylene-d8	14.48	160	935022	20.60	ng/ul	0.00
51) 4-Nitrophenol-d4	15.00	143	59883	8.70	ng/ul	0.01
57) Fluorene-d10	15.78	176	755398	20.27	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	71170	9.31	ng/ul	0.00
70) Anthracene-d10	17.64	188	1189088	22.16	ng/ul	0.00
76) Pyrene-d10	19.93	212	1358058	21.92	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.00	264	1195448	22.27	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.23	163	554136	13.87	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG080416\
Data File : BG023474.D
Acq On : 5 Aug 2016 5:46
Operator : UM/SJ
Sample : H4208-18
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDJK7

Quant Time: Aug 05 06:48:55 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 05 03:48:01 2016
Response via : Initial Calibration

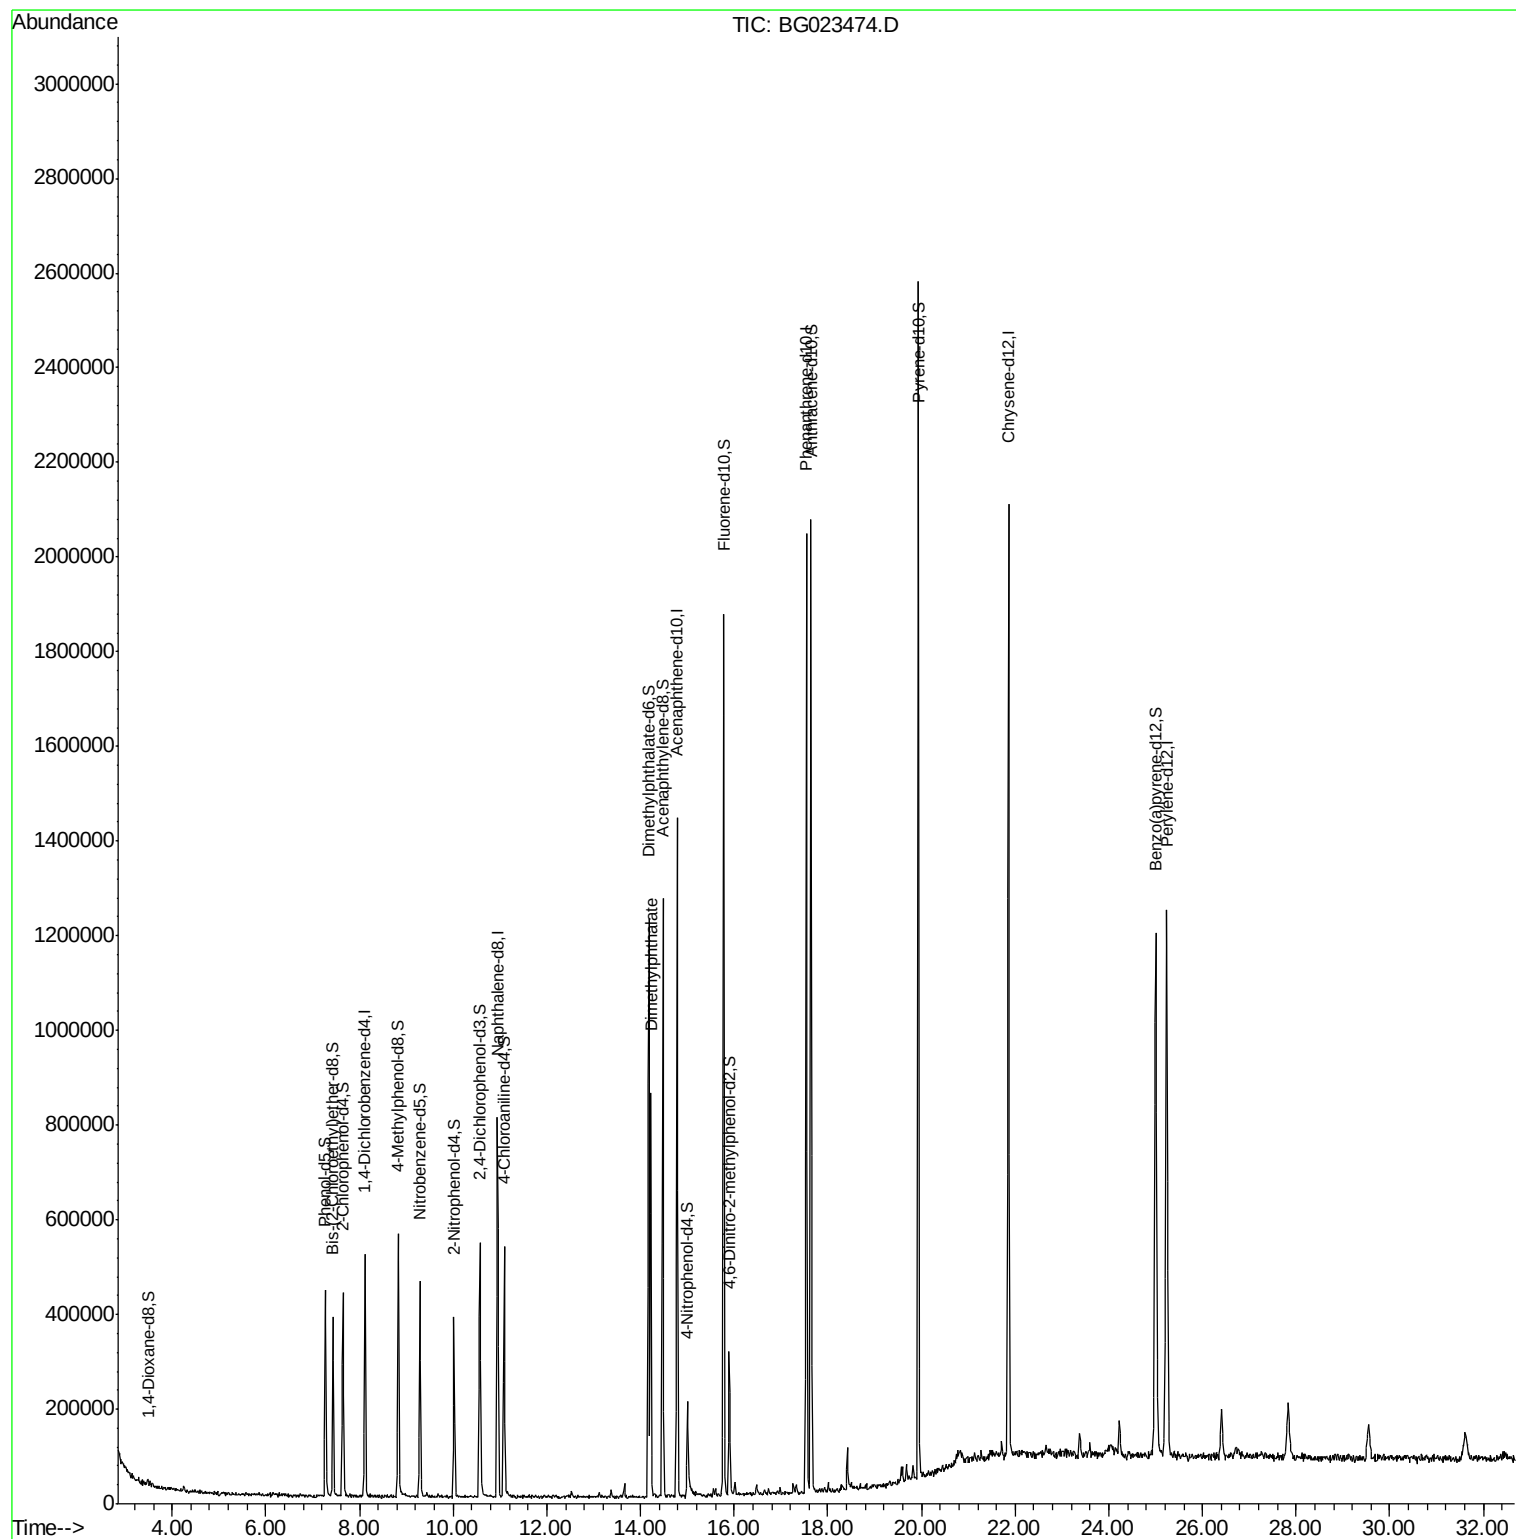

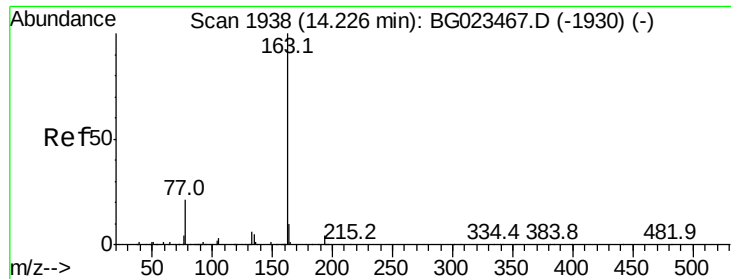

#44

Dimethylphthalate

Concen: 13.87 ng/ul

RT: 14.23 min Scan# 1938

Delta R.T. -0.00 min

Lab File: BG023474.D

Acq: 5 Aug 2016 5:46

Instrument :

BNA_G

ClientSampleId :

BDJK7

Tot Ion:163 Resp: 554136

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.2

164 10.3 8.8 13.2

