
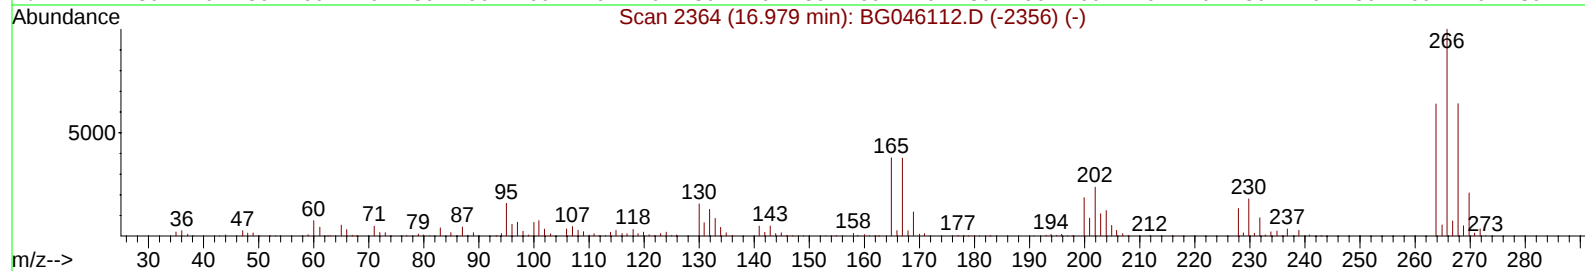
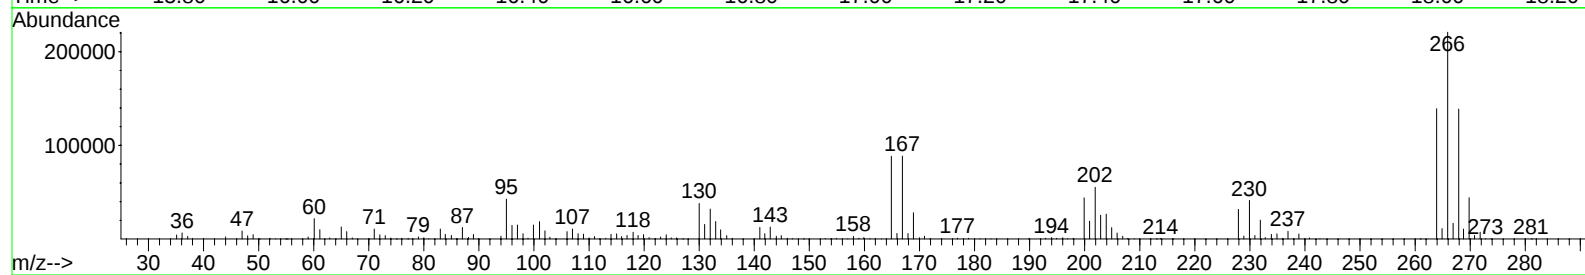


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080420\  
Data File : BG046161.D  
Acq On : 4 Aug 2020 7:59  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 04 18:14:52 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG073020.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jul 30 18:43:49 2020  
Response via : Initial Calibration

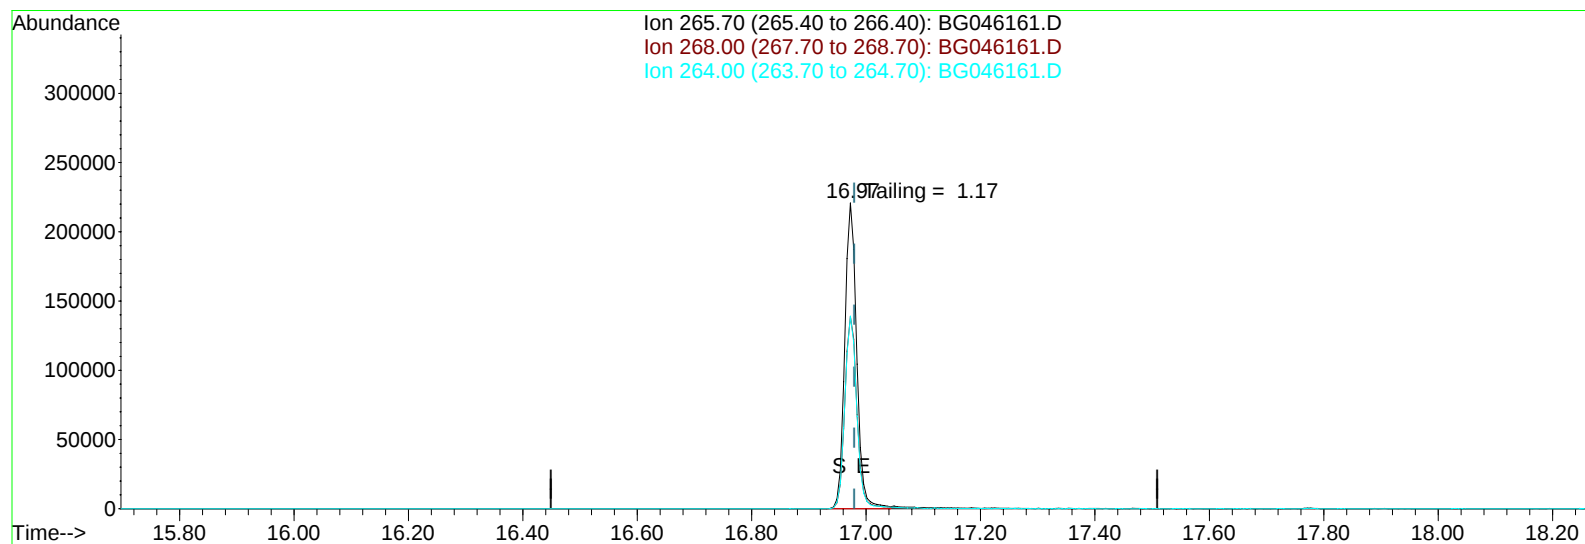

TIC: BG046161.D

(70) Pentachlorophenol (C)




16.972min (-0.007) 67927.90ng

response 325429

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 64.00 | 62.84 |
| 264.00 | 63.90 | 63.01 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080420\  
 Data File : BG046161.D  
 Acq On : 4 Aug 2020 7:59  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 04 18:14:52 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG073020.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Thu Jul 30 18:43:49 2020  
 Response via : Initial Calibration

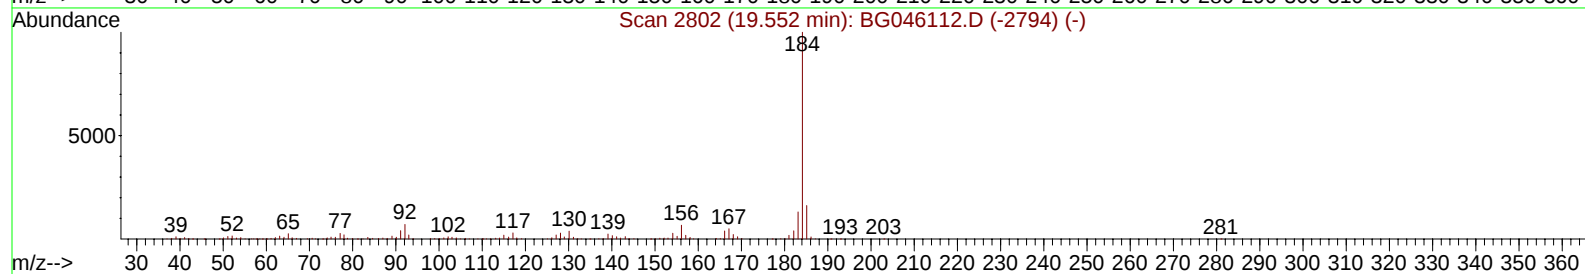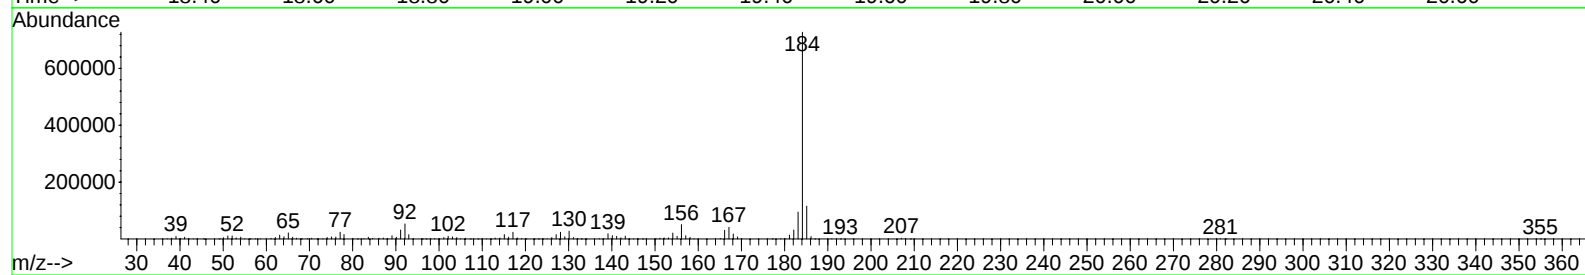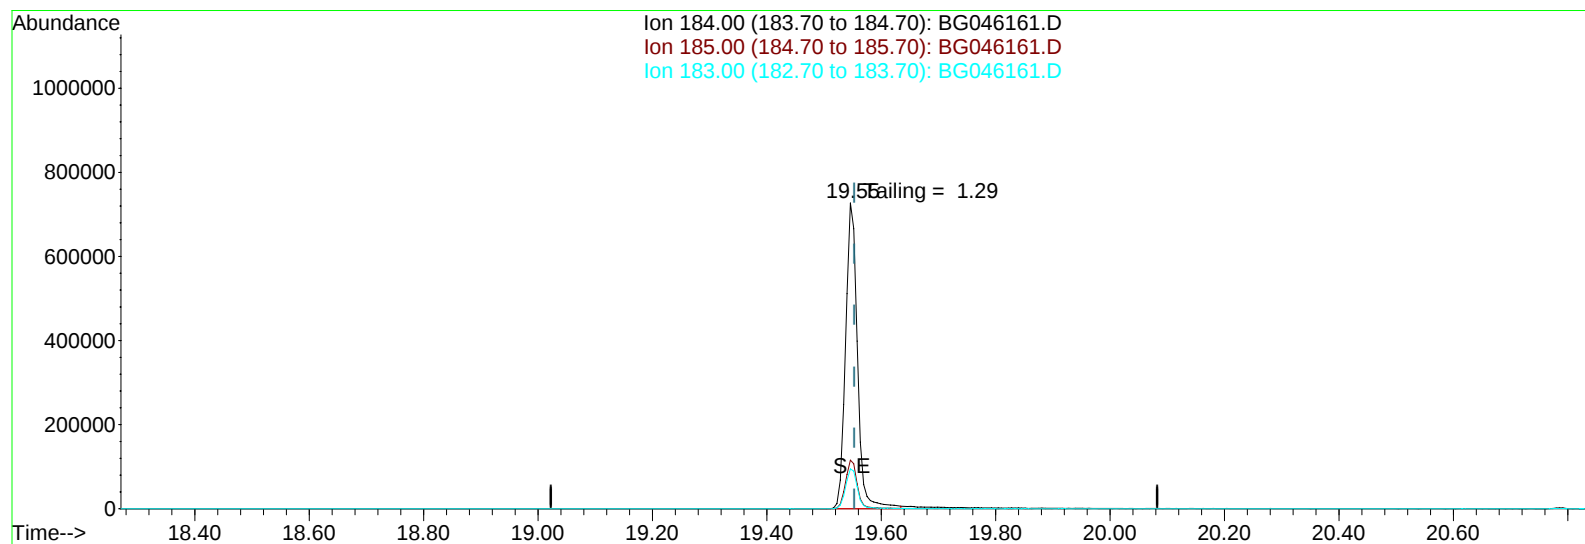

TIC: BG046161.D

(77) Benzidine

19.546min (-0.007) 42131.78ng

response 1070489

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 16.20 | 15.92 |
| 183.00 | 13.10 | 13.04 |
| 0.00   | 0.00  | 0.00  |