

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080420\  
 Data File : BG046165.D  
 Acq On : 4 Aug 2020 10:40  
 Operator : CG/JU  
 Sample : L3525-01  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 TILCON-FL-002

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON  
 Sampling : 1  
 Start Thrs: 0.2  
 Stop Thrs : 0  
 Filtering: 5  
 Min Area: 3 % of largest Peak  
 Max Peaks: 100  
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG073020.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.159       | 8             | 12          | 29           | rVB      | 328385         | 541478        | 10.16%          | 2.079%        |
| 2         | 5.068       | 331           | 337         | 345          | rBV      | 153305         | 232083        | 4.35%           | 0.891%        |
| 3         | 5.532       | 410           | 416         | 431          | rBV      | 1004345        | 1647033       | 30.90%          | 6.324%        |
| 4         | 7.119       | 678           | 686         | 701          | rBV      | 1055175        | 1831491       | 34.37%          | 7.032%        |
| 5         | 7.953       | 820           | 828         | 837          | rBV      | 364739         | 603537        | 11.32%          | 2.317%        |
| 6         | 9.105       | 1015          | 1024        | 1036         | rBV      | 726933         | 1313397       | 24.64%          | 5.043%        |
| 7         | 10.750      | 1296          | 1304        | 1316         | rBV      | 482700         | 880194        | 16.52%          | 3.379%        |
| 8         | 13.200      | 1714          | 1721        | 1733         | rBV      | 2075488        | 3231143       | 60.63%          | 12.406%       |
| 9         | 14.028      | 1856          | 1862        | 1870         | rBV      | 239006         | 337304        | 6.33%           | 1.295%        |
| 10        | 14.575      | 1948          | 1955        | 1963         | rBV      | 793099         | 1260009       | 23.64%          | 4.838%        |
| 11        | 16.061      | 2201          | 2208        | 2230         | rBV      | 1563447        | 2280015       | 42.78%          | 8.754%        |
| 12        | 17.319      | 2415          | 2422        | 2433         | rBV      | 1029514        | 1563881       | 29.34%          | 6.004%        |
| 13        | 19.933      | 2861          | 2867        | 2875         | rBV      | 4016472        | 5329347       | 100.00%         | 20.461%       |
| 14        | 21.238      | 3083          | 3089        | 3100         | rBV      | 586027         | 810709        | 15.21%          | 3.113%        |
| 15        | 21.567      | 3138          | 3145        | 3153         | rBV      | 1128692        | 1841469       | 34.55%          | 7.070%        |
| 16        | 22.389      | 3279          | 3285        | 3292         | rBV7     | 50426          | 103860        | 1.95%           | 0.399%        |
| 17        | 23.235      | 3425          | 3429        | 3438         | rVB3     | 36196          | 64821         | 1.22%           | 0.249%        |
| 18        | 24.675      | 3663          | 3674        | 3684         | rBV2     | 687862         | 1901226       | 35.67%          | 7.300%        |
| 19        | 25.944      | 3883          | 3890        | 3900         | rBV5     | 90331          | 272771        | 5.12%           | 1.047%        |


Sum of corrected areas: 26045768

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080420\  
Data File : BG046165.D  
Acq On : 4 Aug 2020 10:40  
Operator : CG/JU  
Sample : L3525-01  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
TILCON-FL-002

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG073020.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

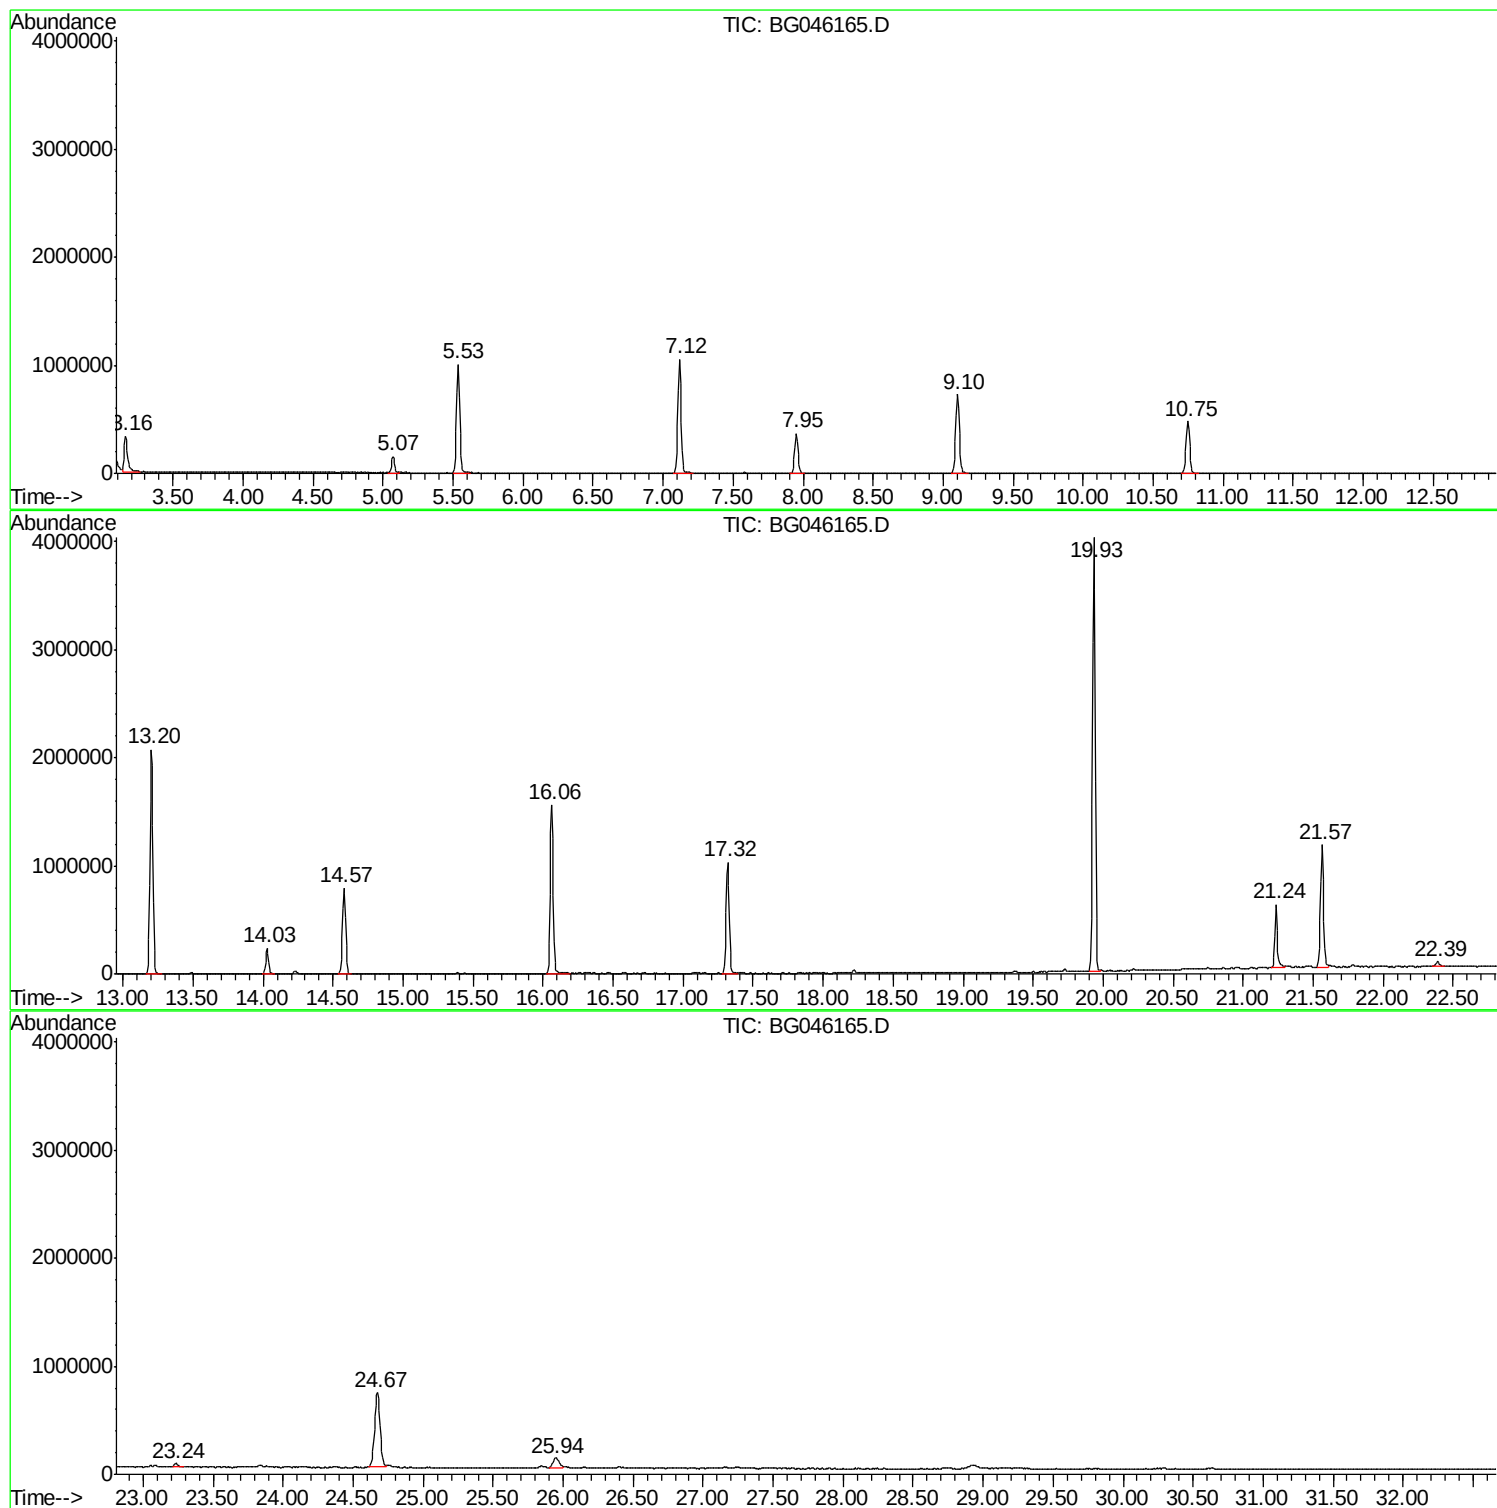

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG080420\  
Data File : BG046165.D  
Acq On : 4 Aug 2020 10:40  
Operator : CG/JU  
Sample : L3525-01  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
TILCON-FL-002

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG073020.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG080420\  
Data File : BG046165.D  
Acq On : 4 Aug 2020 10:40  
Operator : CG/JU  
Sample : L3525-01  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
TILCON-FL-002

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG073020.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | ---Internal Standard--- |
|------------------|----|---------|-------|----------|-------------------------|
|                  |    |         |       |          | # RT Resp Conc          |