


Data Path : Z:\HPCHEM1\BNA G\DATA\BG080516\
Data File : BG023478.D
Acq On : 5 Aug 2016 8:26
Operator : UM/SJ
Sample : DFTPP02
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Title : SVOA CALIBRATION
Last Update : Mon Aug 30 02:24:23 2004

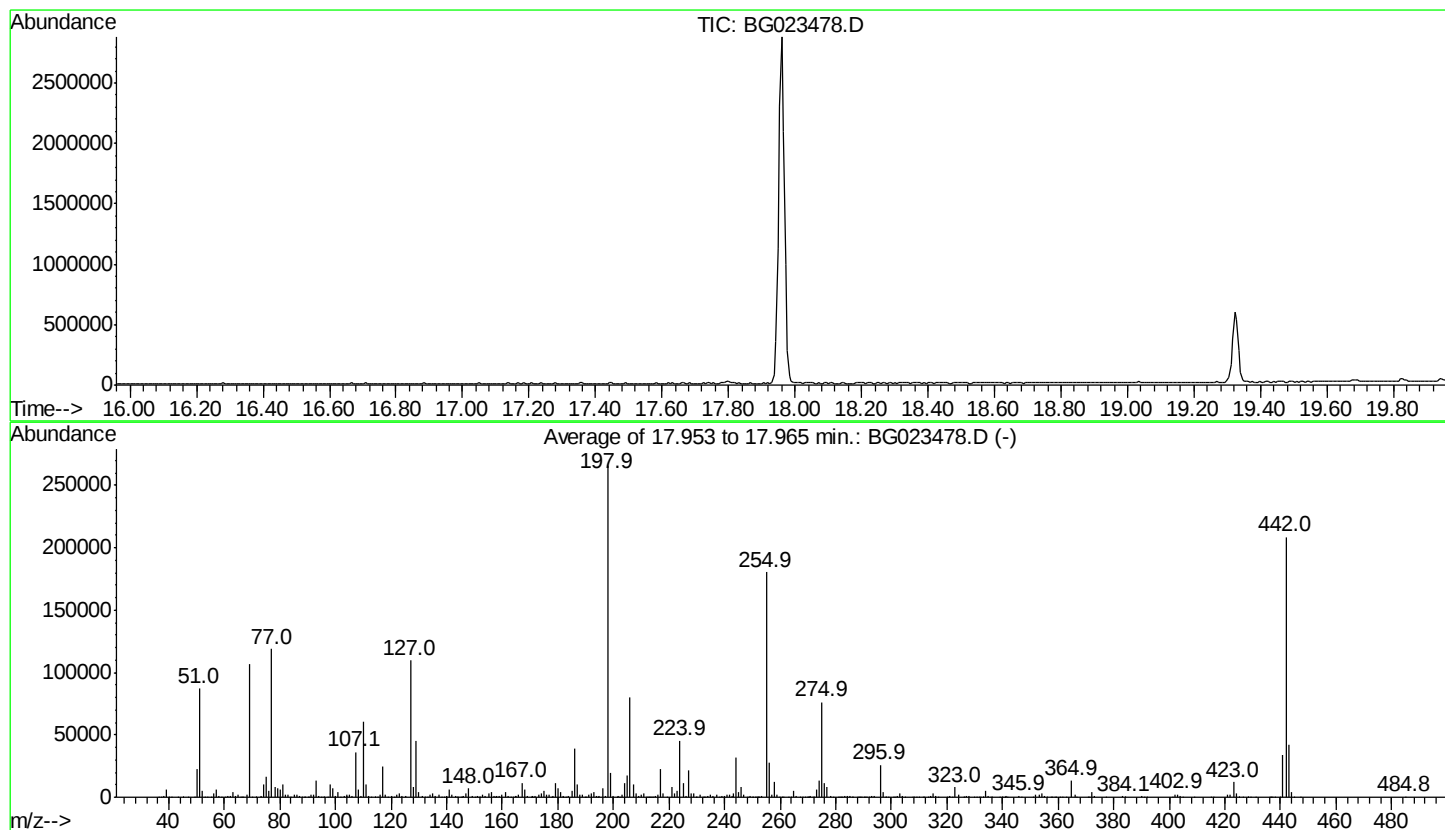

AutoFind: Scans 2573, 2574, 2575; Background Corrected with Scan 2567

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	87036	PASS
68	69	0.00	2	1.5	1634	PASS
69	198	0.00	100	40.3	107066	PASS
70	69	0.00	2	0.3	357	PASS
127	198	10	80	41.3	109810	PASS
197	198	0.00	2	0.5	1331	PASS
198	198	100	100	100.0	265898	PASS
199	198	5	9	7.3	19290	PASS
275	198	10	60	28.7	76306	PASS
365	198	1	100	4.9	13059	PASS
441	442	0.01	100	16.5	34312	PASS
442	198	50	100	78.4	208512	PASS
443	442	15	24	20.1	41826	PASS