

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA G\Data\BG080516\
 Data File : BG023485.D
 Acq On : 5 Aug 2016 13:08
 Operator : UM/SJ
 Sample : H4209-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampled :
 BDJH7

Manual Integrations
 APPROVED

sohil
 8/8/2016 6:56:00 PM

Quant Time: Aug 06 00:21:57 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 30 02:24:23 2004
 Response via : Initial Calibration

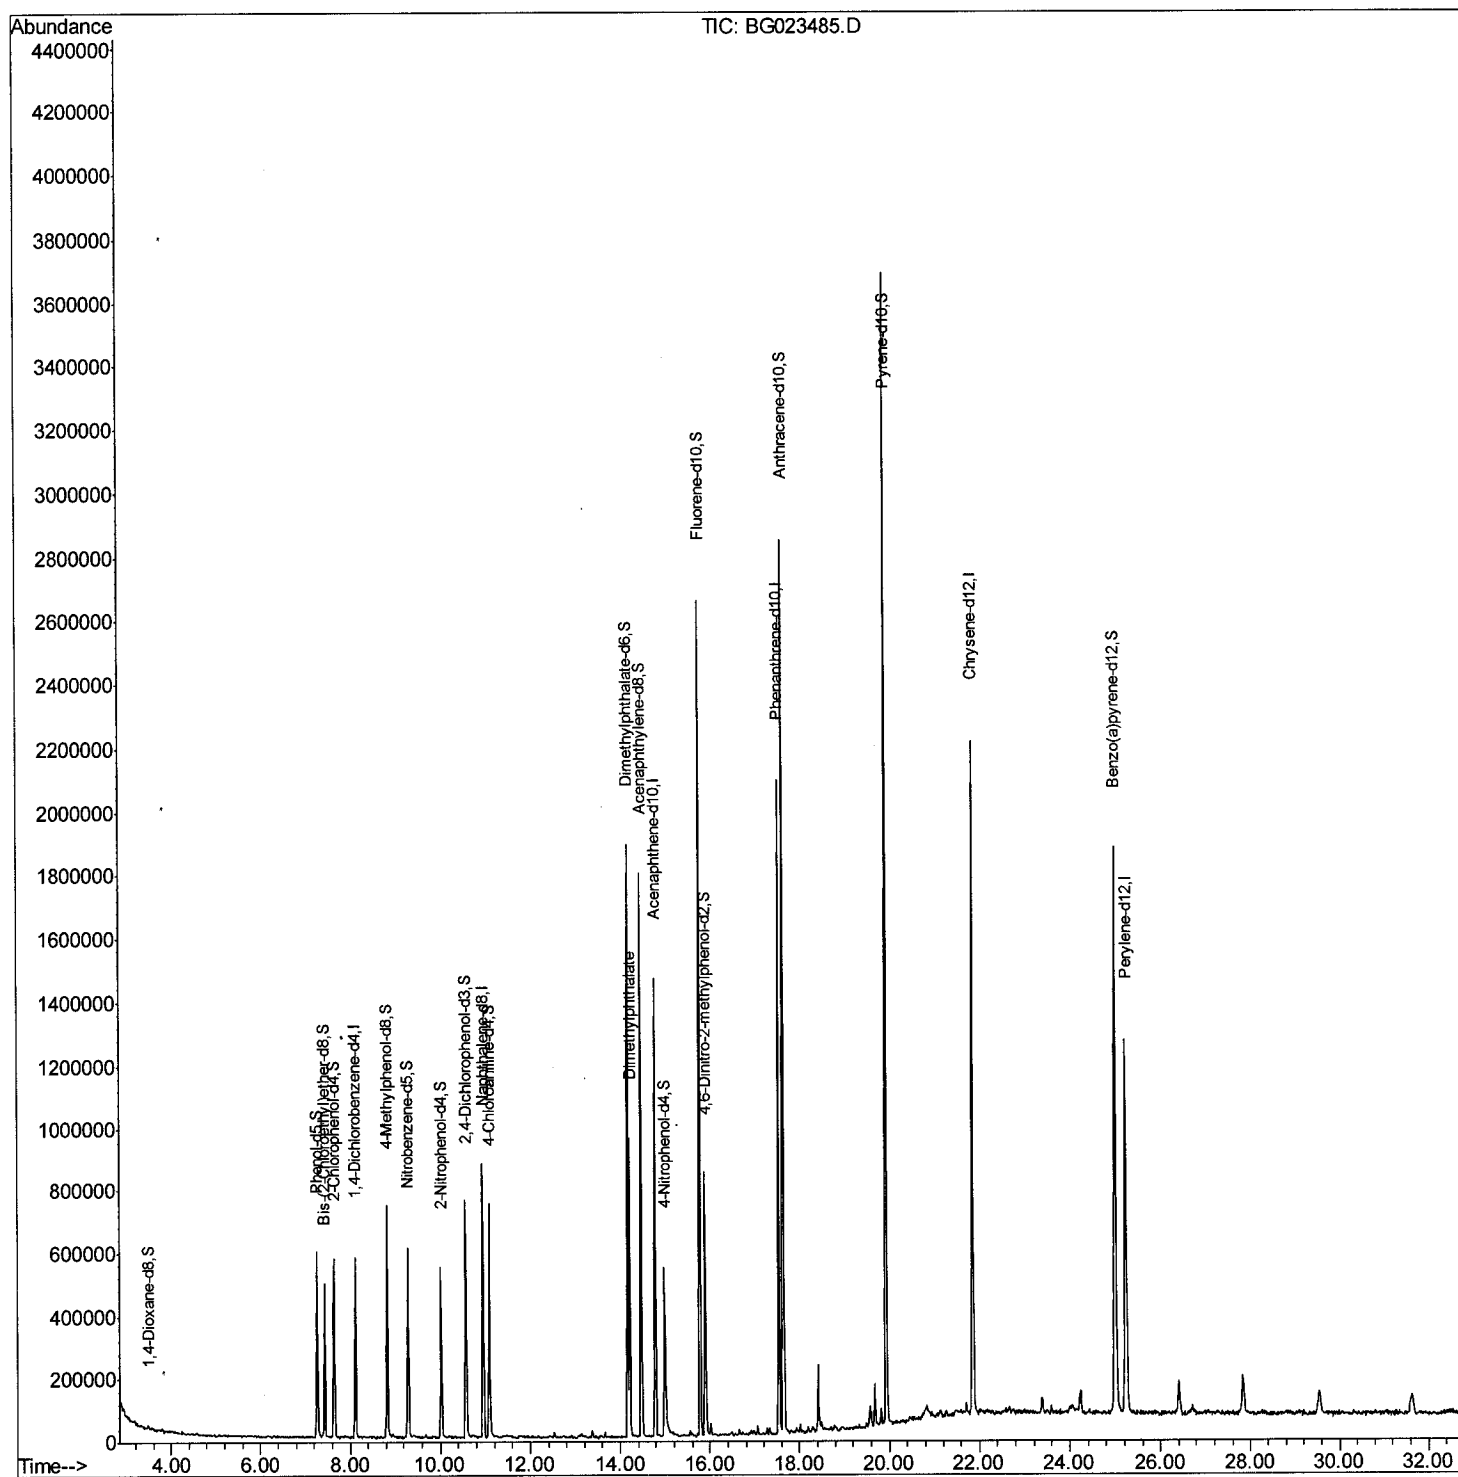

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA G\Data\BG080516\
 Data File : BG023485.D
 Acq On : 5 Aug 2016 13:08
 Operator : UM/SJ
 Sample : H4209-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Quant Time: Aug 05 23:14:59 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 30 02:24:23 2004
 Response via : Initial Calibration

Instrument :
 BNA G
 ClientSampleId :
 BDJH7

Manual Integrations
 APPROVED

sohil
 8/8/2016 6:56:00 PM

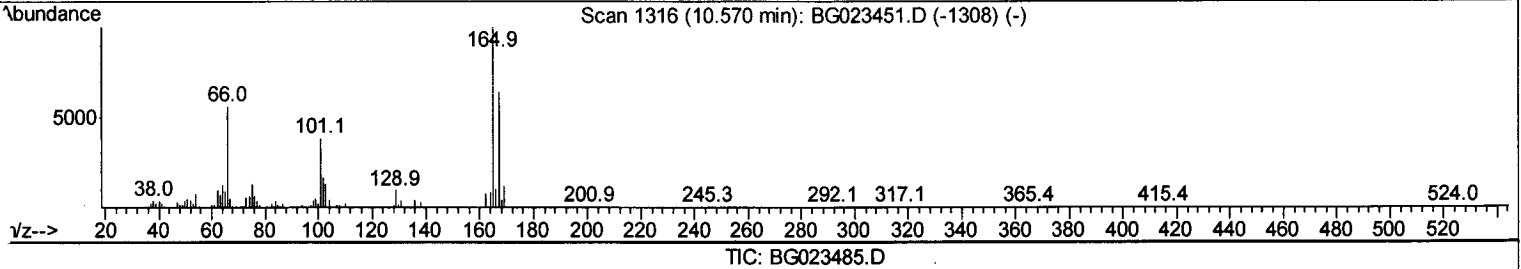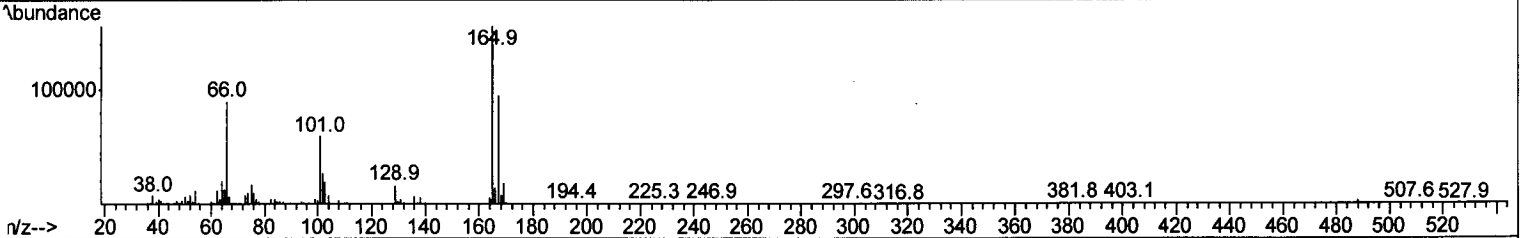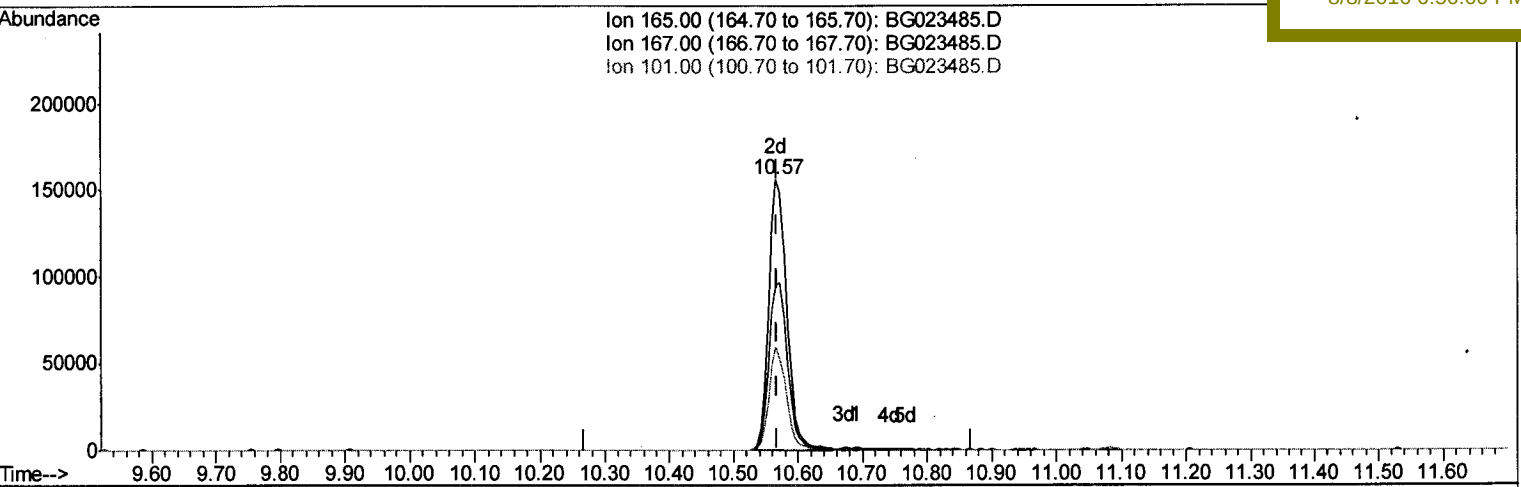

(26) 2,4-Dichlorophenol-d3 (S)

10.566min (-0.003) 24.25ng/ul m

response 292840

U.M
 08/09/16

Ion	Exp%	Act%
165.00	100	100
167.00	60.90	60.80
101.00	31.80	38.34#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA G\Data\BG080516\
 Data File : BG023485.D
 Acq On : 5 Aug 2016 13:08
 Operator : UM/SJ
 Sample : H4209-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDJH7

Manual Integrations
 APPROVED

sohil
 8/8/2016 6:56:00 PM

Quant Time: Aug 05 23:14:59 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 30 02:24:23 2004
 Response via : Initial Calibration

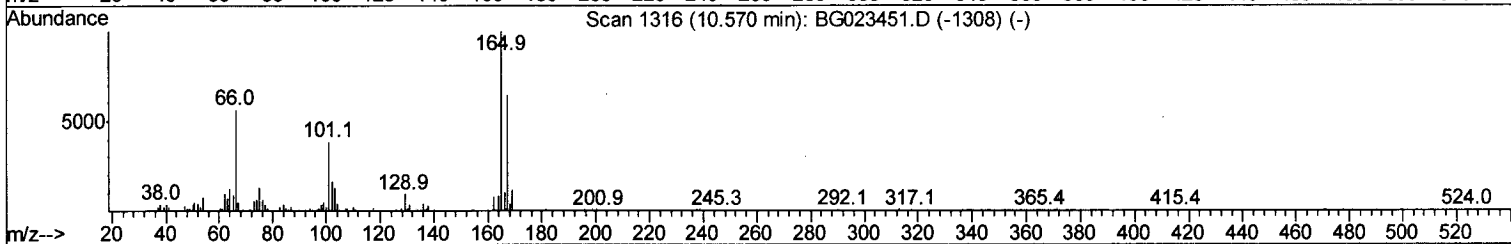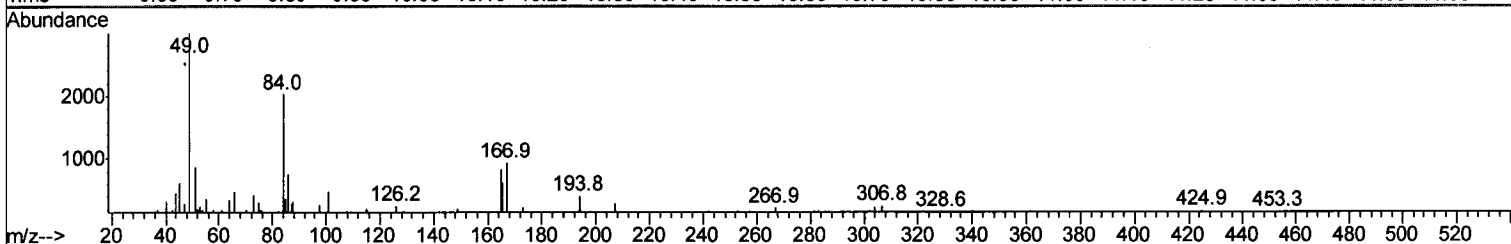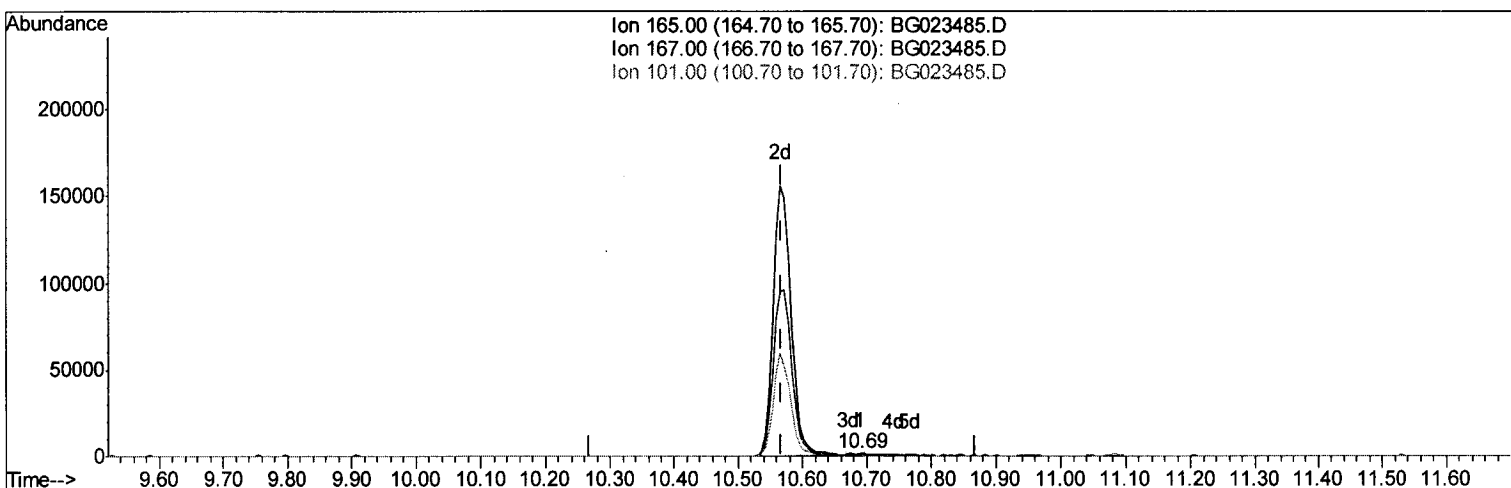

TIC: BG023485.D

(26) 2,4-Dichlorophenol-d3 (S)

10.689min (+0.121) 0.06ng/ul

response 668

Ion	Exp%	Act%
165.00	100	100
167.00	60.90	63.88
101.00	31.80	33.10
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG080516\
 Data File : BG023485.D
 Acq On : 5 Aug 2016 13:08
 Operator : UM/SJ
 Sample : H4209-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDJH7

Manual Integrations
 APPROVED

sohil
 8/8/2016 6:56:00 PM

Quant Time: Aug 06 00:21:57 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 30 02:24:23 2004
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	152403	20.00	ng/ul	0.00
18) Naphthalene-d8	10.95	136	707226	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.78	164	503713	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.54	188	1238283	20.00	ng/ul	0.00
75) Chrysene-d12	21.86	240	1305778	20.00	ng/ul	0.00
83) Perylene-d12	25.24	264	1258055	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.49	96	7422	2.07	ng/uL	0.00
5) Phenol-d5	7.27	99	361529	23.55	ng/ul	0.00
7) Bis- (2-Chloroethyl) ether-d	7.43	67	255805	26.00	ng/ul	0.00
9) 2-Chlorophenol-d4	7.64	132	251328	24.00	ng/ul	0.00
13) 4-Methylphenol-d8	8.83	113	284696	23.75	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	140098	25.13	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	166728	26.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.57	165	292840m	24.25	ng/ul	0.00
29) 4-Chloroaniline-d4	11.09	131	381583	26.93	ng/ul	0.00
43) Dimethylphthalate-d6	14.18	166	1207376	29.28	ng/ul	0.00
46) Acenaphthylene-d8	14.47	160	1298270	27.97	ng/ul	0.00
51) 4-Nitrophenol-d4	15.00	143	169136	24.02	ng/ul	0.00
57) Fluorene-d10	15.78	176	1064348	27.93	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.89	200	182551	22.98	ng/ul	0.00
70) Anthracene-d10	17.64	188	1621385	29.06	ng/ul	0.00
76) Pyrene-d10	19.93	212	1939524	29.34	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.00	264	1845511	32.41	ng/ul	0.00

U.M
 08/09/16

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.23	163	625529	15.32	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed