

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA G\DATA\BG080516\
 Data File : BG023523.D
 Acq On : 6 Aug 2016 15:06
 Operator : UM/SJ
 Sample : H4249-17
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampled :
 BDJQ8

Manual Integrations
 APPROVED

sohil
 8/8/2016 6:57:07 PM

Quant Time: Aug 08 01:58:07 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 01 04:44:16 2004
 Response via : Initial Calibration

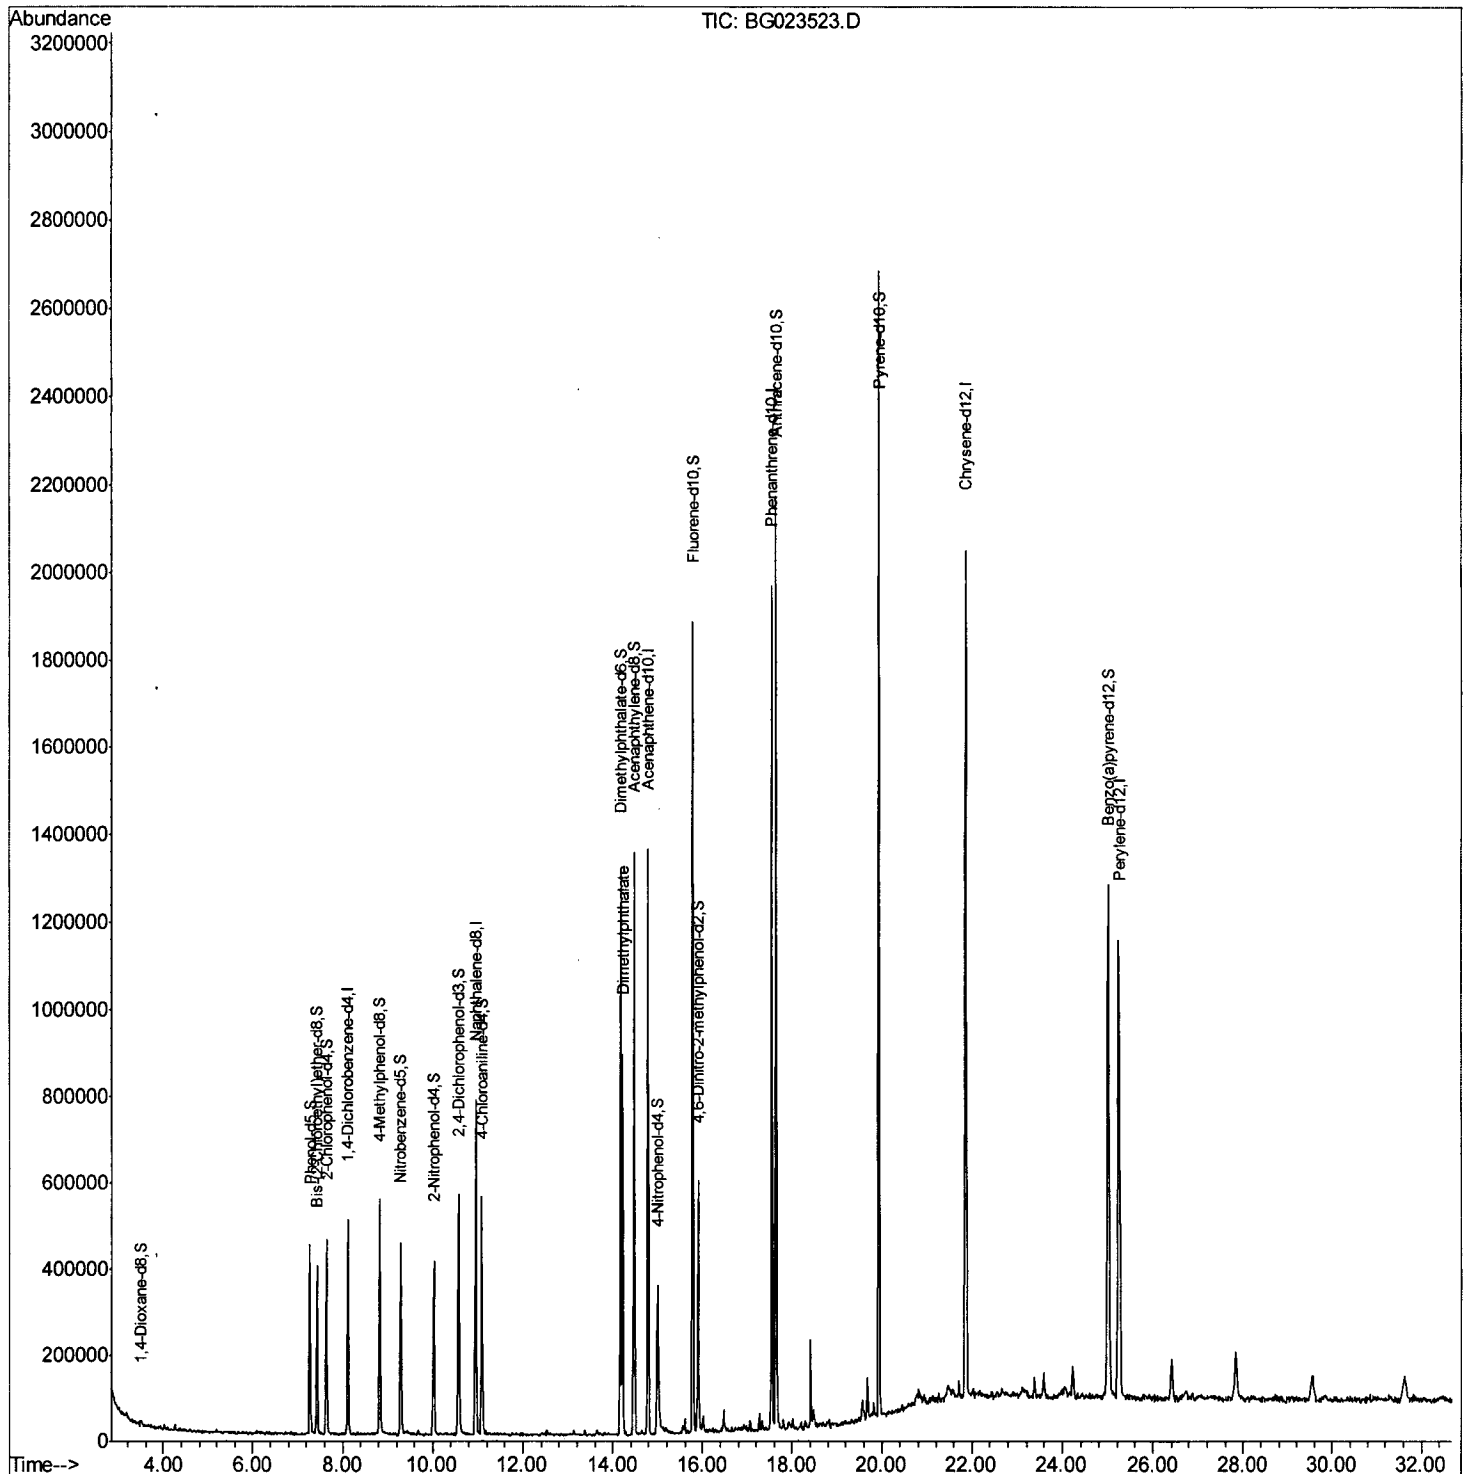

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA G\DATA\BG080516\
 Data File : BG023523.D
 Acq On : 6 Aug 2016 15:06
 Operator : UM/SJ
 Sample : H4249-17
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDJQ8

Manual Integrations
 APPROVED

sohil
 8/8/2016 6:57:07 PM

Quant Time: Aug 08 01:34:43 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 01 04:44:16 2004
 Response via : Initial Calibration

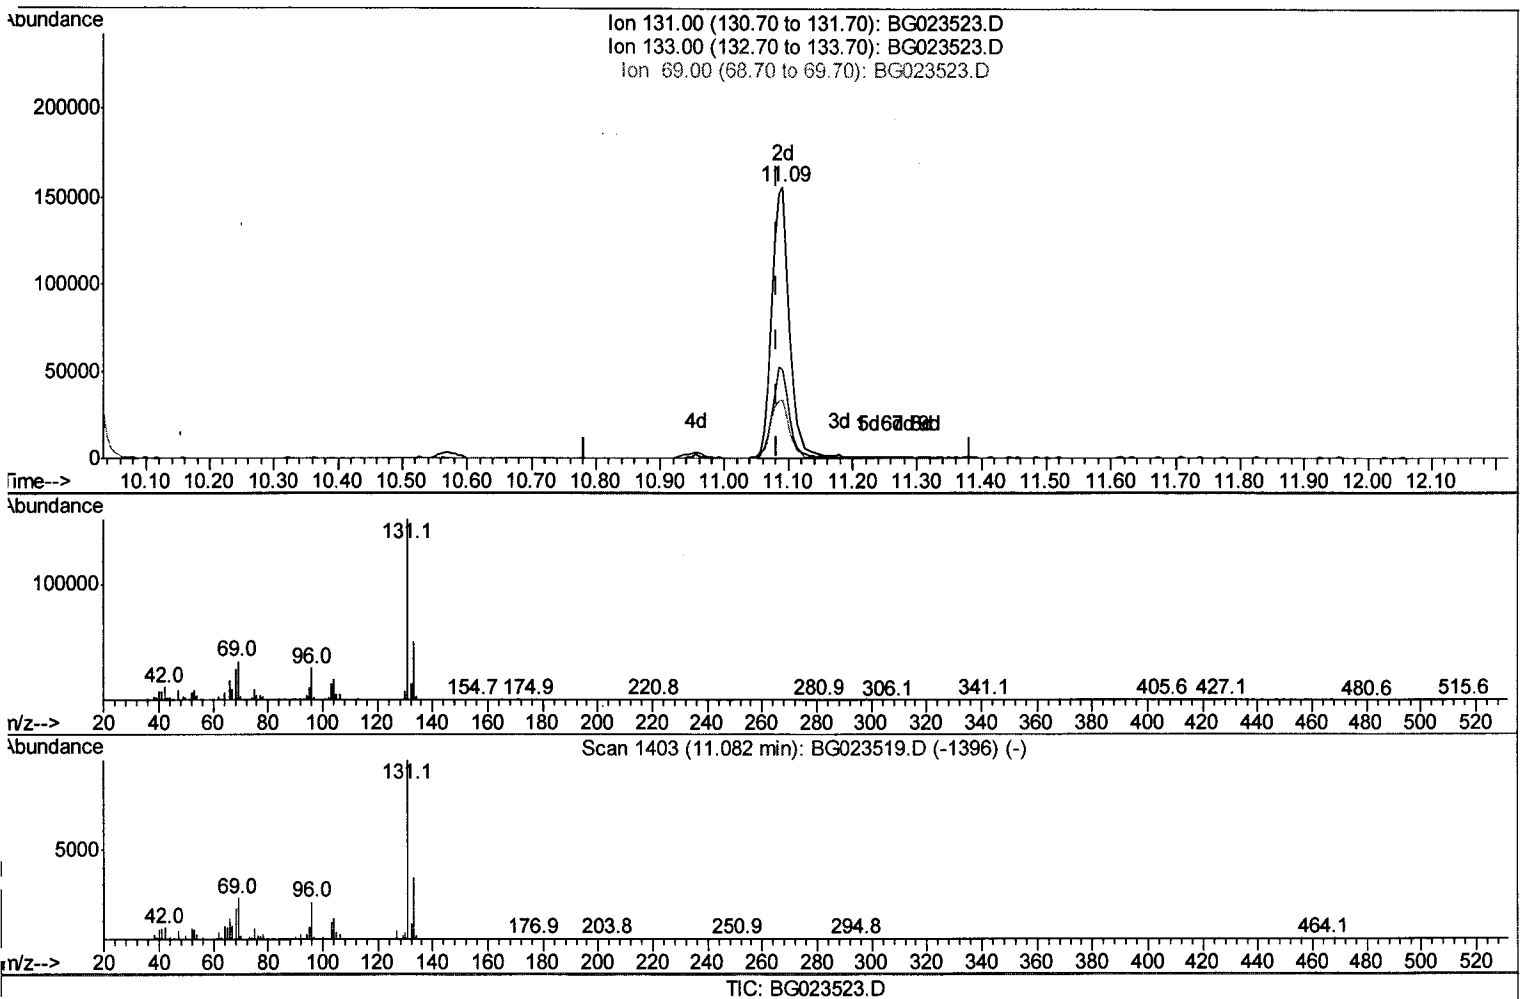

(29) 4-Chloroaniline-d4 (S)

11.091min (+0.009) 23.54ng/ul m

response 300897

Ion Exp% Act%

131.00 100 100

133.00 33.10 32.11

69.00 15.40 21.58#

0.00 0.00 0.00

U.M
 08/09/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA G\DATA\BG080516\
 Data File : BG023523.D
 Acq On : 6 Aug 2016 15:06
 Operator : UM/SJ
 Sample : H4249-17
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Quant Time: Aug 08 01:34:43 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 01 04:44:16 2004
 Response via : Initial Calibration

Instrument :
 BNA_G
 ClientSampleId :
 BDJQ8

Manual Integrations
 APPROVED

sohil
 8/8/2016 6:57:07 PM

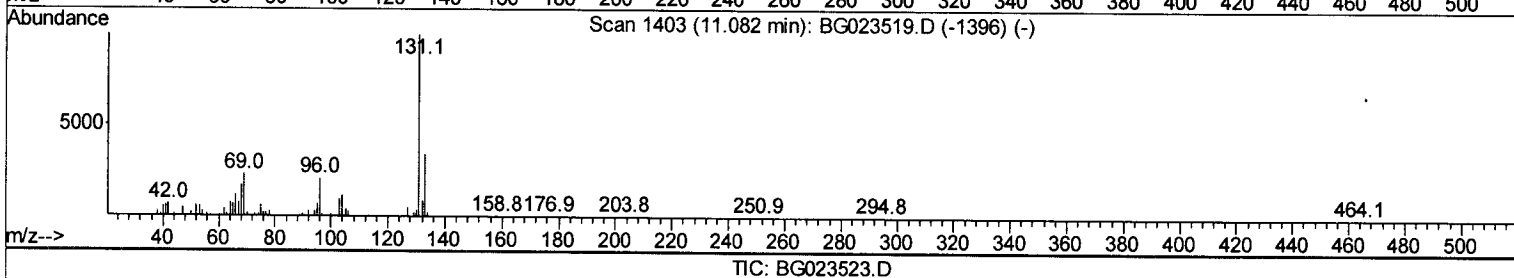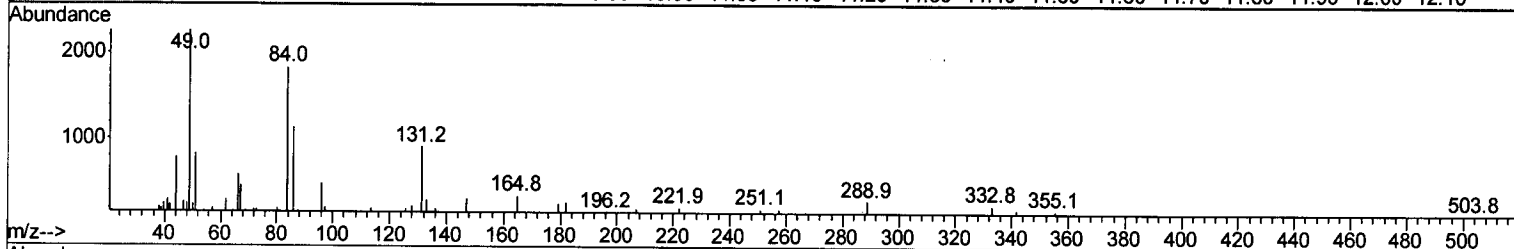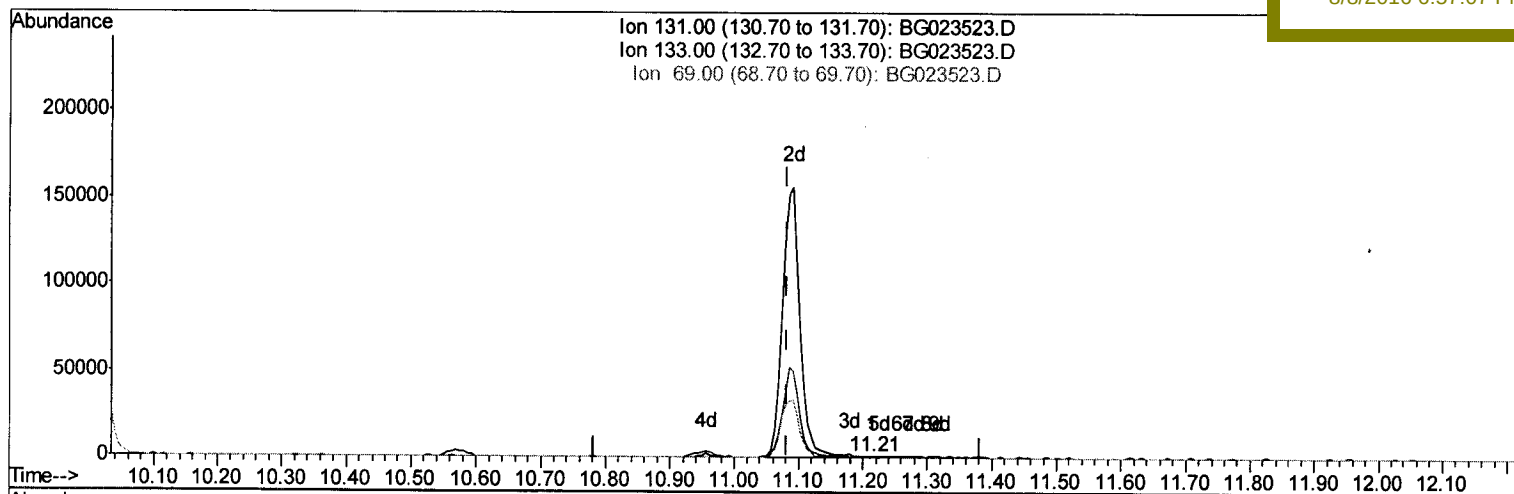

(29) 4-Chloroaniline-d4 (S)

11.214min (+0.133) 0.04ng/ul

response 564

Ion	Exp%	Act%
131.00	100	100
133.00	33.10	32.05
69.00	15.40	17.89
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG080516\
 Data File : BG023523.D
 Acq On : 6 Aug 2016 15:06
 Operator : UM/SJ
 Sample : H4249-17
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDJQ8

Manual Integrations
 APPROVED

sohil
 8/8/2016 6:57:07 PM

Quant Time: Aug 08 01:58:07 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 01 04:44:16 2004
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	138131	20.00	ng/ul	0.00
18) Naphthalene-d8	10.95	136	638012	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.78	164	462624	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.54	188	1170020	20.00	ng/ul	0.00
75) Chrysene-d12	21.86	240	1183916	20.00	ng/ul	0.00
83) Perylene-d12	25.24	264	1160174	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.49	96	6109	1.88	ng/uL	0.00
5) Phenol-d5	7.27	99	277507	19.94	ng/ul	0.00
7) Bis- (2-Chloroethyl) ether-d	7.43	67	197724	22.18	ng/ul	0.00
9) 2-Chlorophenol-d4	7.64	132	201291	21.20	ng/ul	0.00
13) 4-Methylphenol-d8	8.83	113	215599	19.85	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	108529	21.58	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	131454	22.76	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.57	165	218746	20.08	ng/ul	0.00
29) 4-Chloroaniline-d4	11.09	131	300897m	23.54	ng/ul	0.00
43) Dimethylphthalate-d6	14.18	166	834886	22.04	ng/ul	0.00
46) Acenaphthylene-d8	14.47	160	954710	22.40	ng/ul	0.00
51) 4-Nitrophenol-d4	15.00	143	112481	17.40	ng/ul	0.00
57) Fluorene-d10	15.78	176	766748	21.91	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	129242	17.22	ng/ul	0.00
70) Anthracene-d10	17.64	188	1184819	22.48	ng/ul	0.00
76) Pyrene-d10	19.93	212	1378462	23.00	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.01	264	1266943	24.13	ng/ul	0.00

U.M
 8/8/08/16

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.22	163	510944	13.62	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed