

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080516\
 Data File : BG023487.D
 Acq On : 5 Aug 2016 14:28
 Operator : UM/SJ
 Sample : H4209-05
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDJH9

Manual Integrations
 APPROVED

sohil
 8/8/2016 6:56:04 PM

Quant Time: Aug 06 00:39:53 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 30 02:24:23 2004
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	140602	20.00	ng/ul	0.00
18) Naphthalene-d8	10.95	136	655344	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.78	164	469664	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.54	188	1150822	20.00	ng/ul	0.00
75) Chrysene-d12	21.86	240	1175198	20.00	ng/ul	0.00
83) Perylene-d12	25.24	264	1125279	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.49	96	5870	1.77	ng/uL	0.00
5) Phenol-d5	7.27	99	314307	22.19	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.43	67	229683	25.31	ng/ul	0.00
9) 2-Chlorophenol-d4	7.65	132	224410	23.22	ng/ul	0.00
13) 4-Methylphenol-d8	8.83	113	258312	23.36	ng/ul	0.00
19) Nitrobenzene-d5	9.30	128	122313	23.68	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	147559	24.87	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.57	165	251617	22.48	ng/ul	0.00
29) 4-Chloroaniline-d4	11.09	131	362082m	27.58	ng/ul	0.00
43) Dimethylphthalate-d6	14.18	166	964073	25.07	ng/ul	0.00
46) Acenaphthylene-d8	14.48	160	1052593	24.32	ng/ul	0.00
51) 4-Nitrophenol-d4	15.00	143	94788	14.44	ng/ul	0.00
57) Fluorene-d10	15.78	176	862735	24.28	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	119273	16.15	ng/ul	0.00
70) Anthracene-d10	17.64	188	1358849	26.21	ng/ul	0.00
76) Pyrene-d10	19.93	212	1586138	26.66	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.00	264	1415929	27.80	ng/ul	0.00

Target Compounds					Qvalue
44) Dimethylphthalate	14.22	163	664897	17.46 ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080516\
Data File : BG023487.D
Acq On : 5 Aug 2016 14:28
Operator : UM/SJ
Sample : H4209-05
Misc :
ALS Vial : 30 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
BDJH9

Manual Integrations
APPROVED

sohil
8/8/2016 6:56:04 PM

Quant Time: Aug 06 00:39:53 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 30 02:24:23 2004
Response via : Initial Calibration

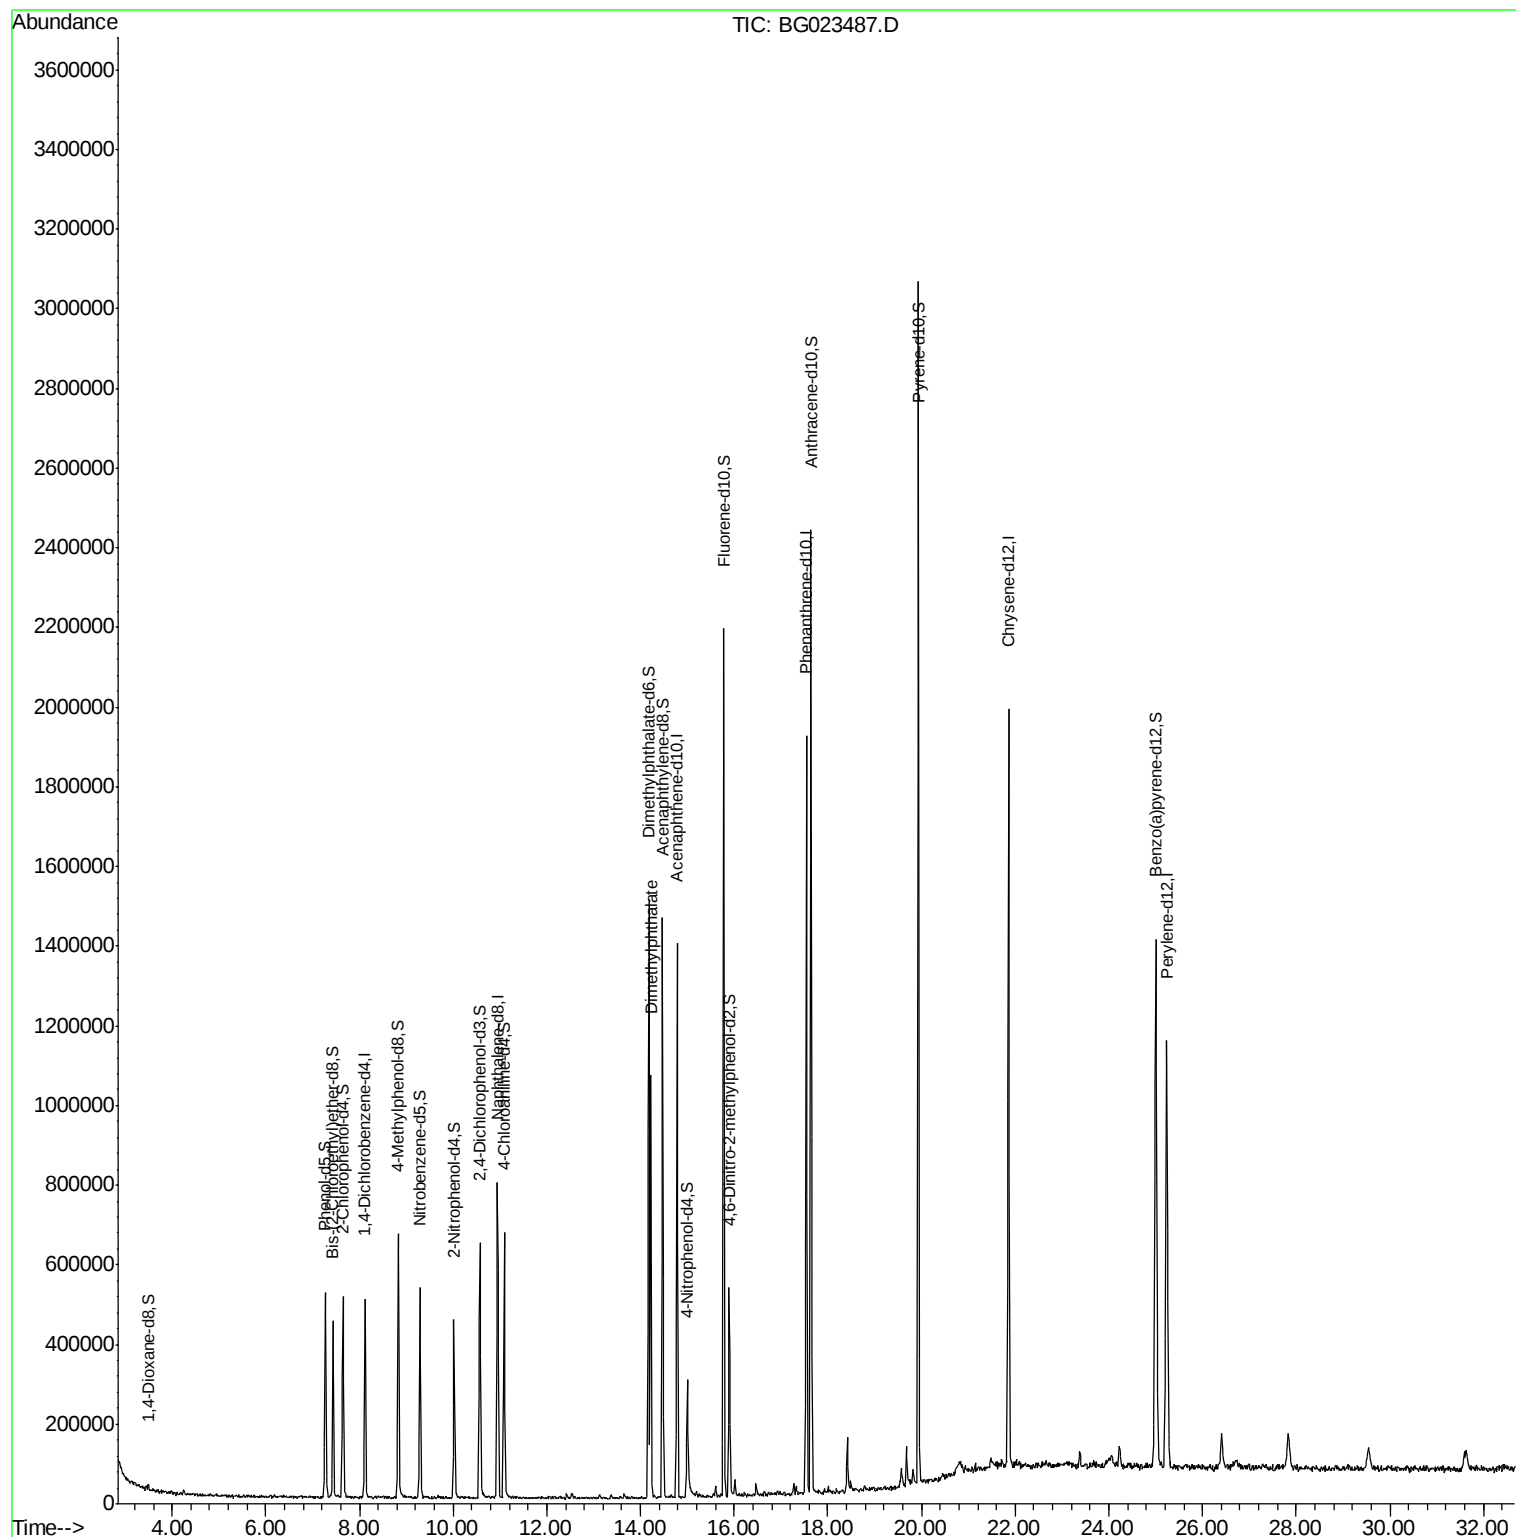

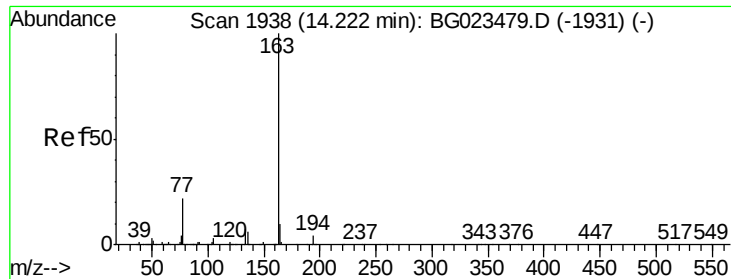

#44
 Dimethylphthalate
 Concen: 17.46 ng/ul
 RT: 14.22 min Scan# 1938
 Delta R.T. 0.00 min
 Lab File: BG023487.D
 Acq: 5 Aug 2016 14:28

Instrument :
 BNA_G
 ClientSampleId :
 BDJH9

Tgt Ion	Ratio	Resp Lower	Resp Upper
163	100		
194	4.8	3.4	5.2
164	11.0	8.8	13.2

Manual Integrations
 APPROVED

sohil
 8/8/2016 6:56:04 PM

