

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080516\
 Data File : BG023491.D
 Acq On : 5 Aug 2016 17:08
 Operator : UM/SJ
 Sample : H4209-10
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDJM3

Manual Integrations
 APPROVED

sohil
 8/8/2016 6:56:13 PM

Quant Time: Aug 06 01:07:17 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 30 02:24:23 2004
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	141763	20.00	ng/ul	0.00
18) Naphthalene-d8	10.95	136	652012	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.78	164	473685	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.54	188	1209789	20.00	ng/ul	0.00
75) Chrysene-d12	21.85	240	1253148	20.00	ng/ul	0.00
83) Perylene-d12	25.24	264	1217904	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.49	96	4794	1.44	ng/uL	0.00
5) Phenol-d5	7.27	99	243710	17.07	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.43	67	175853	19.22	ng/ul	0.00
9) 2-Chlorophenol-d4	7.64	132	171604	17.61	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	197328	17.70	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	93131m	18.12	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	109504	18.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.57	165	190277	17.09	ng/ul	0.00
29) 4-Chloroaniline-d4	11.09	131	272006m	20.82	ng/ul	0.00
43) Dimethylphthalate-d6	14.18	166	760802	19.62	ng/ul	0.00
46) Acenaphthylene-d8	14.48	160	855514	19.60	ng/ul	0.00
51) 4-Nitrophenol-d4	15.00	143	86216	13.02	ng/ul	0.00
57) Fluorene-d10	15.77	176	685704	19.13	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	99858	12.87	ng/ul	0.00
70) Anthracene-d10	17.64	188	1066791	19.57	ng/ul	0.00
76) Pyrene-d10	19.93	212	1217843	19.20	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.00	264	1035914	18.79	ng/ul	0.00

Target Compounds						Qvalue
44) Dimethylphthalate	14.22	163	401773	10.46	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080516\
Data File : BG023491.D
Acq On : 5 Aug 2016 17:08
Operator : UM/SJ
Sample : H4209-10
Misc :
ALS Vial : 34 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
BDJM3

Manual Integrations
APPROVED

sohil
8/8/2016 6:56:13 PM

Quant Time: Aug 06 01:07:17 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 30 02:24:23 2004
Response via : Initial Calibration

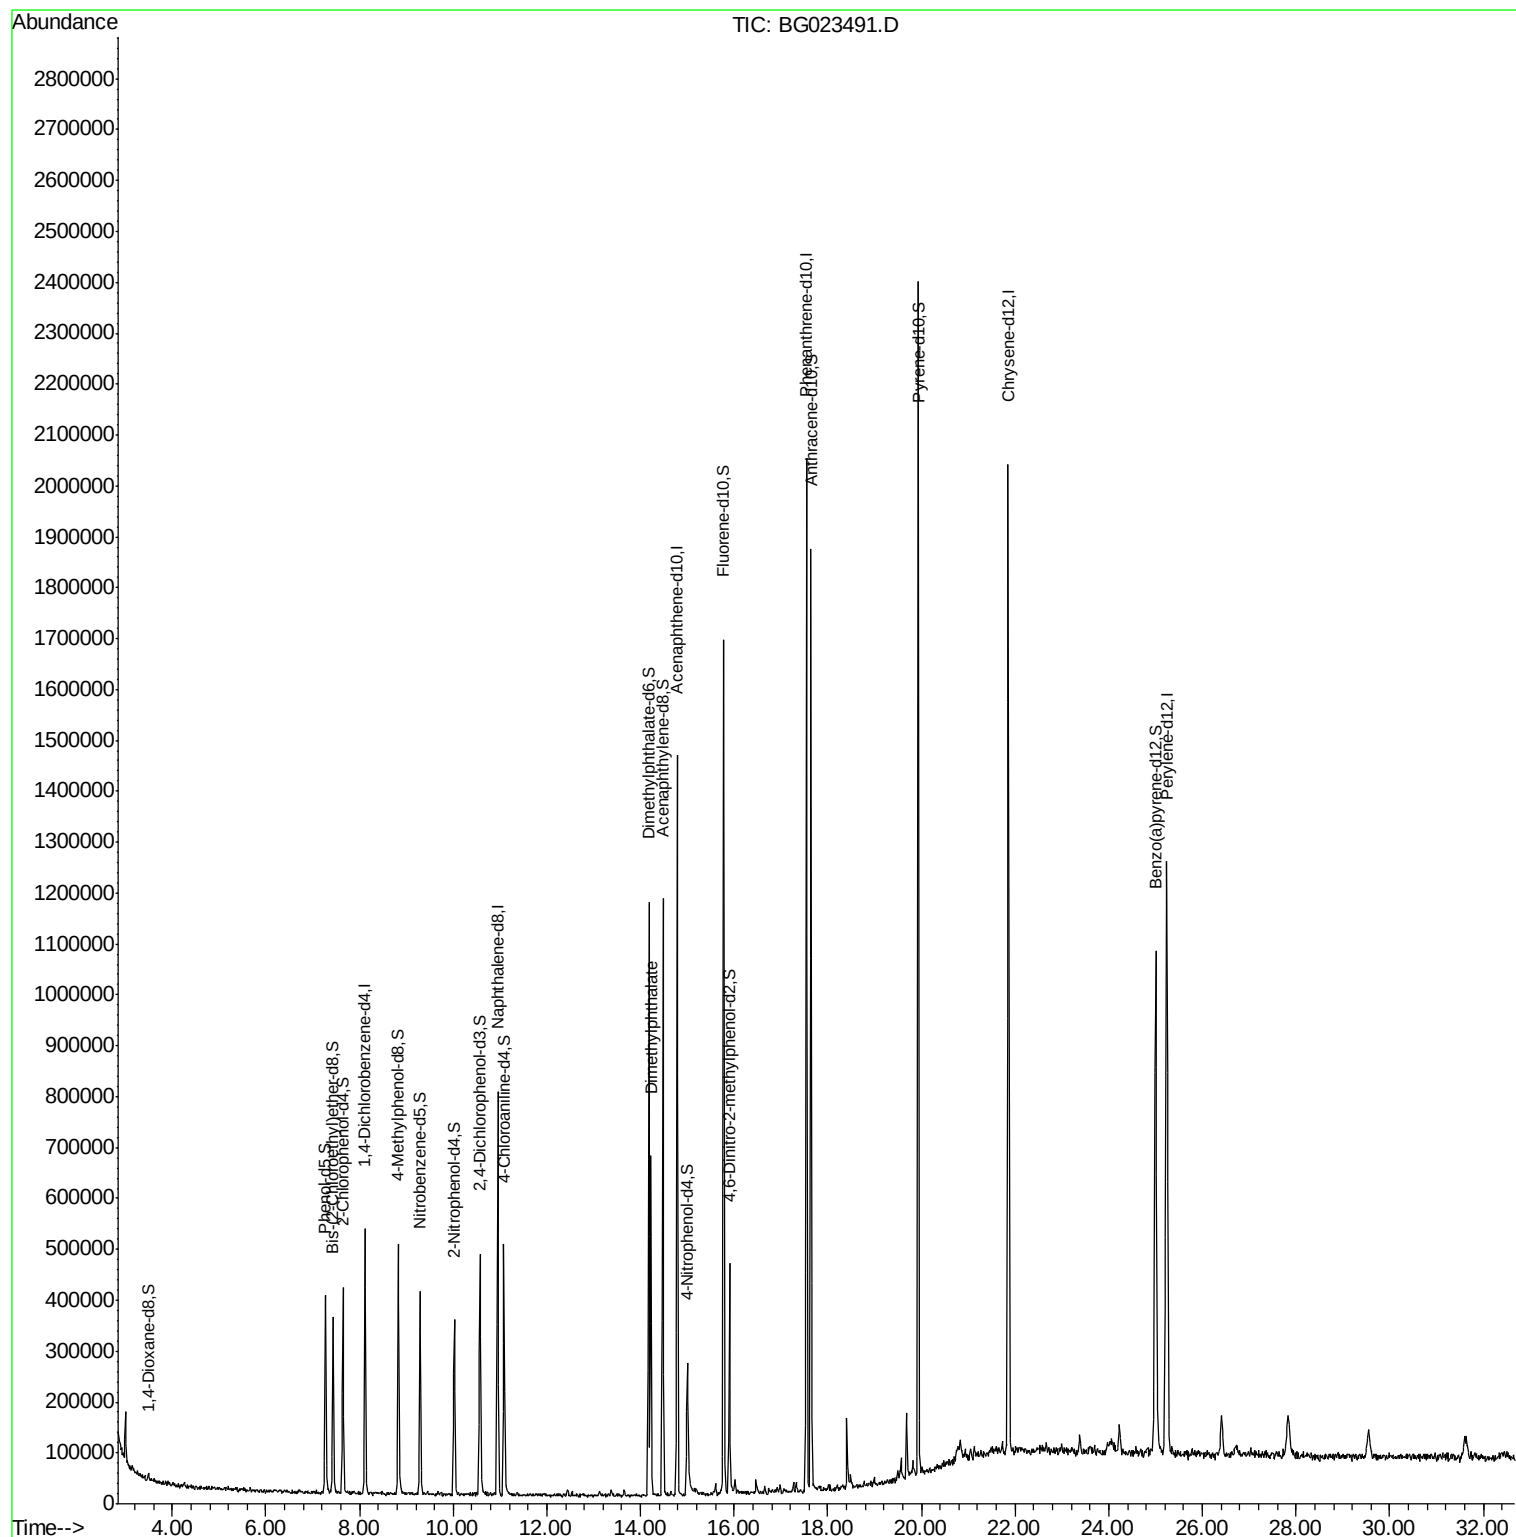

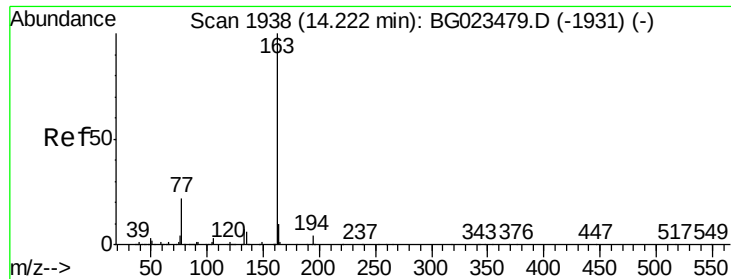

#44

Dimethylphthalate

Concen: 10.46 ng/ul

RT: 14.22 min Scan# 1938

Delta R.T. 0.00 min

Lab File: BG023491.D


Acq: 5 Aug 2016 17:08

Instrument :

BNA_G

ClientSampleId :

BDJM3

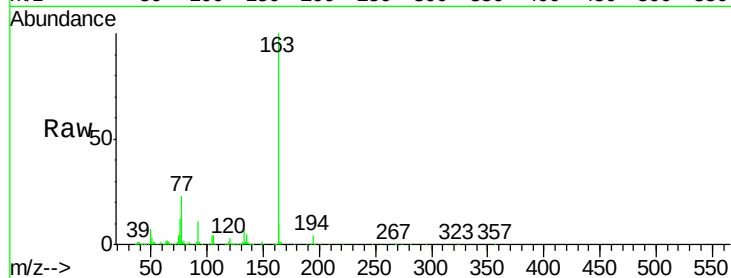

Tgt	Ion	Ratio	Resp	Lower	Upper
163	100		401773		
194	3.9			3.4	5.2
164	10.0			8.8	13.2

Manual Integrations
APPROVED

sohil
8/8/2016 6:56:13 PM

