

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080516\
 Data File : BG023523.D
 Acq On : 6 Aug 2016 15:06
 Operator : UM/SJ
 Sample : H4249-17
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDJQ8

Manual Integrations
 APPROVED

sohil
 8/8/2016 6:57:07 PM

Quant Time: Aug 08 01:58:07 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 01 04:44:16 2004
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	138131	20.00	ng/ul	0.00
18) Naphthalene-d8	10.95	136	638012	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.78	164	462624	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.54	188	1170020	20.00	ng/ul	0.00
75) Chrysene-d12	21.86	240	1183916	20.00	ng/ul	0.00
83) Perylene-d12	25.24	264	1160174	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.49	96	6109	1.88	ng/uL	0.00
5) Phenol-d5	7.27	99	277507	19.94	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.43	67	197724	22.18	ng/ul	0.00
9) 2-Chlorophenol-d4	7.64	132	201291	21.20	ng/ul	0.00
13) 4-Methylphenol-d8	8.83	113	215599	19.85	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	108529	21.58	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	131454	22.76	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.57	165	218746	20.08	ng/ul	0.00
29) 4-Chloroaniline-d4	11.09	131	300897m	23.54	ng/ul	0.00
43) Dimethylphthalate-d6	14.18	166	834886	22.04	ng/ul	0.00
46) Acenaphthylene-d8	14.47	160	954710	22.40	ng/ul	0.00
51) 4-Nitrophenol-d4	15.00	143	112481	17.40	ng/ul	0.00
57) Fluorene-d10	15.78	176	766748	21.91	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	129242	17.22	ng/ul	0.00
70) Anthracene-d10	17.64	188	1184819	22.48	ng/ul	0.00
76) Pyrene-d10	19.93	212	1378462	23.00	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.01	264	1266943	24.13	ng/ul	0.00

Target Compounds					Qvalue
44) Dimethylphthalate	14.22	163	510944	13.62 ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080516\
Data File : BG023523.D
Acq On : 6 Aug 2016 15:06
Operator : UM/SJ
Sample : H4249-17
Misc :
ALS Vial : 63 Sample Multiplier: 1




Instrument :
BNA_G
ClientSampleId :
BDJQ8

Manual Integrations
APPROVED

sohil
8/8/2016 6:57:07 PM

Quant Time: Aug 08 01:58:07 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 01 04:44:16 2004
Response via : Initial Calibration

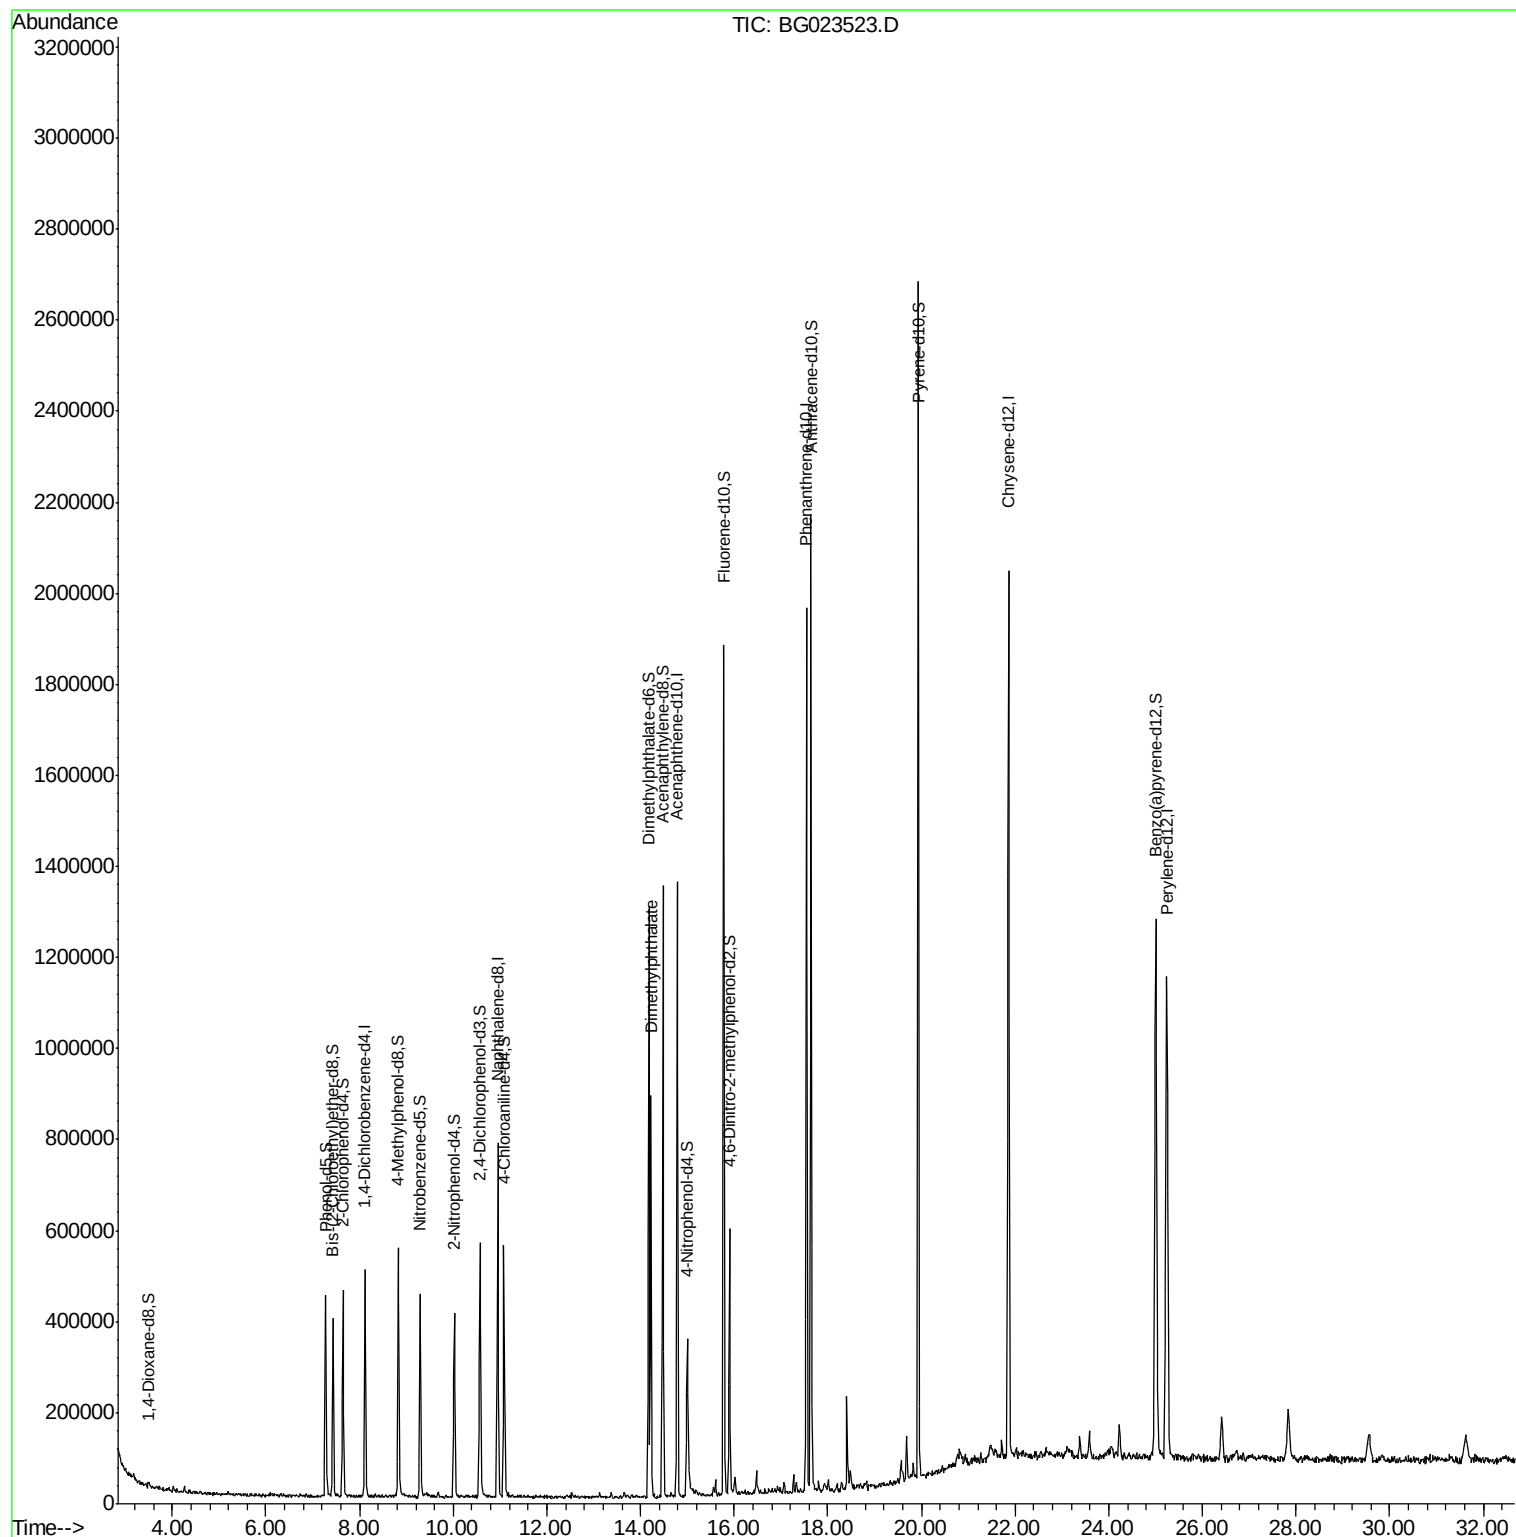

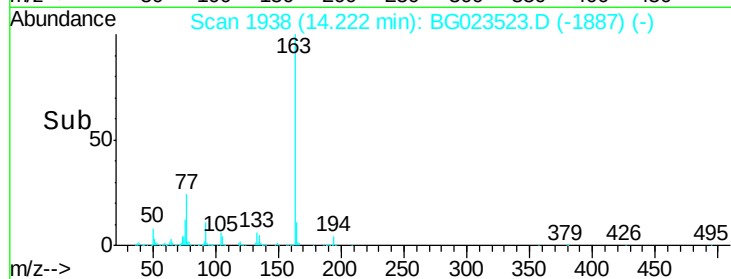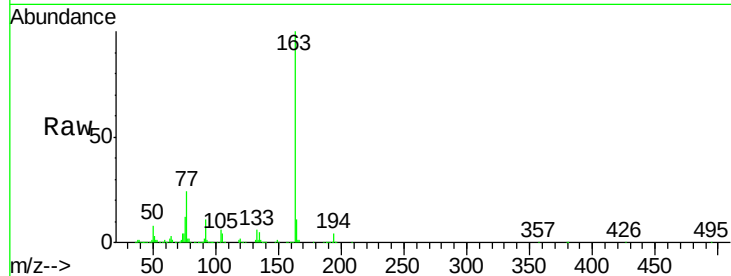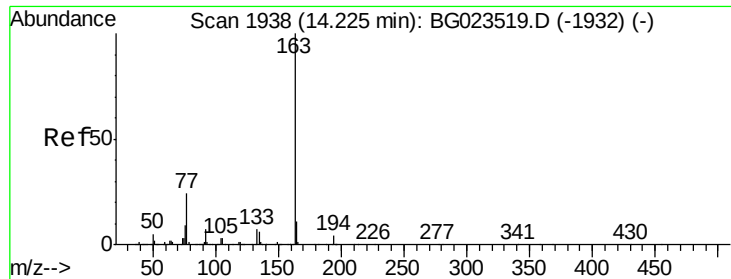

#44

Dimethylphthalate

Concen: 13.62 ng/ul

RT: 14.22 min Scan# 1938

Delta R.T. -0.00 min

Lab File: BG023523.D

Acq: 6 Aug 2016 15:06

Instrument :

BNA_G

ClientSampleId :

BDJQ8

Tgt Ion:	163	Resp:	510944
Ion Ratio	Lower	Upper	
163	100		
194	4.3	3.4	5.2
164	10.6	8.8	13.2

Manual Integrations
APPROVED

sohil
8/8/2016 6:57:07 PM

