

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080516\
 Data File : BG023528.D
 Acq On : 6 Aug 2016 18:26
 Operator : UM/SJ
 Sample : H4249-22
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDJR3

Quant Time: Aug 08 02:10:35 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 01 04:44:16 2004
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	150302	20.00	ng/ul	0.00
18) Naphthalene-d8	10.95	136	689039	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.78	164	513574	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.54	188	1248507	20.00	ng/ul	0.00
75) Chrysene-d12	21.86	240	1287395	20.00	ng/ul	0.00
83) Perylene-d12	25.24	264	1275448	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.49	96	8919	2.52	ng/uL	0.00
5) Phenol-d5	7.27	99	425240	28.09	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.43	67	295052	30.41	ng/ul	0.00
9) 2-Chlorophenol-d4	7.65	132	296338	28.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.83	113	342019	28.93	ng/ul	0.00
19) Nitrobenzene-d5	9.30	128	162985	30.01	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	194437	31.17	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.57	165	343756	29.22	ng/ul	0.00
29) 4-Chloroaniline-d4	11.09	131	460910	33.39	ng/ul	0.00
43) Dimethylphthalate-d6	14.18	166	1326579	31.55	ng/ul	0.00
46) Acenaphthylene-d8	14.48	160	1459063	30.83	ng/ul	0.00
51) 4-Nitrophenol-d4	14.99	143	229656	31.99	ng/ul	0.00
57) Fluorene-d10	15.78	176	1198122	30.84	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	244219	30.49	ng/ul	0.00
70) Anthracene-d10	17.64	188	1869484	33.24	ng/ul	0.00
76) Pyrene-d10	19.94	212	2078744	31.90	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.00	264	2079019	36.01	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	14.23	163	894819	21.49	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080516\
Data File : BG023528.D
Acq On : 6 Aug 2016 18:26
Operator : UM/SJ
Sample : H4249-22
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDJR3

Quant Time: Aug 08 02:10:35 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 01 04:44:16 2004
Response via : Initial Calibration

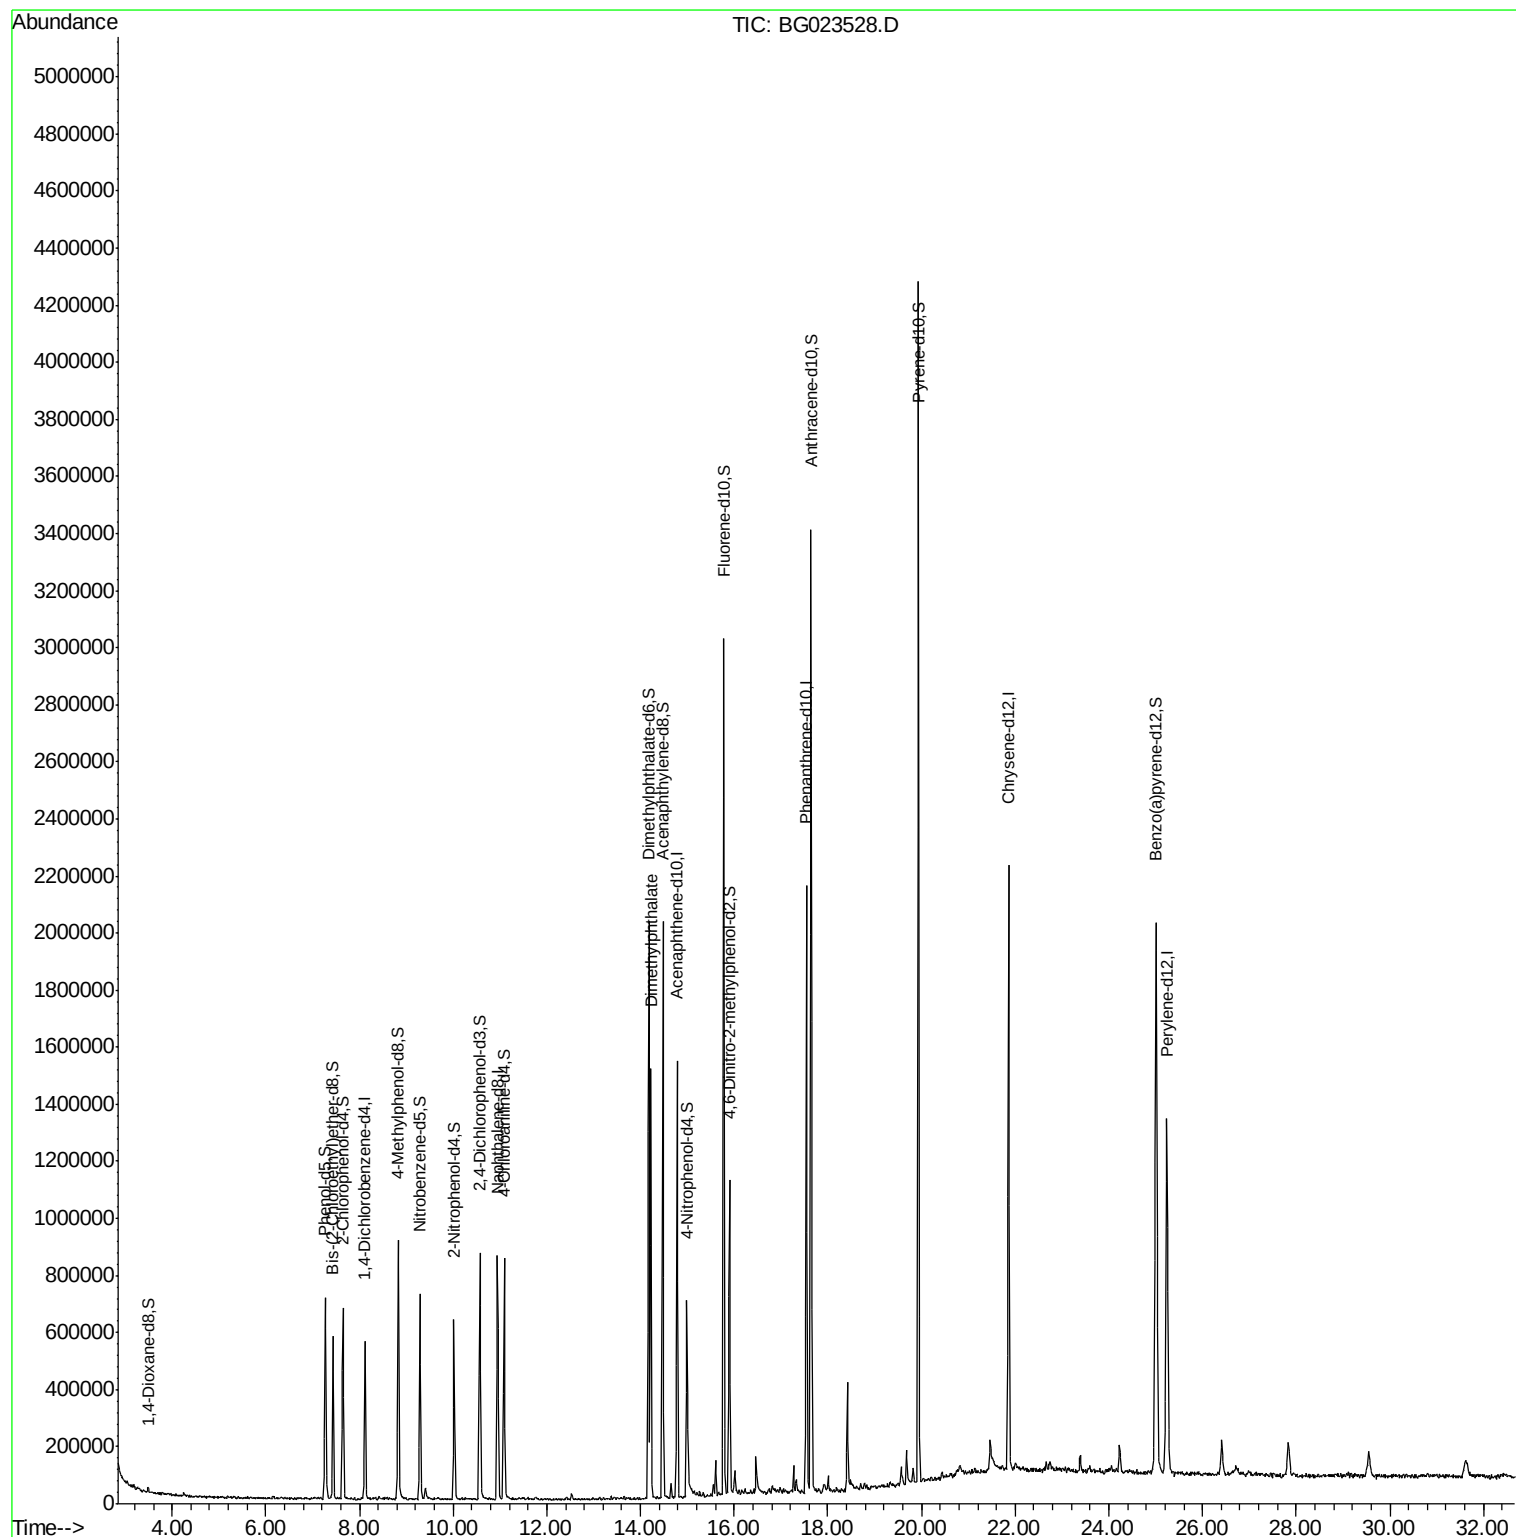

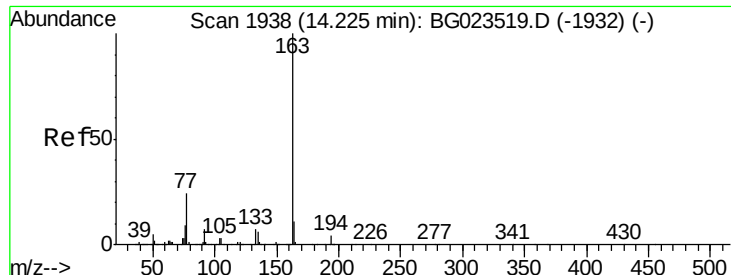

#44

Dimethylphthalate

Concen: 21.49 ng/ul

RT: 14.23 min Scan# 1938

Delta R.T. 0.00 min

Lab File: BG023528.D

Acq: 6 Aug 2016 18:26

Instrument :

BNA_G

ClientSampleId :

BDJR3

Tgt Ion:163 Resp: 894819

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.2

164 11.5 8.8 13.2

