
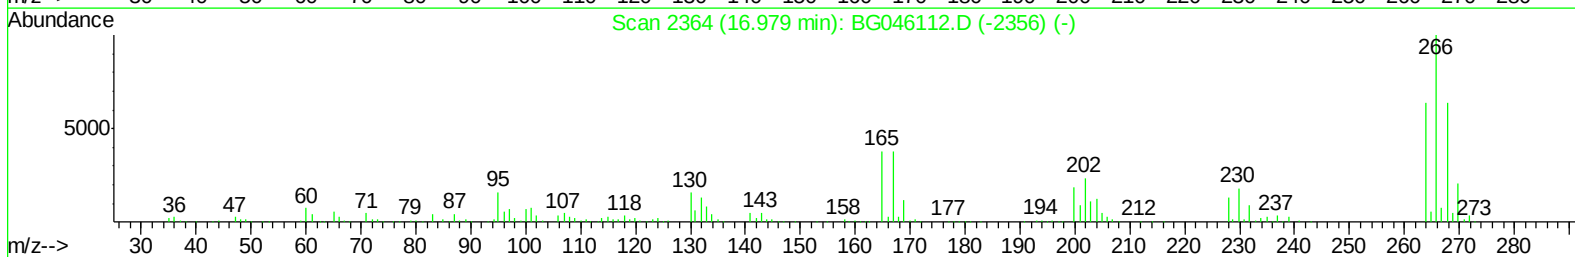
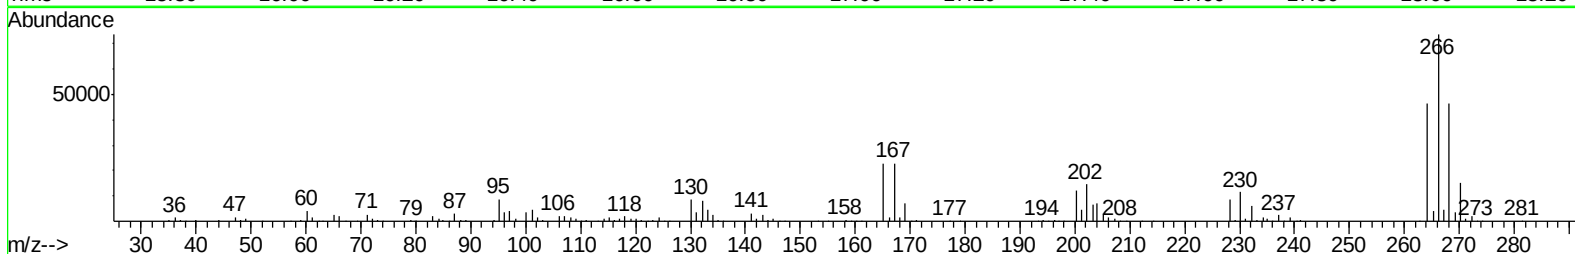


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080520\
 Data File : BG046167.D
 Acq On : 5 Aug 2020 9:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 07:16:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 30 18:43:49 2020
 Response via : Initial Calibration

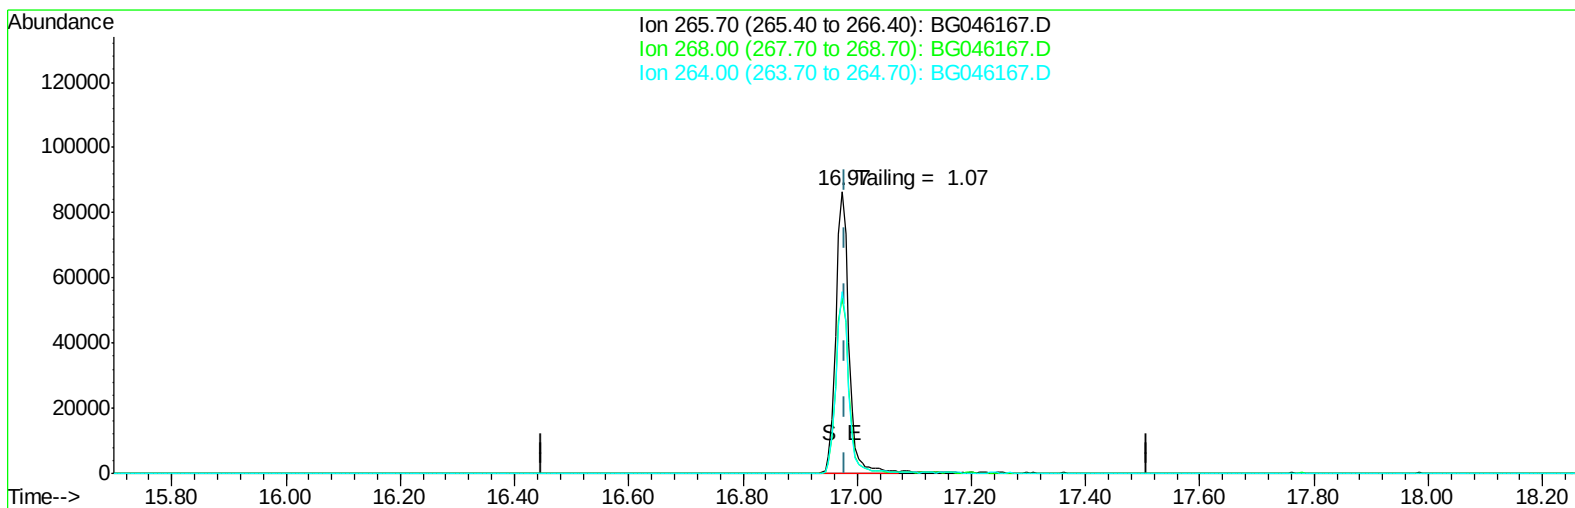

TIC: BG046167.D

(70) Pentachlorophenol (C)




16.974min (-0.006) 244893.56ng

response 136474

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	62.33
264.00	63.90	64.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080520\
 Data File : BG046167.D
 Acq On : 5 Aug 2020 9:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 07:16:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 30 18:43:49 2020
 Response via : Initial Calibration

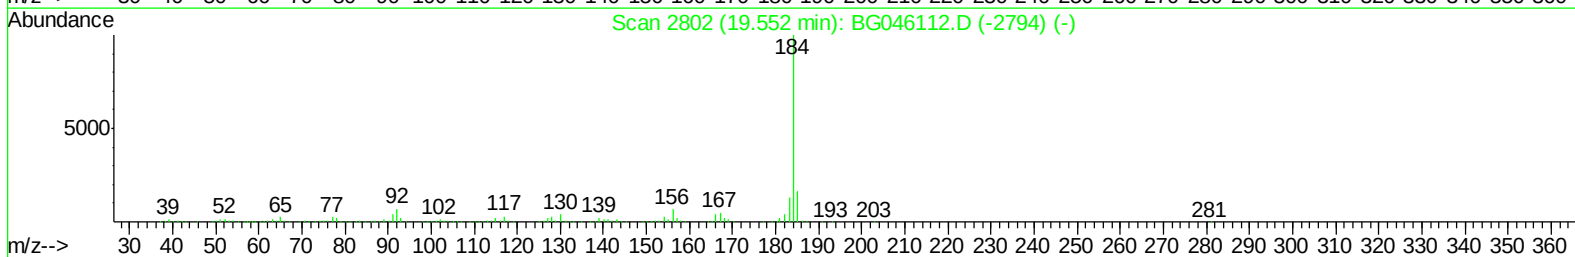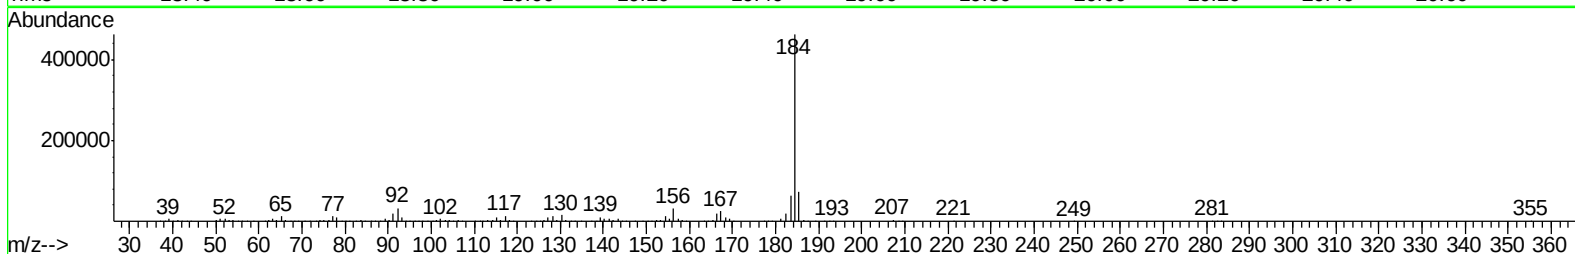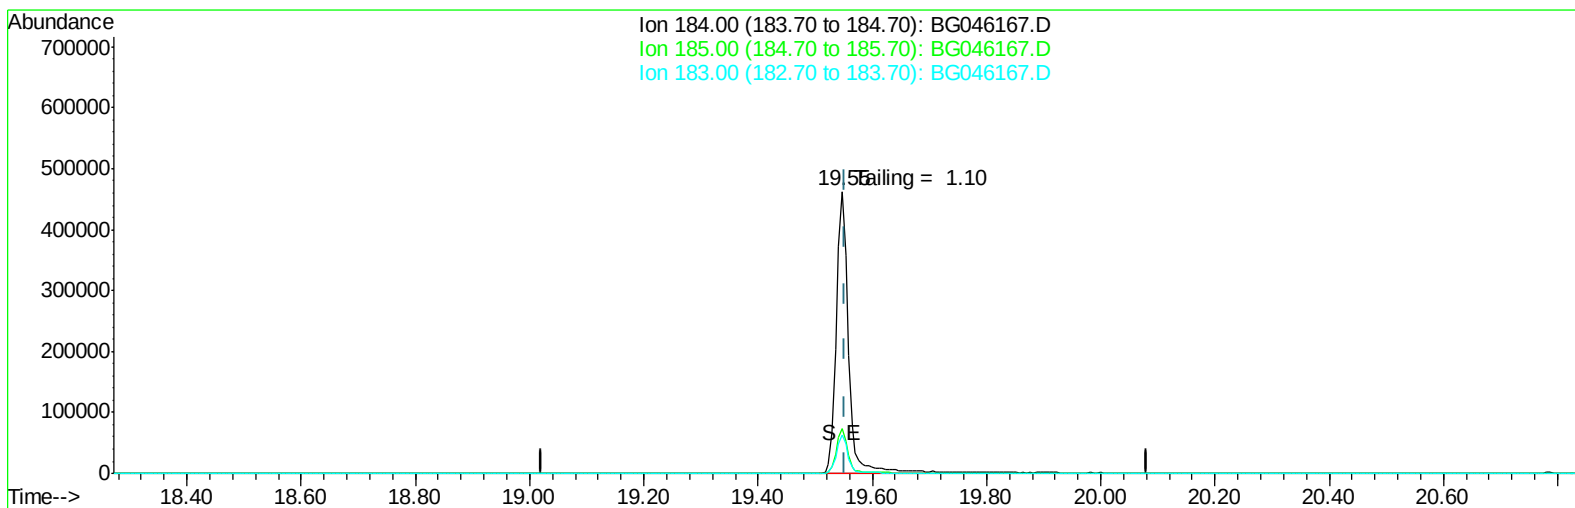

TIC: BG046167.D

(77) Benzidine

19.547min (-0.006) 28598.74ng

response 684516

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	16.10
183.00	13.10	13.64
0.00	0.00	0.00