


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080520\
 Data File : BG046167.D
 Acq On : 5 Aug 2020 9:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG073020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 30 18:43:49 2020

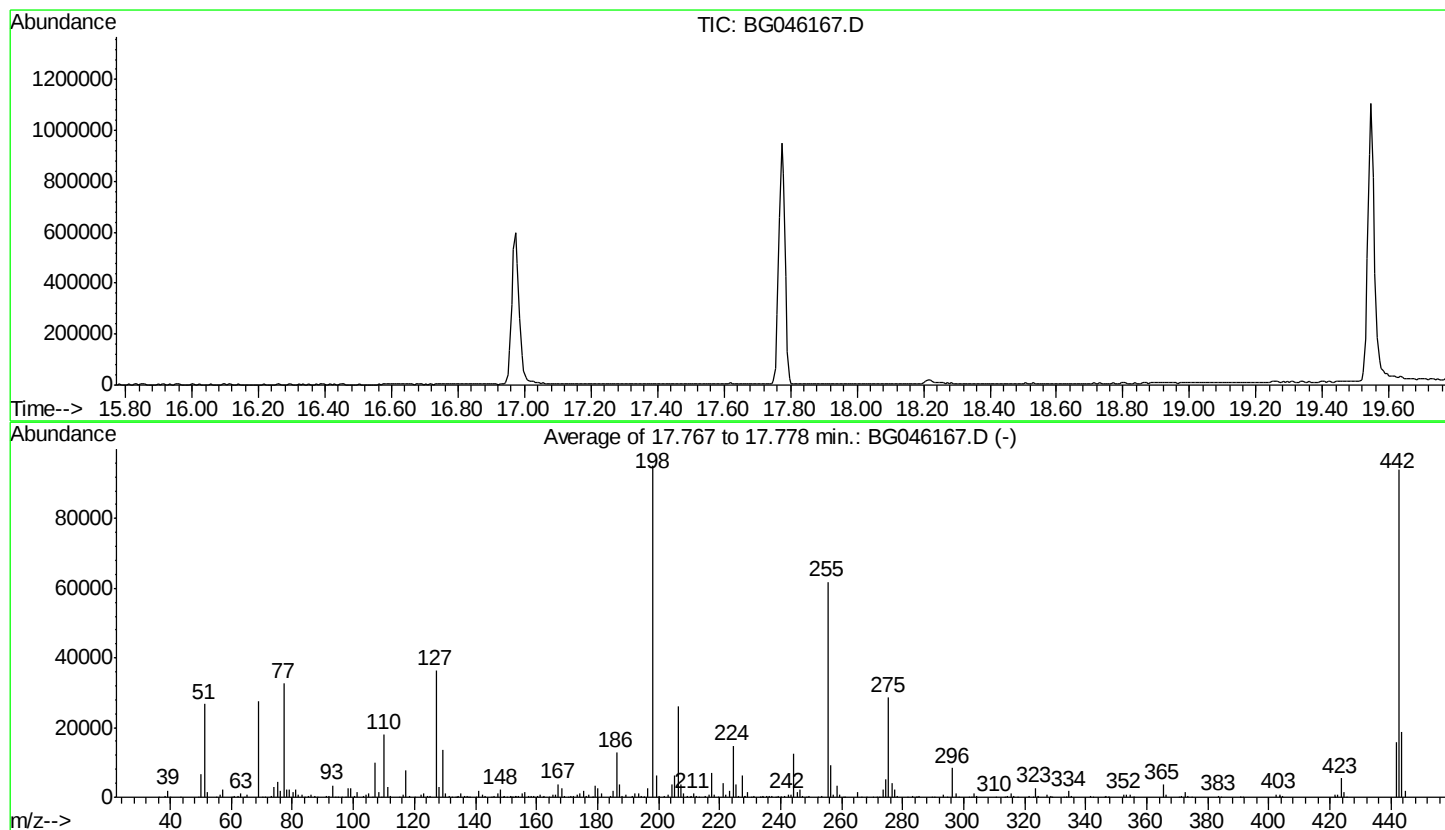

AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2492

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	26744	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	28.9	27525	PASS
70	69	0.00	2	0.6	155	PASS
127	198	10	80	38.1	36240	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	95186	PASS
199	198	5	9	6.5	6181	PASS
275	198	10	60	30.1	28616	PASS
365	198	1	100	3.7	3542	PASS
441	198	0.01	100	16.4	15656	PASS
442	198	50	100	99.0	94261	PASS
443	442	15	24	19.7	18595	PASS