

Data Path : Z:\HPCHEM1\BNA G\DATA\BG080717\
 Data File : BG028176.D
 Acq On : 8 Aug 2017 4:19
 Operator : SJ/JU
 Sample : PB101300BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Aug 08 07:44:47 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 08 03:54:28 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.36	152	41051	20.00	ng/ul	0.00
18) Naphthalene-d8	11.17	136	179887	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.96	164	130249	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.71	188	372705	20.00	ng/ul	0.00
75) Chrysene-d12	22.04	240	399905	20.00	ng/ul	0.00
83) Perylene-d12	25.55	264	379323	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.84	96	9527	10.81	ng/uL	0.00
5) Phenol-d5	7.50	99	119202	26.44	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.67	67	87982	30.81	ng/ul	0.00
9) 2-Chlorophenol-d4	7.89	132	89483	31.46	ng/ul	0.00
13) 4-Methylphenol-d8	9.05	113	100710	26.73	ng/ul	0.00
19) Nitrobenzene-d5	9.52	128	45591	32.41	ng/ul	0.00
22) 2-Nitrophenol-d4	10.25	143	54196	35.14	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.78	165	95106	29.80	ng/ul	0.00
29) 4-Chloroaniline-d4	11.30	131	131120	36.92	ng/ul	0.00
43) Dimethylphthalate-d6	14.35	166	424647	36.66	ng/ul	0.00
46) Acenaphthylene-d8	14.66	160	430651	32.97	ng/ul	0.00
51) 4-Nitrophenol-d4	15.15	143	58672	31.85	ng/ul	0.00
57) Fluorene-d10	15.96	176	341035	32.81	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.07	200	75192	31.06	ng/ul	0.00
70) Anthracene-d10	17.81	188	624607	34.95	ng/ul	0.00
76) Pyrene-d10	20.09	212	730629	35.63	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.31	264	620708	34.95	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	9.05	70	3184	1.042	ng/ul# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG080717\
Data File : BG028176.D
Acq On : 8 Aug 2017 4:19
Operator : SJ/JU
Sample : PB101300BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Aug 08 07:44:47 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 08 03:54:28 2017
Response via : Initial Calibration

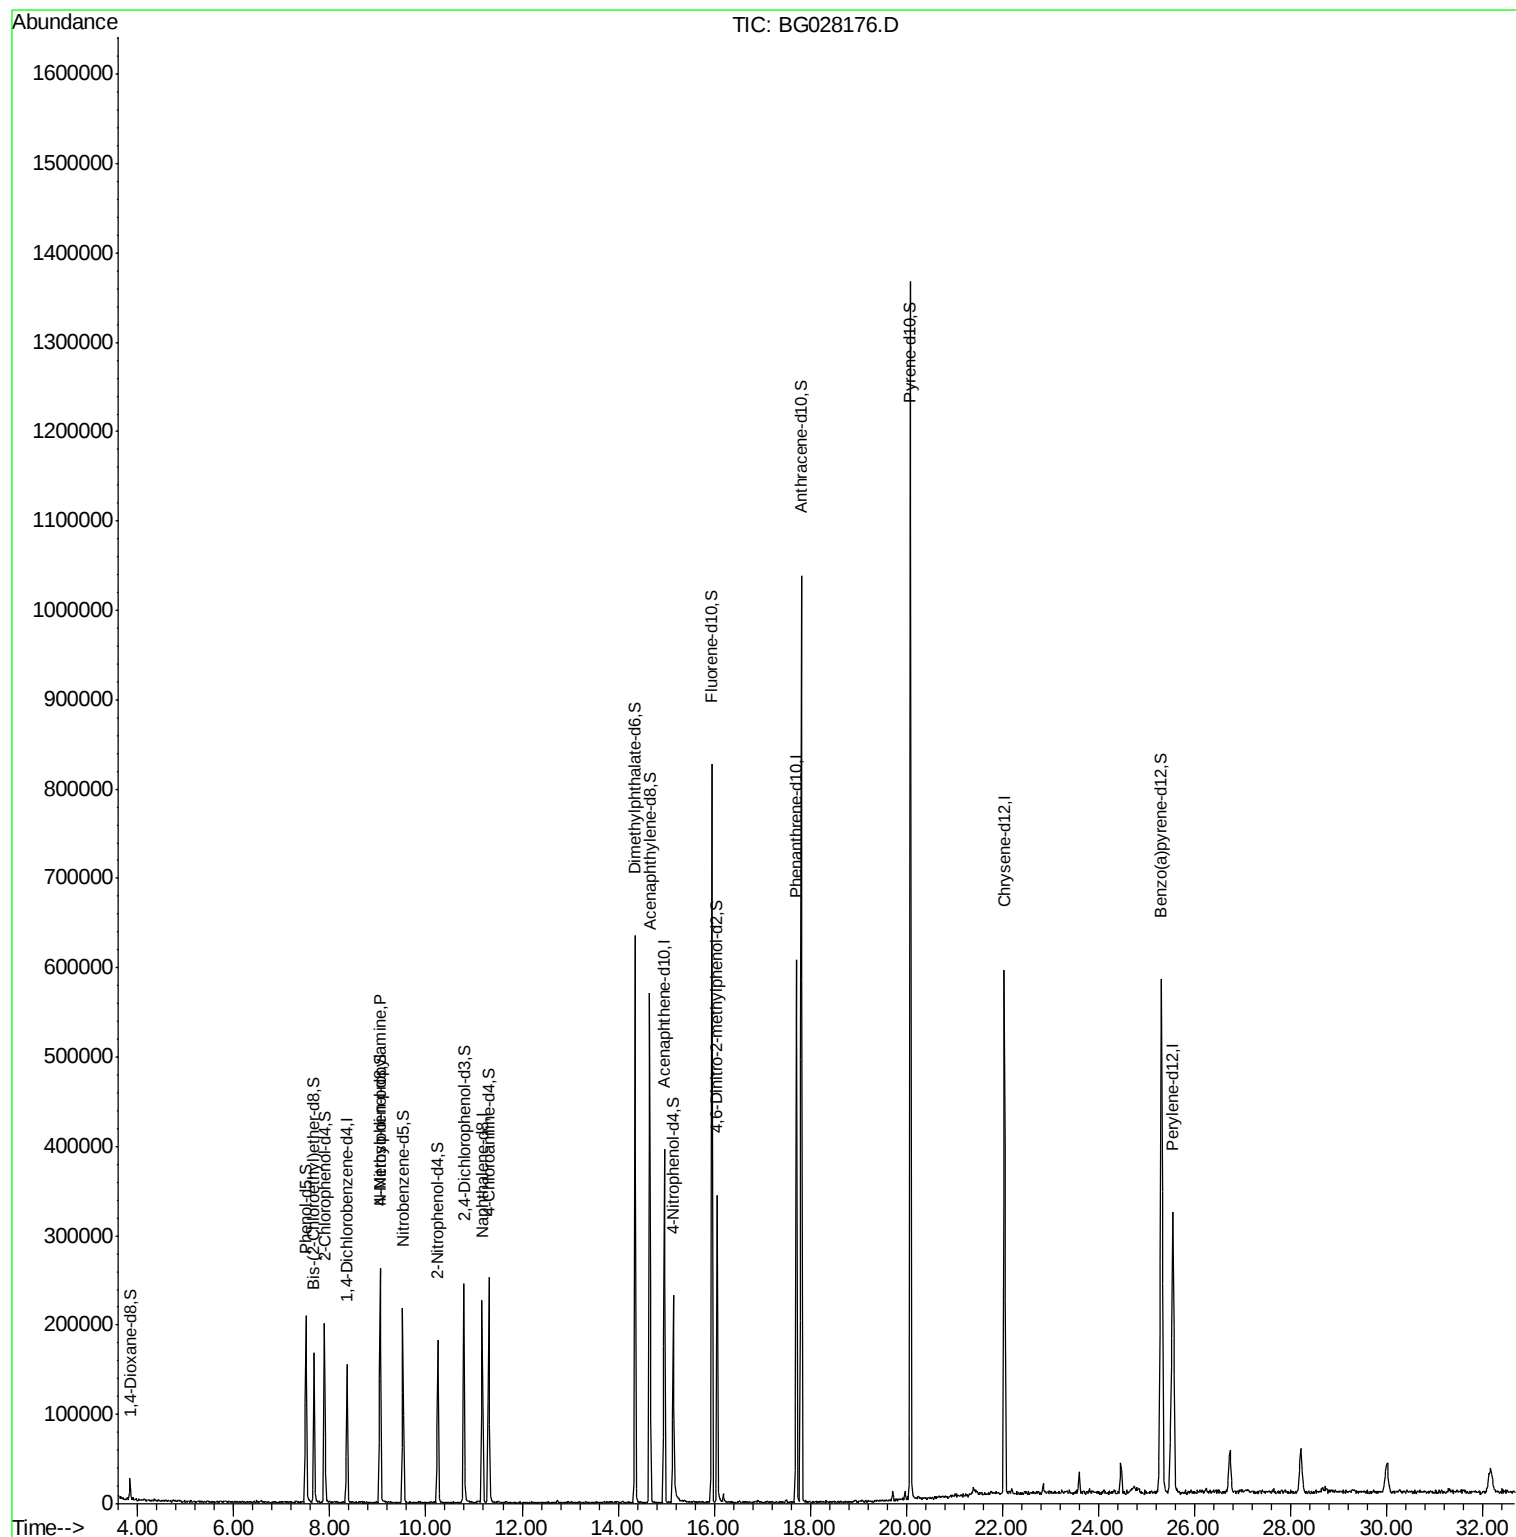

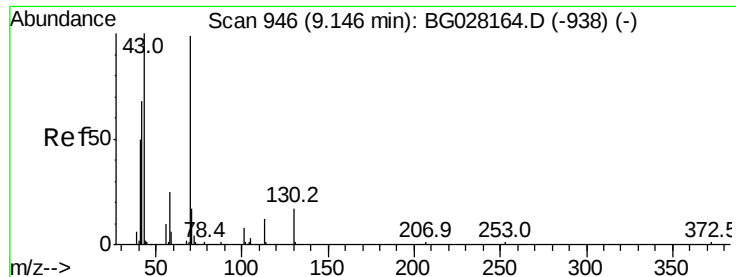

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.042 ng/ul
 RT: 9.05 min Scan# 929
 Delta R.T. -0.10 min
 Lab File: BG028176.D
 Acq: 8 Aug 2017 4:19

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
70	100		
42	343.1	59.0	88.6#
101	0.0	6.6	9.8#
130	0.0	15.6	23.4#

