
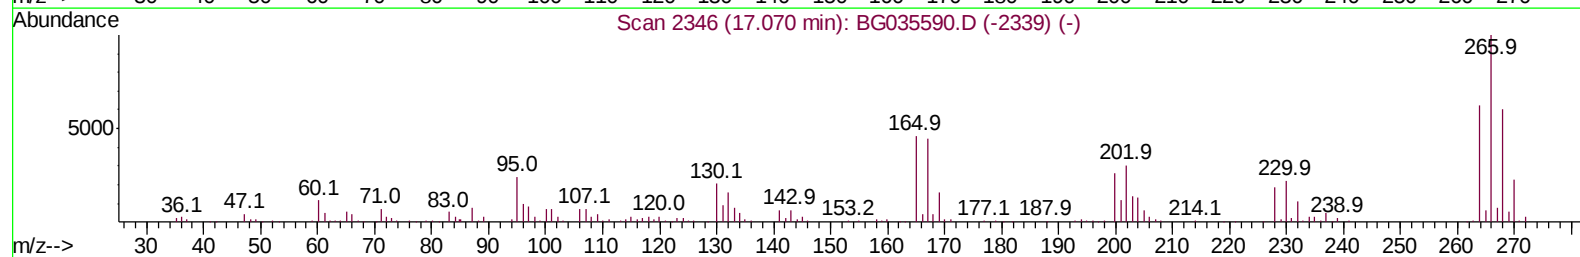
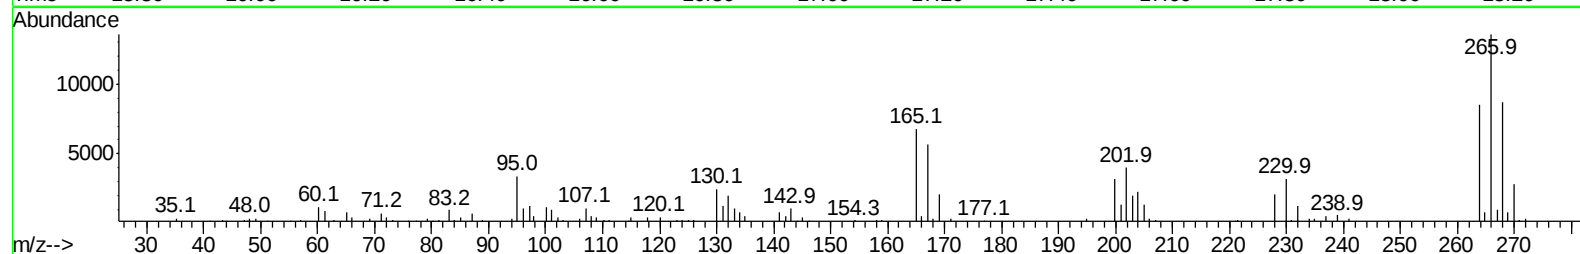


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG080718\
Data File : BG036163.D
Acq On : 7 Aug 2018 15:46
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 08 05:14:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

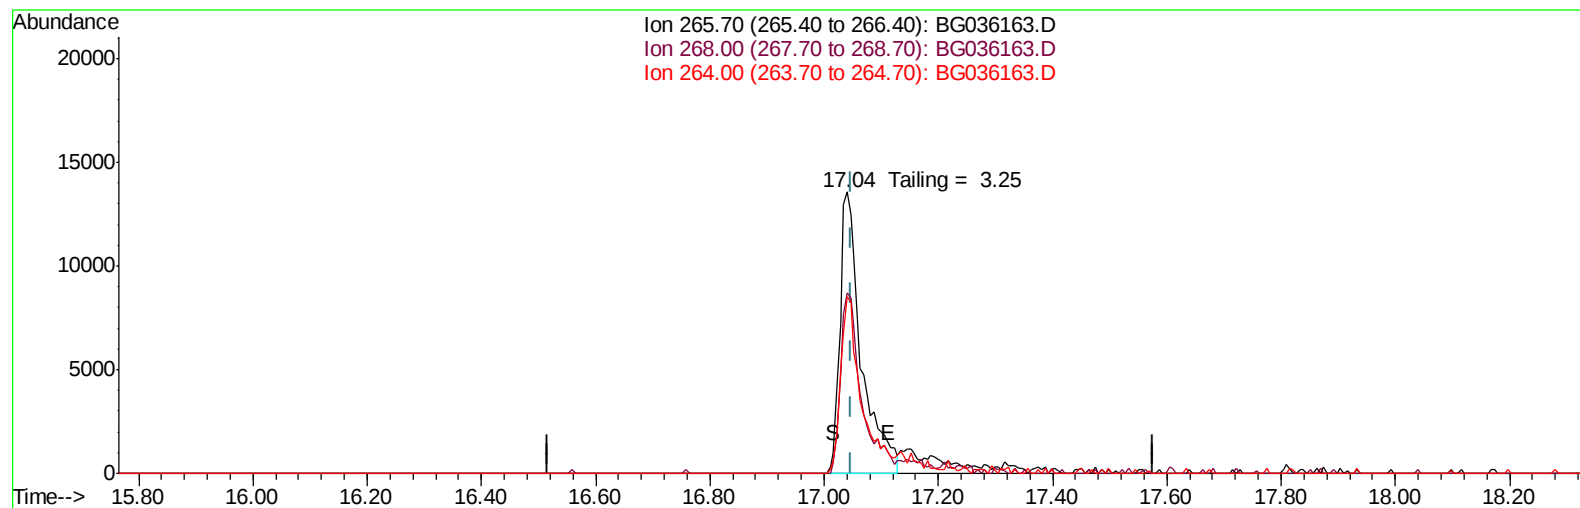

TIC: BG036163.D

(69) Pentachlorophenol (C)




17.040min (-0.007) 86373.18ng

response 35199

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.27
264.00	62.00	62.82
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG080718\
Data File : BG036163.D
Acq On : 7 Aug 2018 15:46
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 08 05:14:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

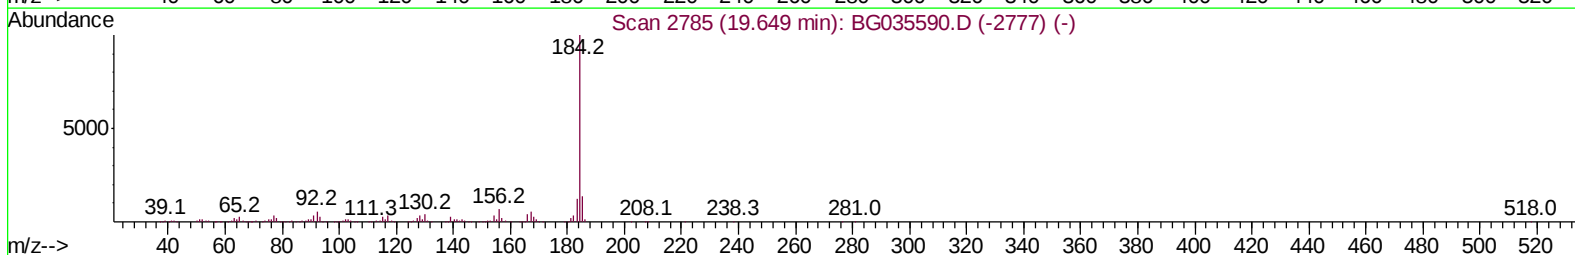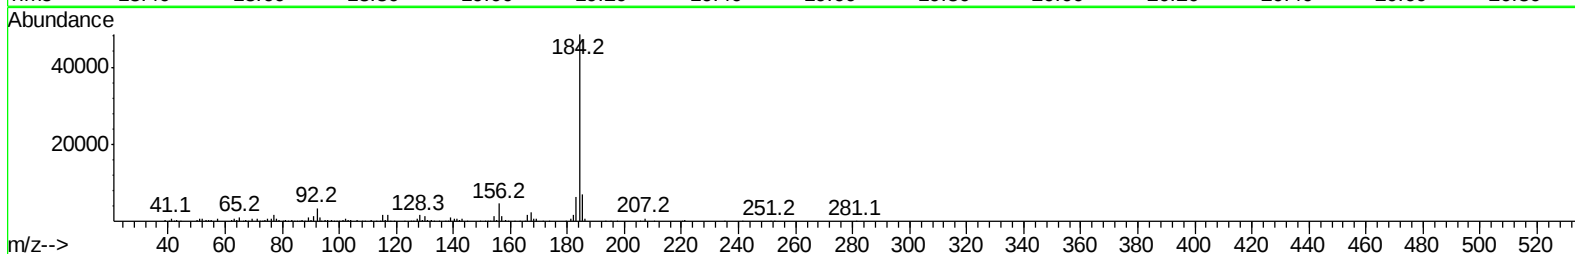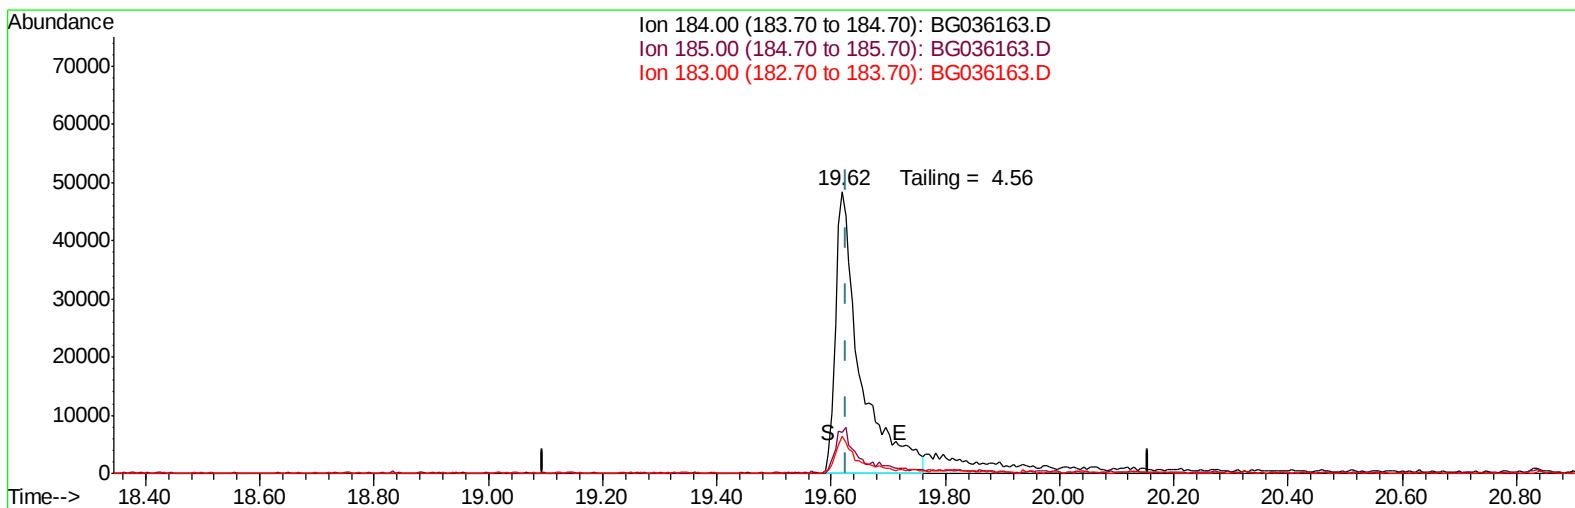

TIC: BG036163.D

(76) Benzidine

19.619min (-0.007) 86268.30ng

response 145153

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.62
183.00	13.30	13.19
0.00	0.00	0.00