
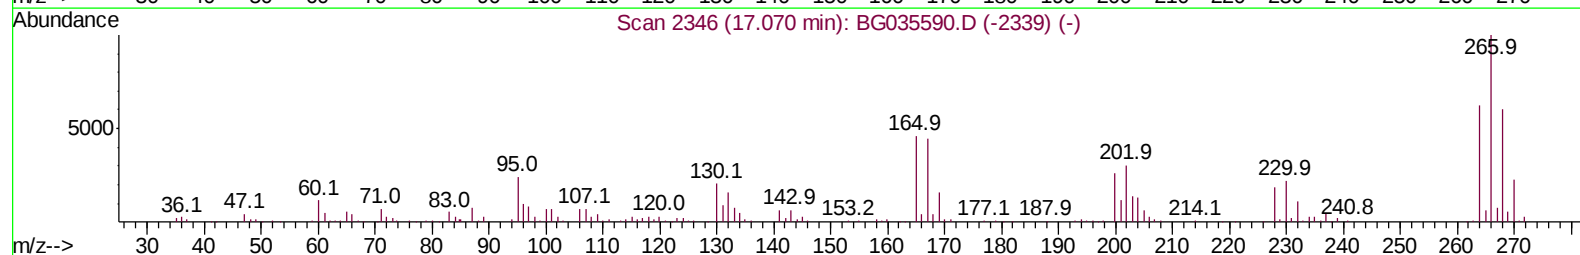
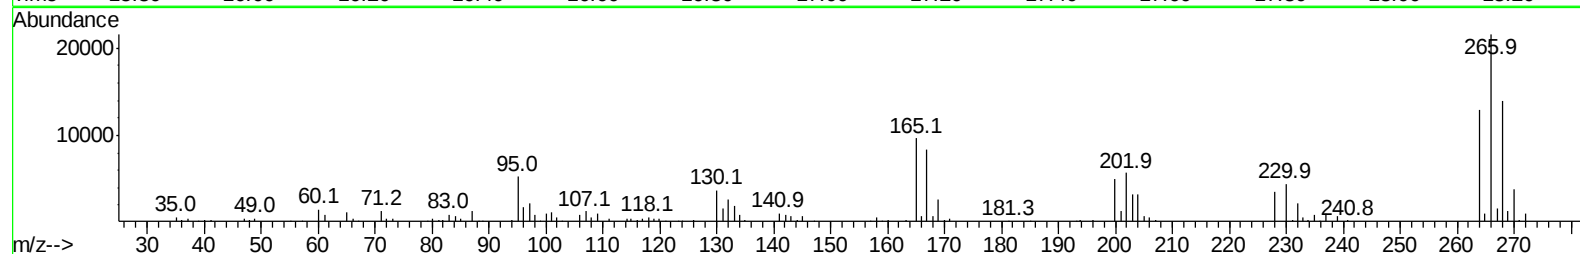


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080718\
Data File : BG036182.D
Acq On : 8 Aug 2018 4:53
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 08 05:30:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 31 12:30:06 2018
Response via : Initial Calibration

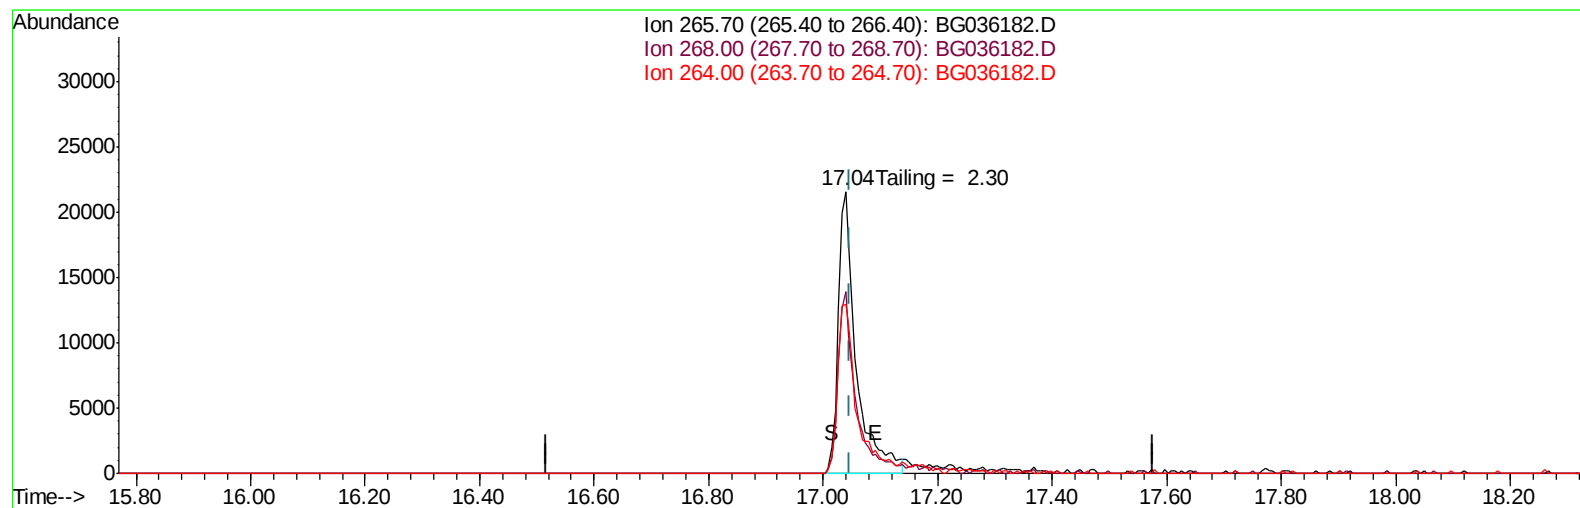

TIC: BG036182.D

(69) Pentachlorophenol (C)




17.039min (-0.009) 15577.98ng

response 47046

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.53
264.00	62.00	59.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080718\
 Data File : BG036182.D
 Acq On : 8 Aug 2018 4:53
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 08 05:30:05 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 31 12:30:06 2018
 Response via : Initial Calibration

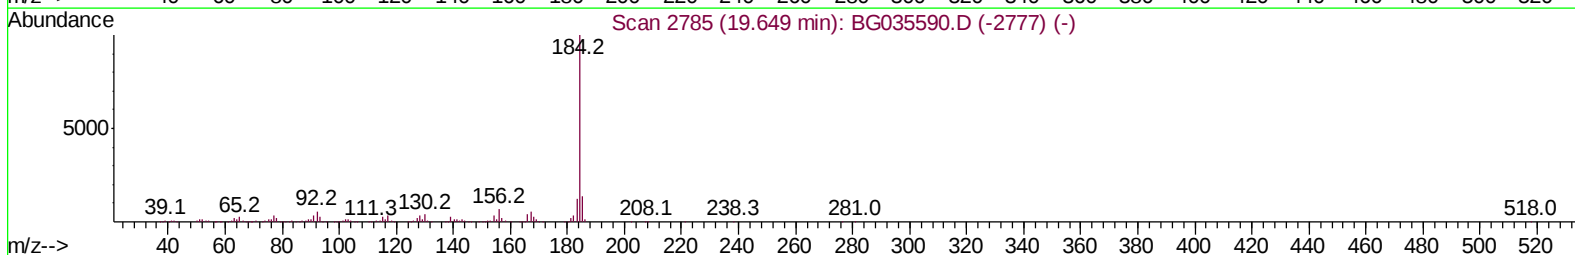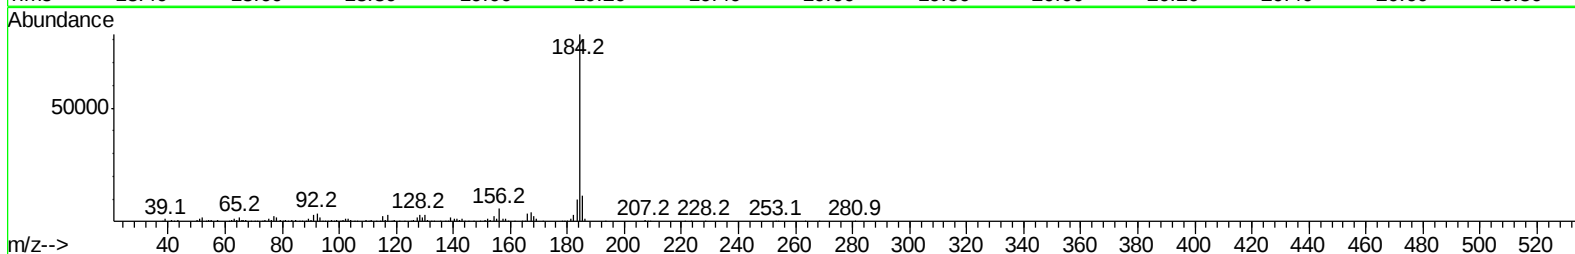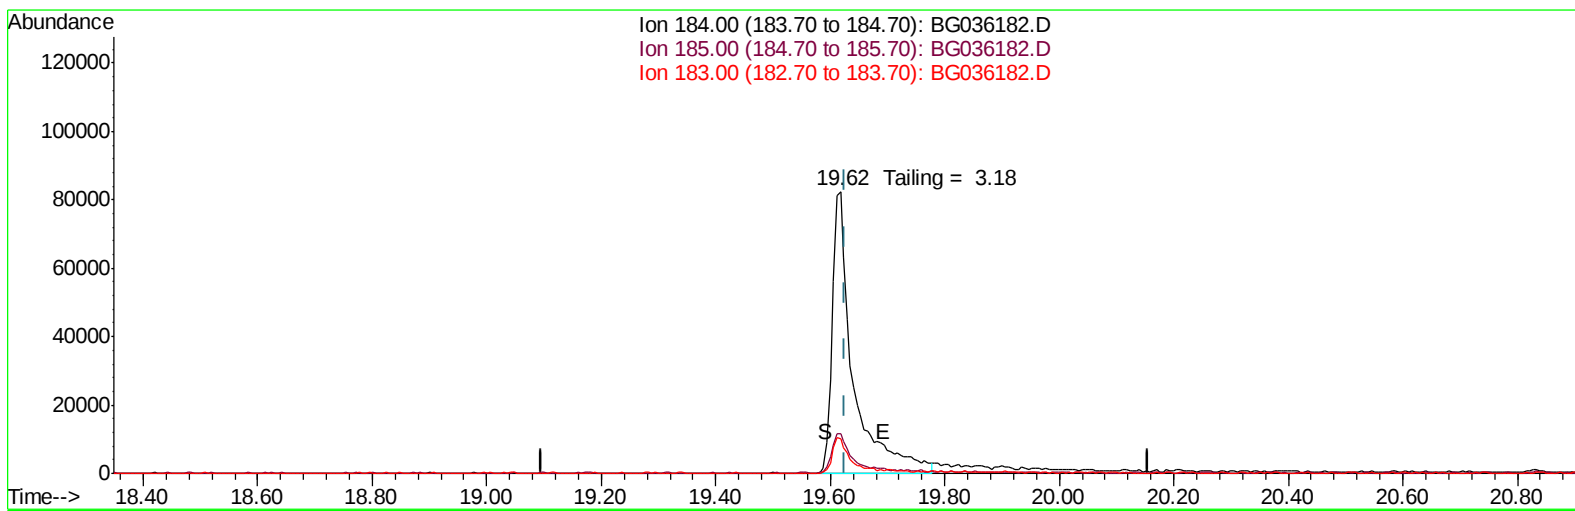

TIC: BG036182.D

(76) Benzidine

19.618min (-0.009) 26446.95ng

response 210675

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.02
183.00	13.30	12.13
0.00	0.00	0.00