


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG080718\
 Data File : BG036163.D
 Acq On : 7 Aug 2018 15:46
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 31 12:30:06 2018

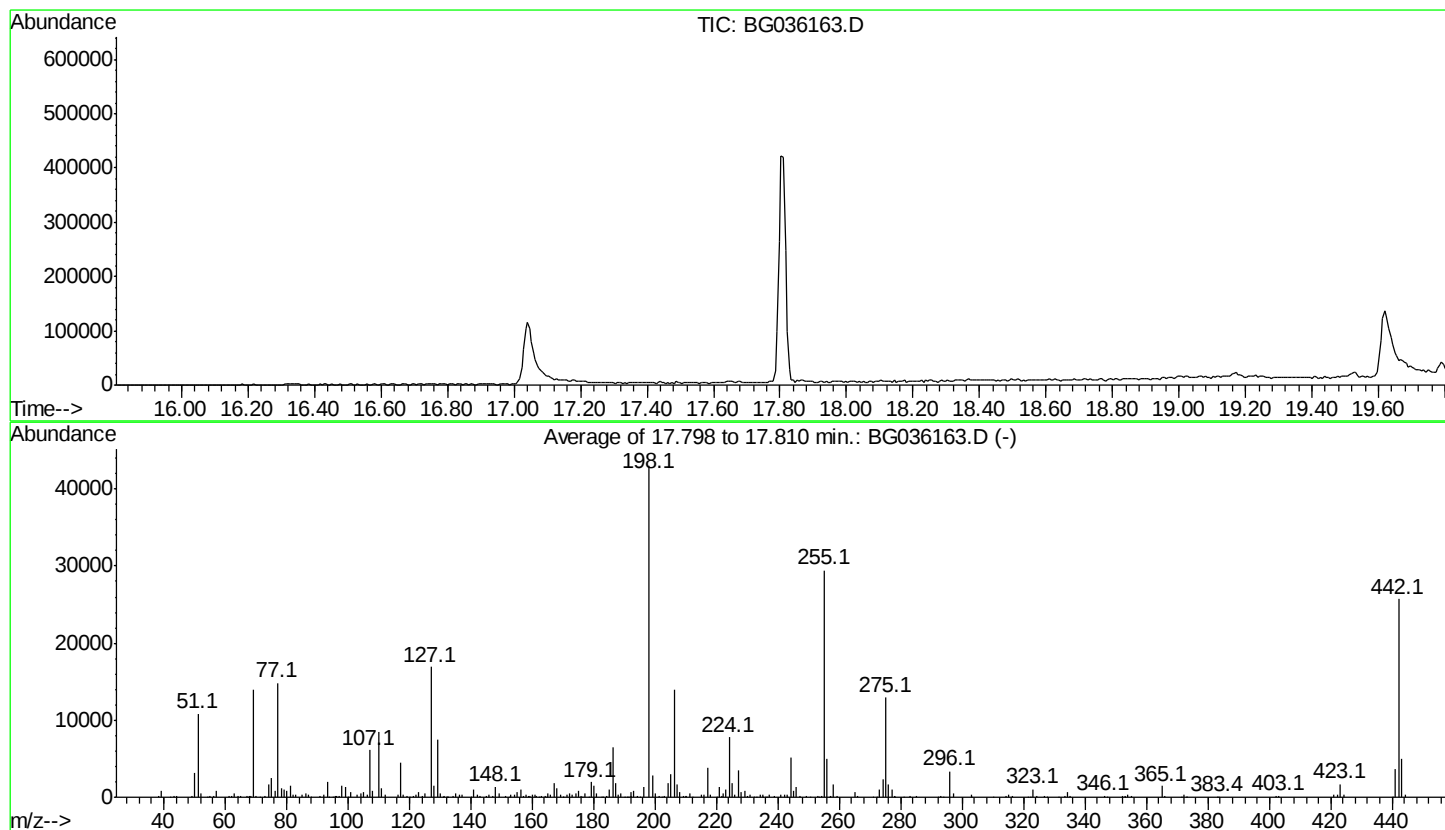

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.2	10858	PASS
68	69	0.00	2	1.4	197	PASS
69	198	0.00	100	32.5	13984	PASS
70	69	0.00	2	0.9	130	PASS
127	198	10	80	39.2	16870	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	43032	PASS
199	198	5	9	6.6	2844	PASS
275	198	10	60	29.9	12881	PASS
365	198	1	100	3.4	1481	PASS
441	198	0.01	100	8.6	3713	PASS
442	198	50	100	59.8	25724	PASS
443	442	15	24	19.5	5008	PASS