


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080718\
 Data File : BG036182.D
 Acq On : 8 Aug 2018 4:53
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG071218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 31 12:30:06 2018

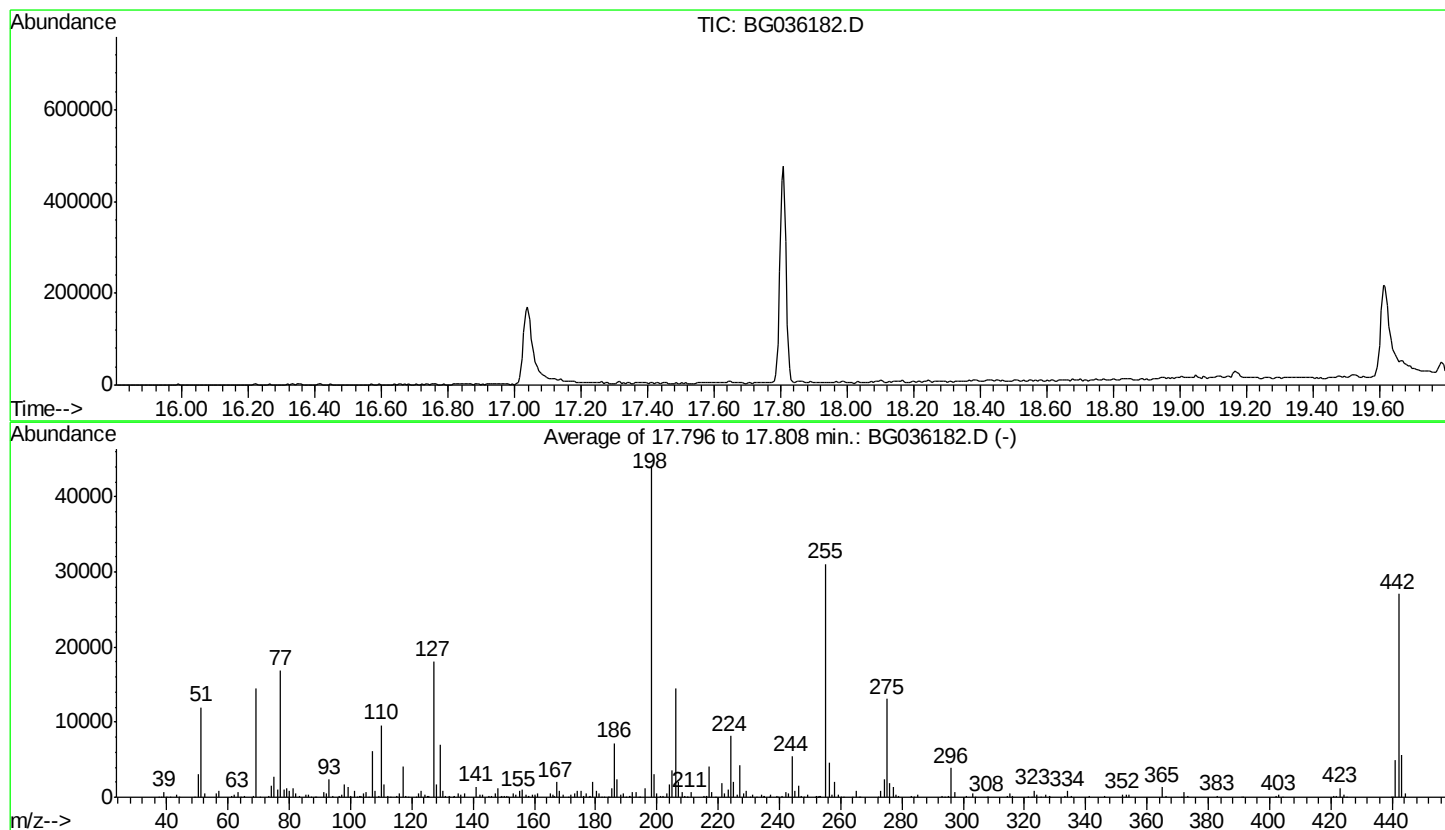

Spectrum Information: Average of 17.796 to 17.808 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.0	11948	PASS
68	69	0.00	2	0.8	119	PASS
69	198	0.00	100	32.8	14484	PASS
70	69	0.00	2	0.5	68	PASS
127	198	10	80	40.8	18034	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	44181	PASS
199	198	5	9	7.1	3135	PASS
275	198	10	60	29.7	13122	PASS
365	198	1	100	3.0	1343	PASS
441	198	0.01	100	11.2	4958	PASS
442	198	50	100	61.2	27059	PASS
443	442	15	24	20.7	5605	PASS