

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG080720\
 Data File : BG046192.D
 Acq On : 7 Aug 2020 14:10
 Operator : CG/JU
 Sample : PB130804BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB130804BL

Quant Time: Aug 07 17:22:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 30 18:43:49 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.95	152	111417	20.00	ng	0.00
21) Naphthalene-d8	10.75	136	422882	20.00	ng	0.00
39) Acenaphthene-d10	14.57	164	274266	20.00	ng	0.00
64) Phenanthrene-d10	17.32	188	646721	20.00	ng	0.00
76) Chrysene-d12	21.56	240	822937	20.00	ng	-0.01
86) Perylene-d12	24.67	264	820277	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.54	112	699934	109.21	ng	0.00
7) Phenol-d6	7.12	99	888318	101.70	ng	0.00
23) Nitrobenzene-d5	9.10	82	588626	75.36	ng	0.00
42) 2,4,6-Tribromophenol	16.06	330	485643	115.28	ng	0.00
45) 2-Fluorobiphenyl	13.20	172	1462447	77.46	ng	0.00
79) Terphenyl-d14	19.93	244	2415545	59.78	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.10	70	74401	13.087	ng	# 76
51) 2,6-Dinitrotoluene	14.57	165	36344	7.419	ng	# 28
57) 2,4-Dinitrotoluene	14.57	165	36344	5.396	ng	# 27
67) 4-Bromophenyl-phenylether	16.06	248	29635	3.709	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG080720\
Data File : BG046192.D
Acq On : 7 Aug 2020 14:10
Operator : CG/JU
Sample : PB130804BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB130804BL

Quant Time: Aug 07 17:22:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 30 18:43:49 2020
Response via : Initial Calibration

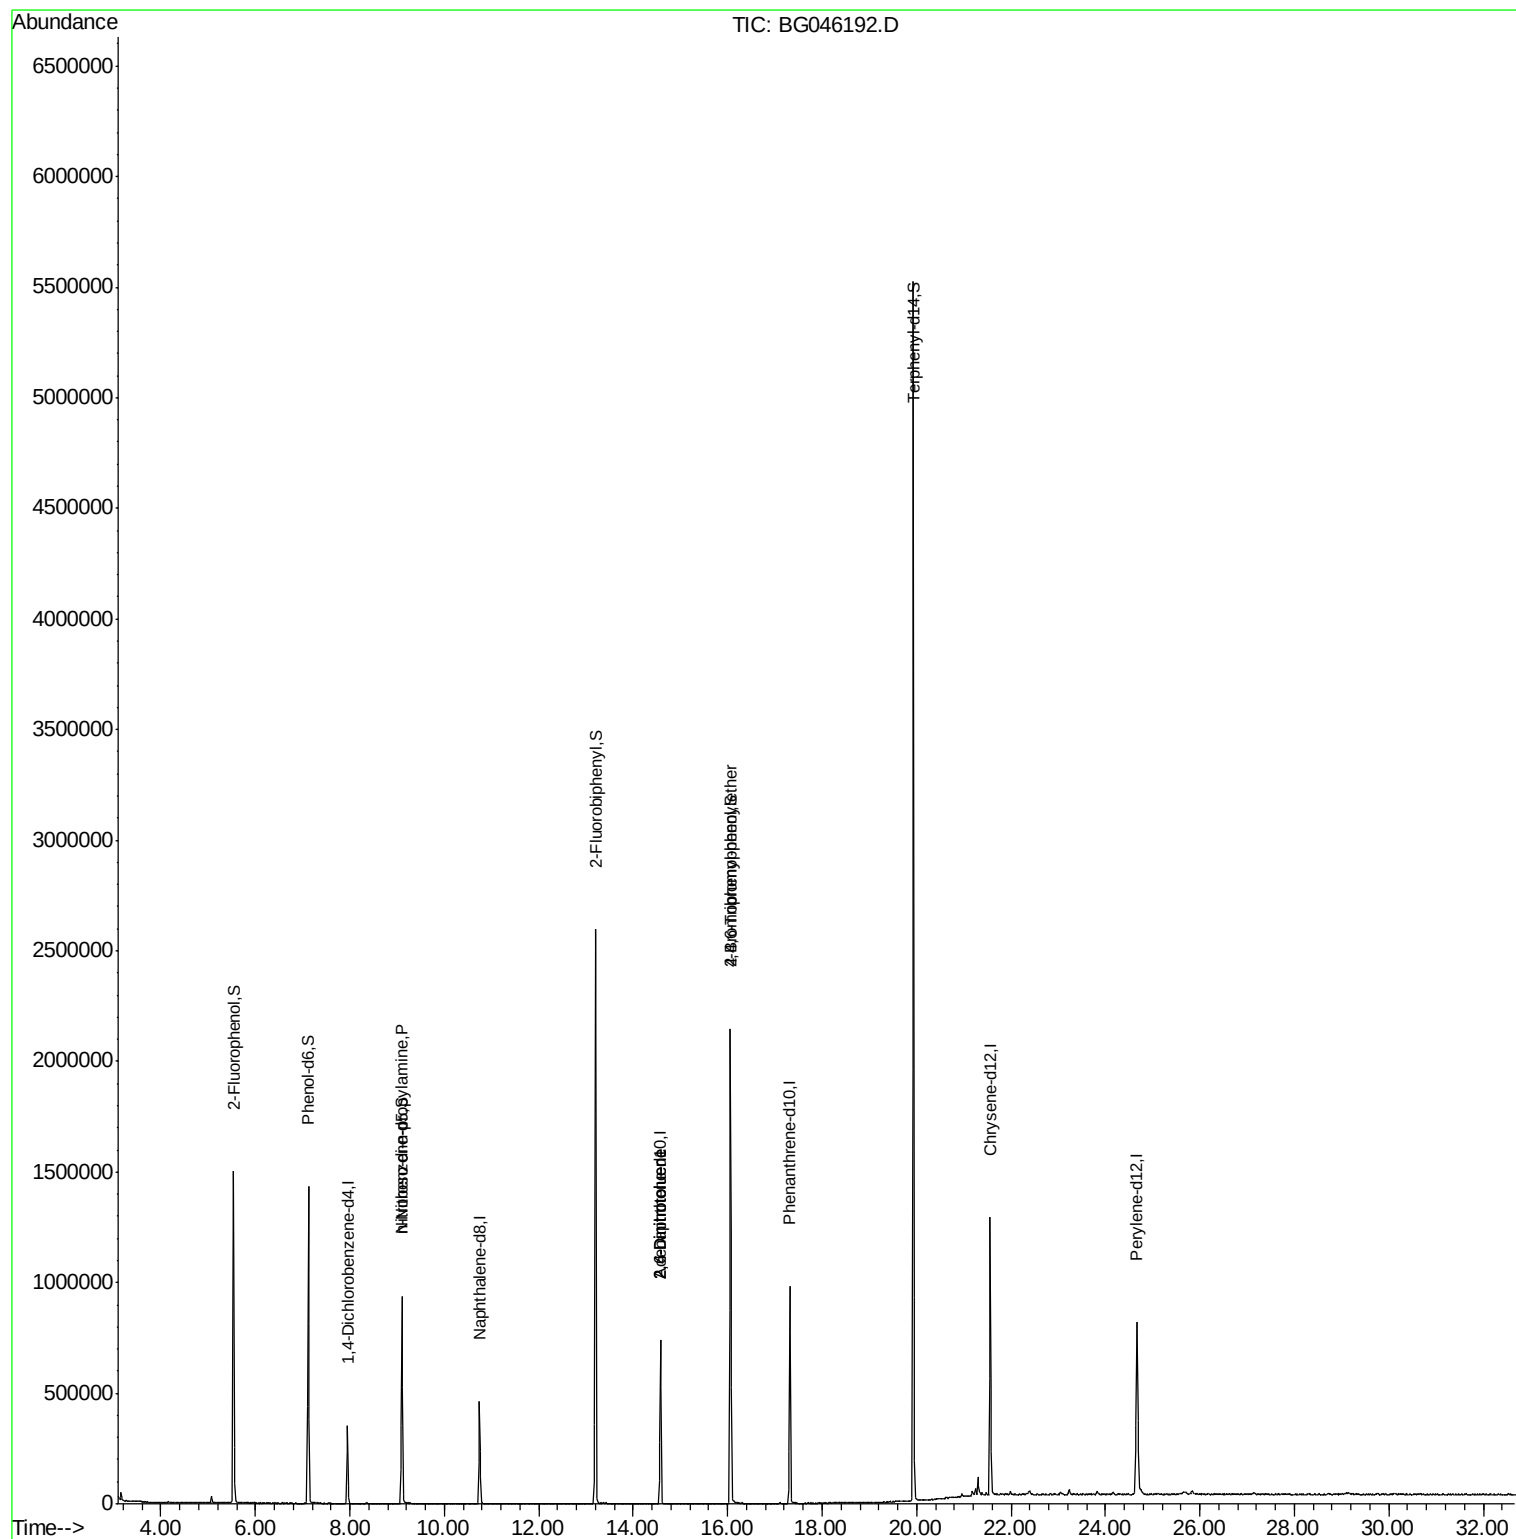

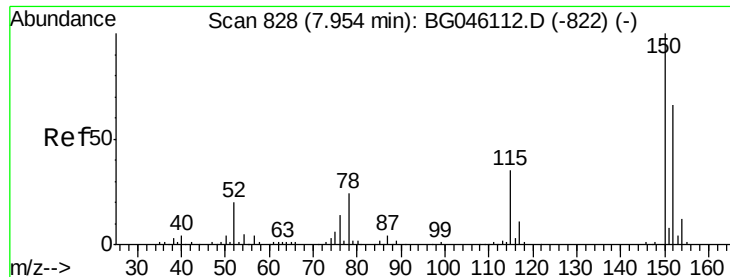


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.95 min Scan# 828
Delta R.T. -0.00 min
Lab File: BG046192.D
Acq: 7 Aug 2020 14:10

Instrument :
BNA_G
ClientSampleId :
PB130804BL

Tot Ion:152 Resp: 111417
Ion Ratio Lower Upper
152 100
150 151.9 122.1 183.1
115 52.1 43.2 64.8

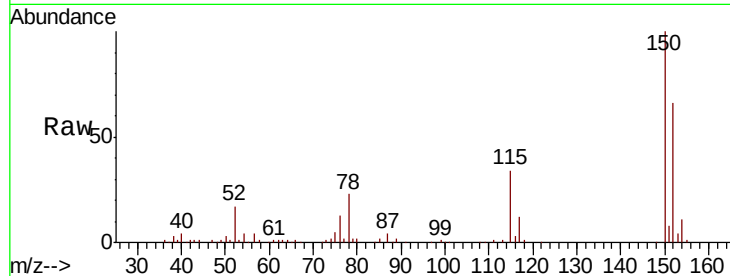


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

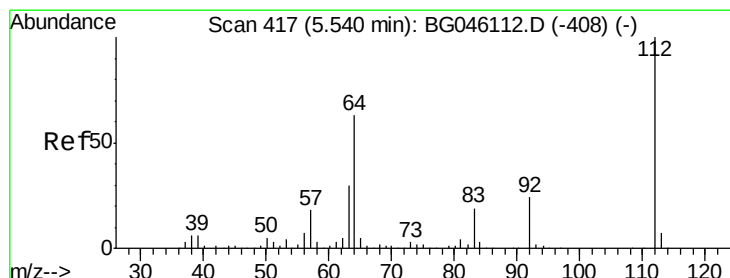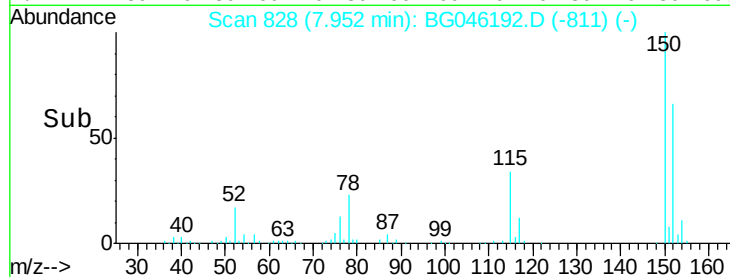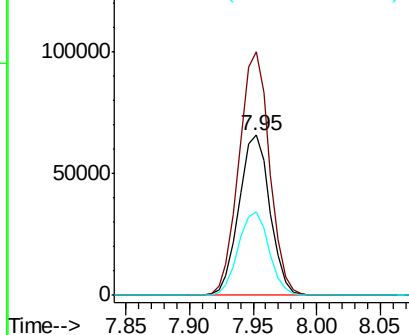



#5


2-Fluorophenol
Concen: 109.206 ng
RT: 5.54 min Scan# 417
Delta R.T. -0.00 min
Lab File: BG046192.D
Acq: 7 Aug 2020 14:10

Tgt Ion:112 Resp: 699934
Ion Ratio Lower Upper
112 100
64 60.4 50.2 75.2
63 29.5 24.2 36.4

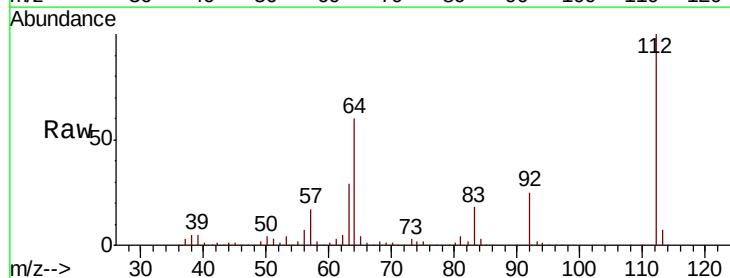

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

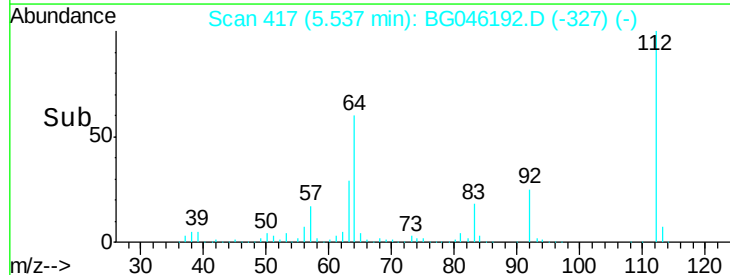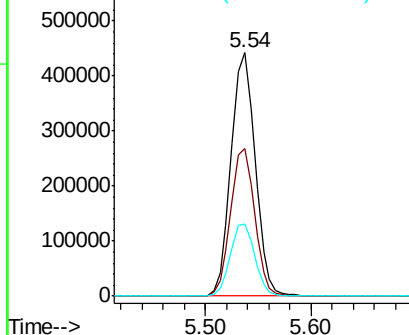

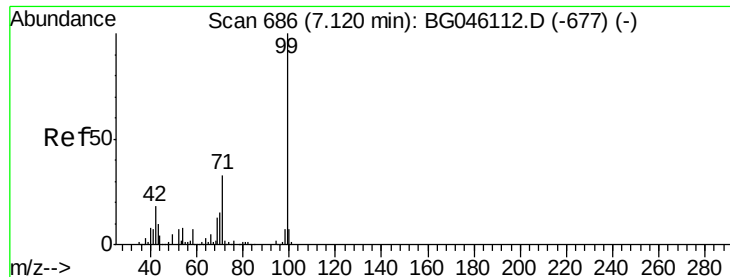

#7

Phenol-d6

Concen: 101.697 ng

RT: 7.12 min Scan# 686

Delta R.T. -0.00 min

Lab File: BG046192.D

Acq: 7 Aug 2020 14:10

Instrument :

BNA_G

ClientSampleId :

PB130804BL





Tot Ion: 99 Resp: 888318

Ion Ratio Lower Upper

99 100

42 16.9 14.7 22.1

71 31.4 26.5 39.7

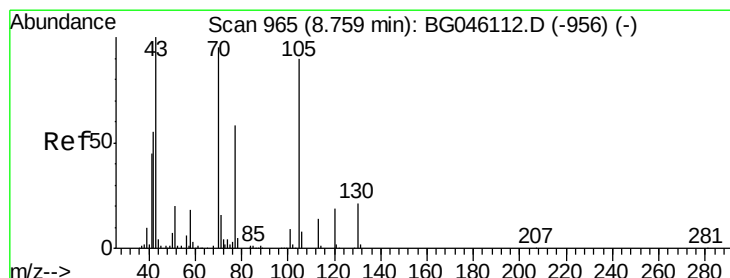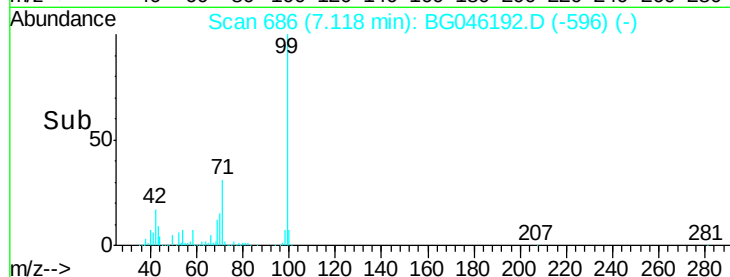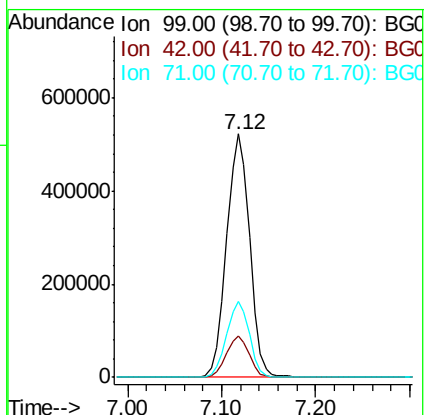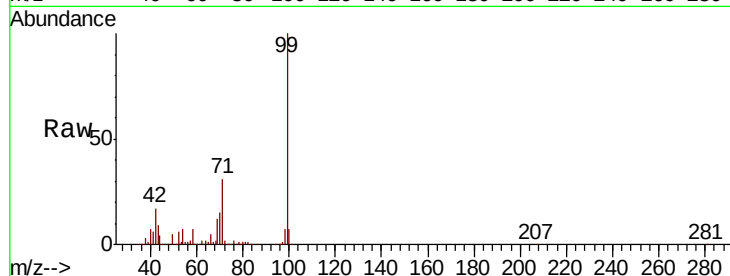

#19

n-Nitroso-di-n-propylamine

Concen: 13.087 ng

RT: 9.10 min Scan# 1024

Delta R.T. 0.34 min

Lab File: BG046192.D

Acq: 7 Aug 2020 14:10

Tgt Ion: 70 Resp: 74401




Ion Ratio Lower Upper


70 100

42 45.6 46.5 69.7#

101 0.0 7.6 11.4#

130 2.4 17.3 25.9#

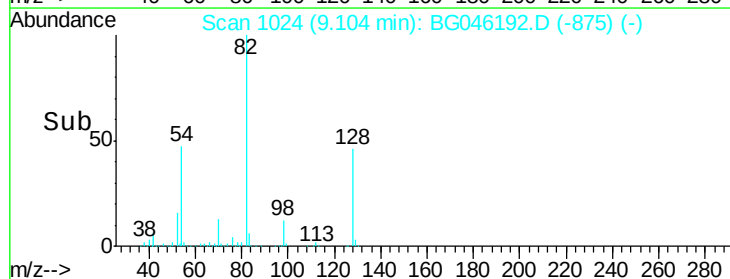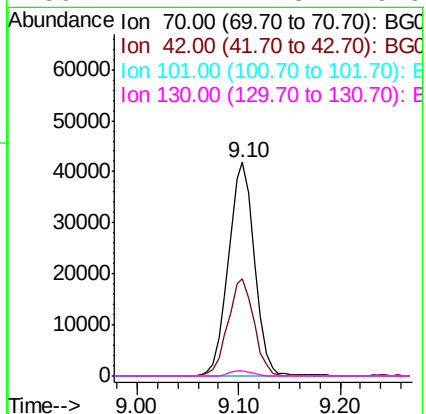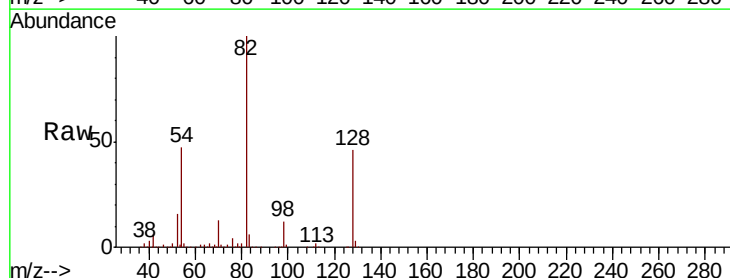


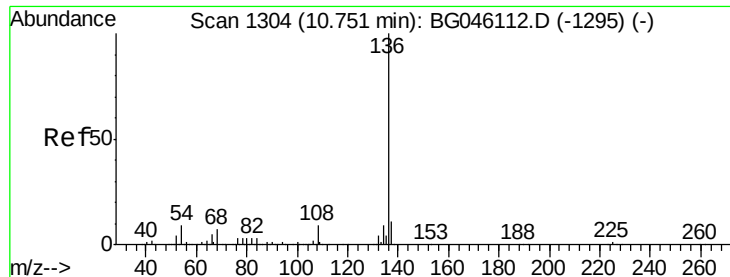




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.75 min Scan# 1304
Delta R.T. -0.00 min
Lab File: BG046192.D
Acq: 7 Aug 2020 14:10

Instrument :
BNA_G
ClientSampleId :
PB130804BL

Tot Ion:136	Resp:	422882
Ion	Ratio	Lower Upper
136	100	
137	10.7	8.8 13.2
54	8.0	7.0 10.4
68	5.9	5.3 7.9

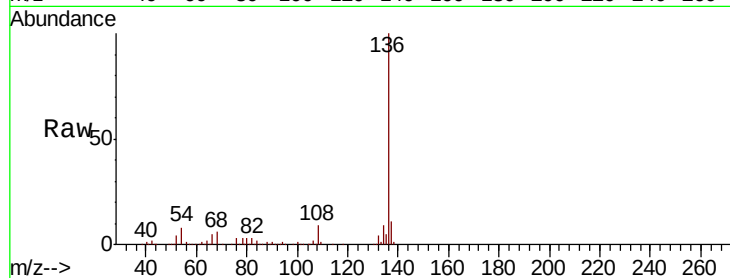


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

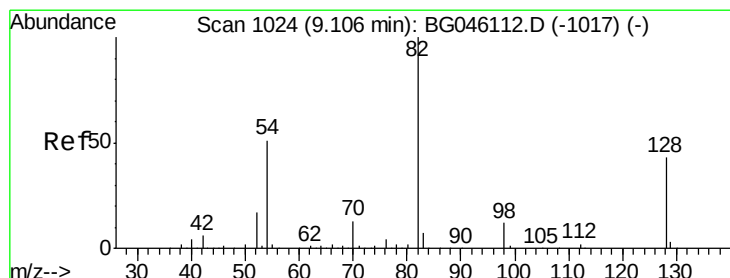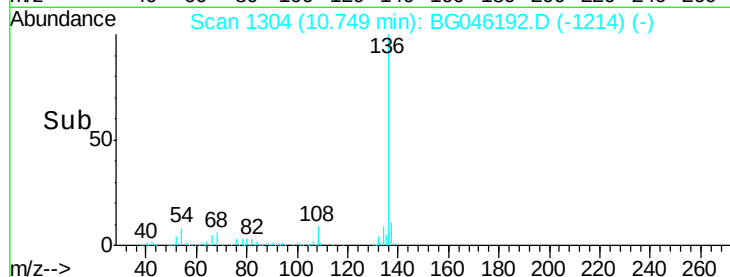
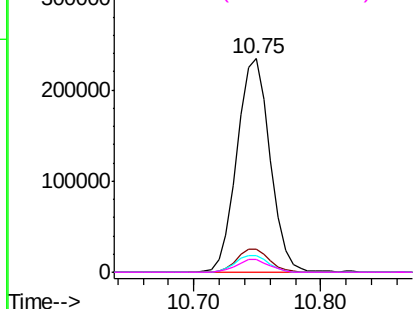



#23
Nitrobenzene-d5
Concen: 75.363 ng
RT: 9.10 min Scan# 1024
Delta R.T. -0.00 min
Lab File: BG046192.D
Acq: 7 Aug 2020 14:10

Tgt Ion: 82	Resp:	588626
Ion	Ratio	Lower Upper
82	100	
128	45.7	34.4 51.6
54	47.2	40.8 61.2

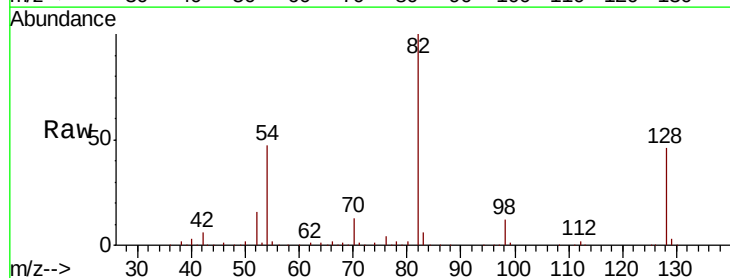

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

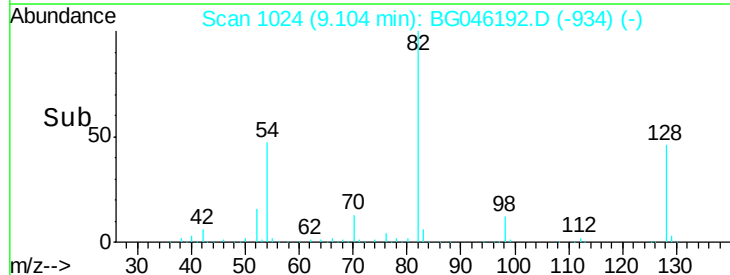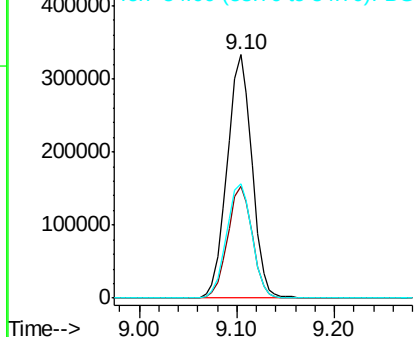

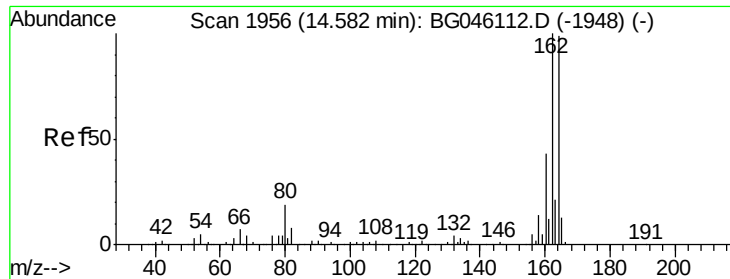

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.57 min Scan# 1955

Delta R.T. -0.01 min

Lab File: BG046192.D

Acq: 7 Aug 2020 14:10

Instrument :

BNA_G

ClientSampleId :

PB130804BL





Tot Ion:164 Resp: 274266

Ion Ratio Lower Upper

164 100

162 104.6 80.6 121.0

160 44.3 34.9 52.3

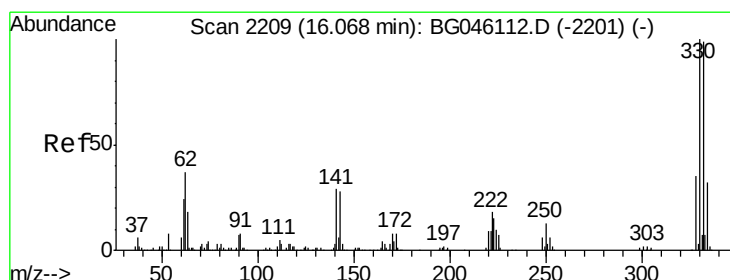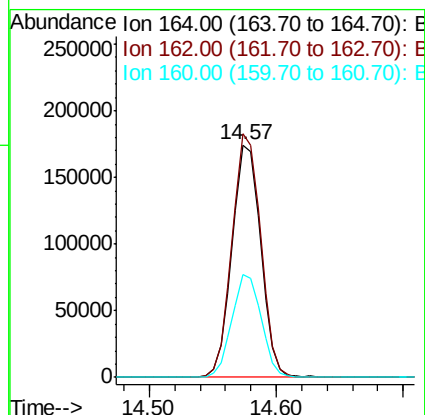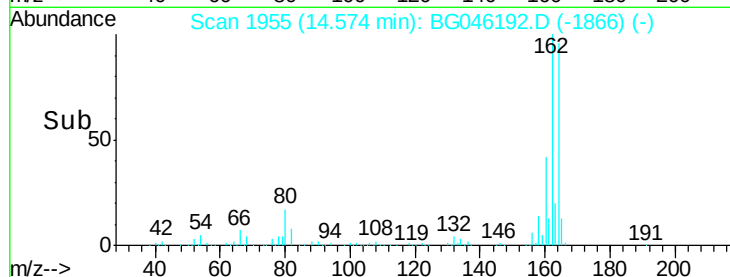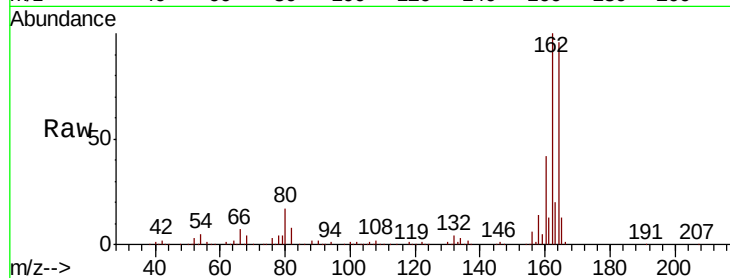

#42

2,4,6-Tribromophenol

Concen: 115.281 ng

RT: 16.06 min Scan# 2208

Delta R.T. -0.01 min

Lab File: BG046192.D

Acq: 7 Aug 2020 14:10




Tgt Ion:330 Resp: 485643


Ion Ratio Lower Upper

330 100

332 97.5 77.4 116.2

141 26.0 23.4 35.0

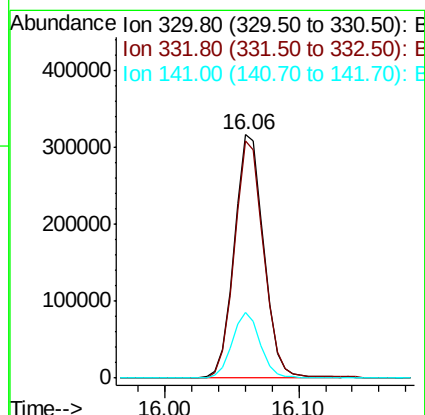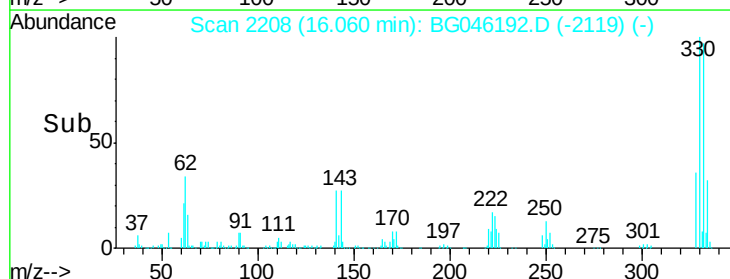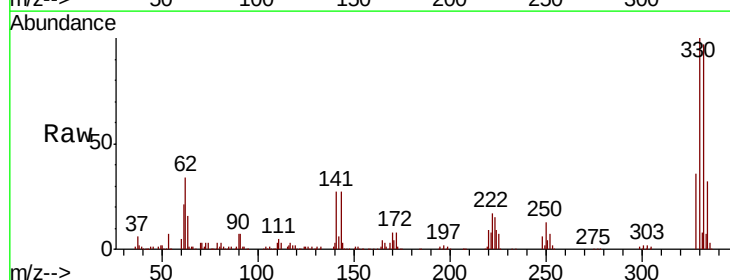


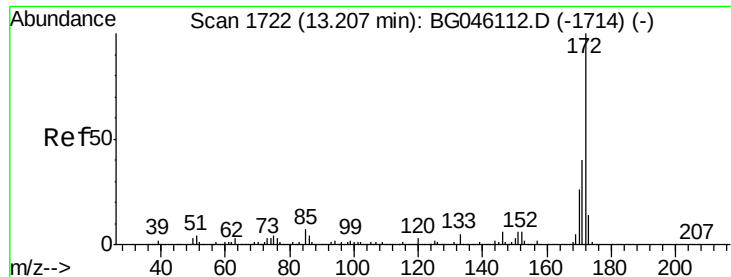




#45
 2-Fluorobiphenyl
 Concen: 77.458 ng
 RT: 13.20 min Scan# 1722
 Delta R.T. -0.00 min
 Lab File: BG046192.D
 Acq: 7 Aug 2020 14:10

Instrument :
 BNA_G
 ClientSampleId :
 PB130804BL

Tot Ion:172 Resp: 1462447
 Ion Ratio Lower Upper
 172 100
 171 39.8 31.7 47.5
 170 26.2 20.9 31.3

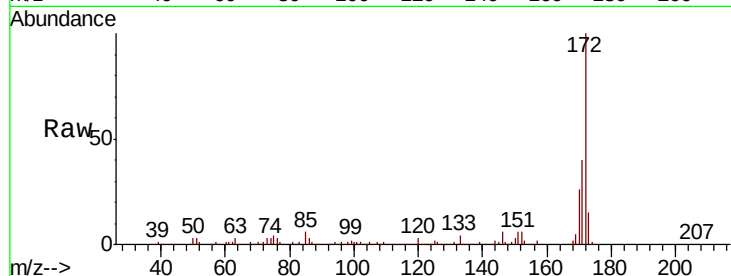


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

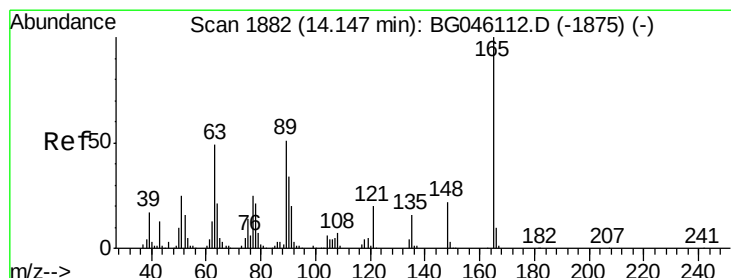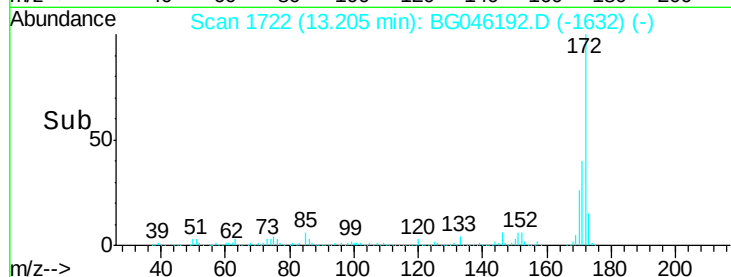
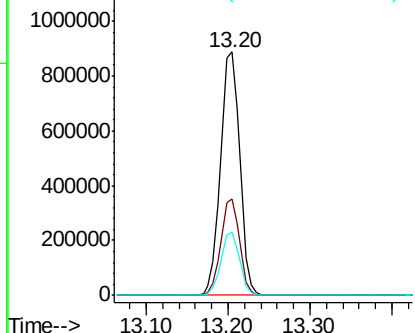



#51
 2,6-Dinitrotoluene
 Concen: 7.419 ng
 RT: 14.57 min Scan# 1955
 Delta R.T. 0.43 min
 Lab File: BG046192.D
 Acq: 7 Aug 2020 14:10

Tgt Ion:165 Resp: 36344
 Ion Ratio Lower Upper
 165 100
 63 0.7 39.7 59.5#
 89 0.0 41.0 61.6#

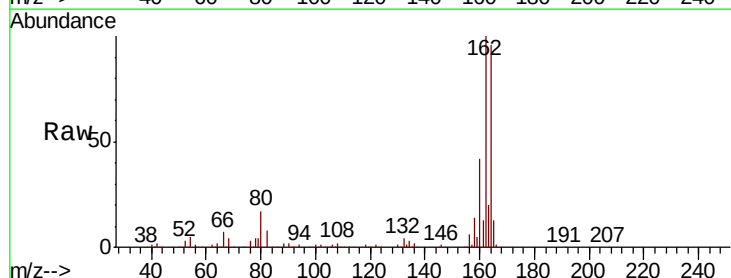

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BG0
 Ion 89.00 (88.70 to 89.70): BG0



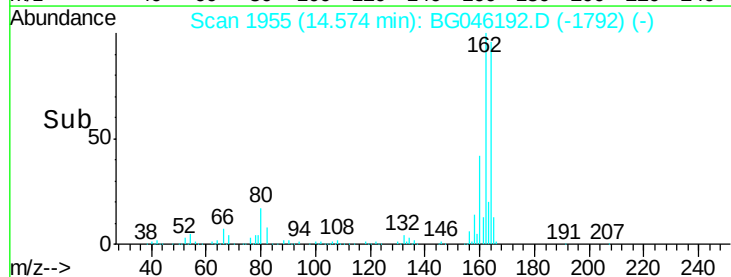
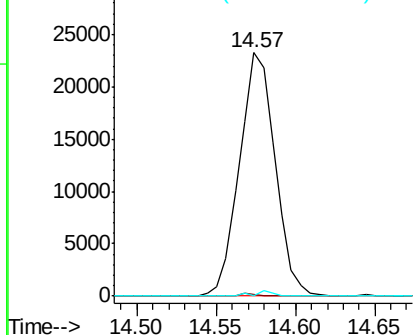


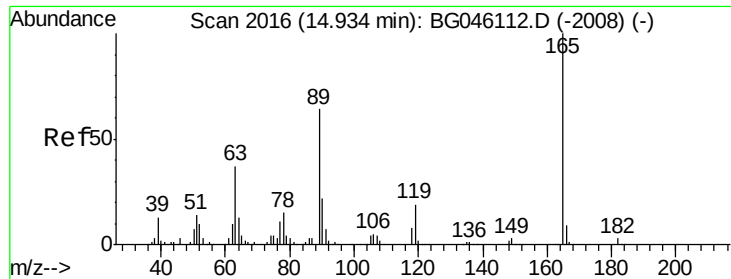

#57
 2,4-Dinitrotoluene
 Concen: 5.396 ng
 RT: 14.57 min Scan# 1955
 Delta R.T. -0.36 min
 Lab File: BG046192.D
 Acq: 7 Aug 2020 14:10




Instrument :
 BNA_G
 ClientSampleId :
 PB130804BL


Tot Ion:165 Resp: 36344
 Ion Ratio Lower Upper
 165 100
 63 0.7 30.1 45.1#
 89 0.0 51.4 77.2#
 182 0.0 2.3 3.5#

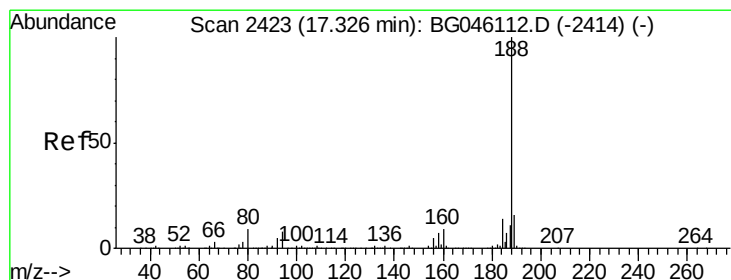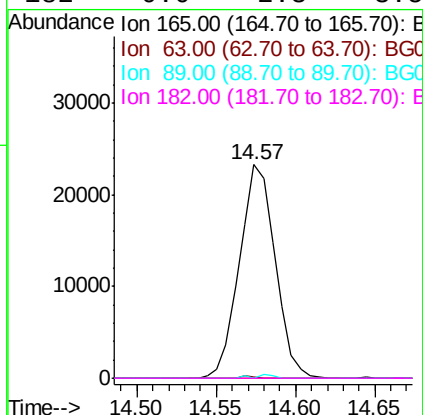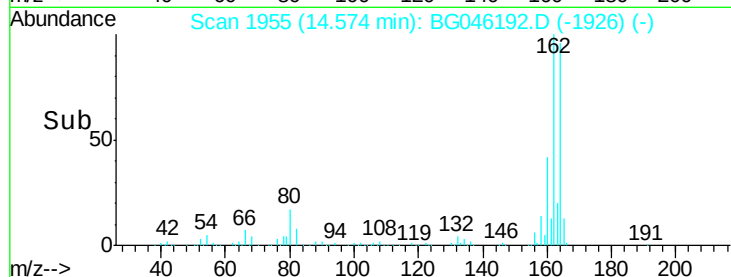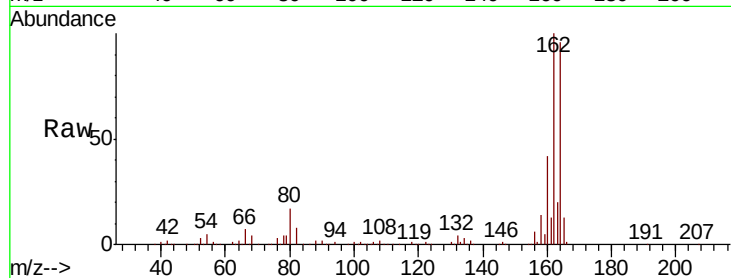

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.32 min Scan# 2422
 Delta R.T. -0.01 min
 Lab File: BG046192.D
 Acq: 7 Aug 2020 14:10

Tgt Ion:188 Resp: 646721
 Ion Ratio Lower Upper
 188 100
 94 8.2 6.4 9.6
 80 8.5 7.4 11.0

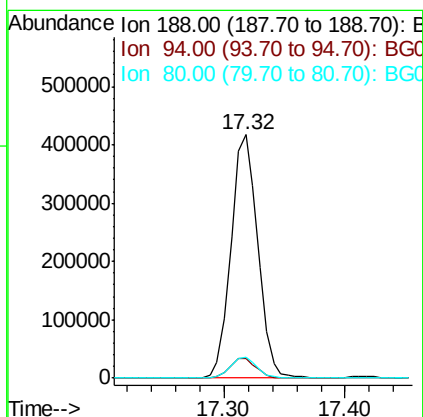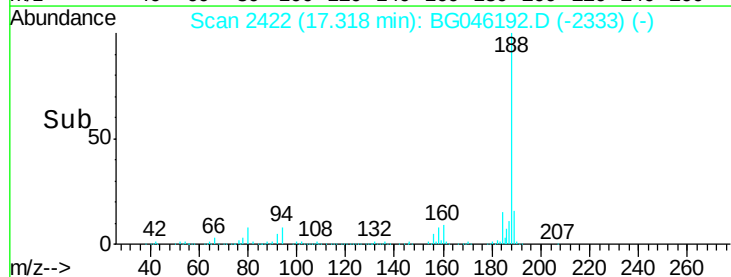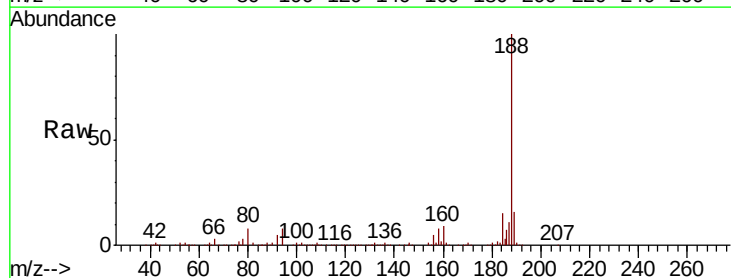


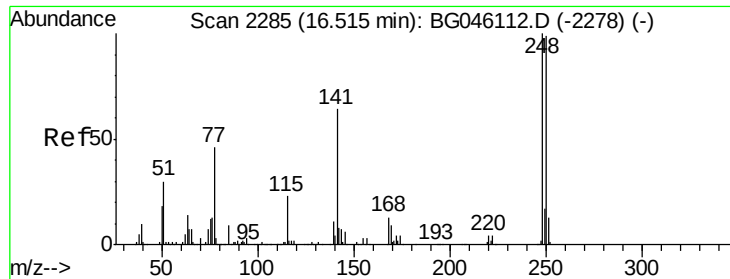




#67
4-Bromophenyl-phenylether
Concen: 3.709 ng
RT: 16.06 min Scan# 2208
Delta R.T. -0.45 min
Lab File: BG046192.D
Acq: 7 Aug 2020 14:10

Instrument :
BNA_G
ClientSampleId :
PB130804BL

Tot Ion:248 Resp: 29635
Ion Ratio Lower Upper
248 100
250 198.9 79.4 119.0#
141 431.0 50.9 76.3#

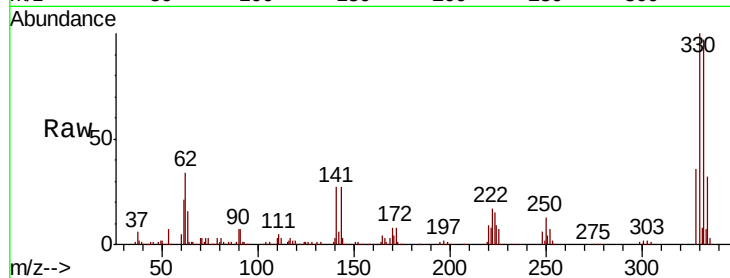


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

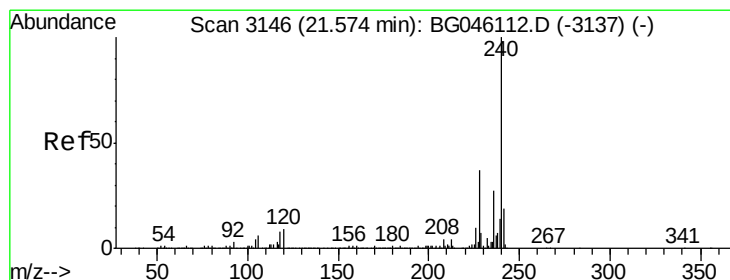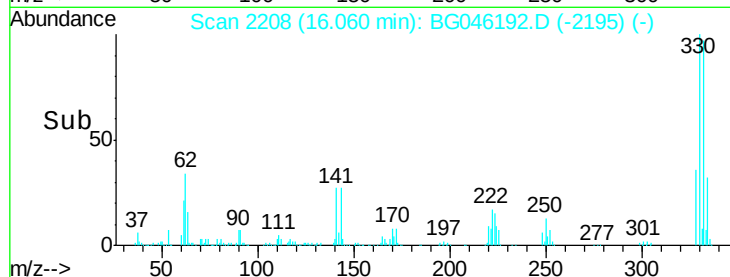
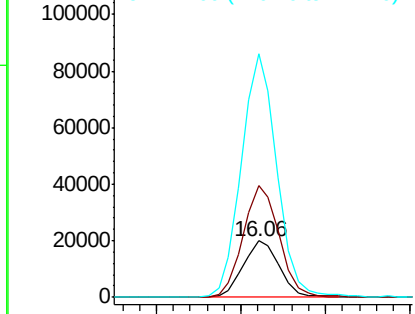



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.56 min Scan# 3144
Delta R.T. -0.01 min
Lab File: BG046192.D
Acq: 7 Aug 2020 14:10

Tgt Ion:240 Resp: 822937
Ion Ratio Lower Upper
240 100
120 8.6 7.1 10.7
236 25.9 21.7 32.5

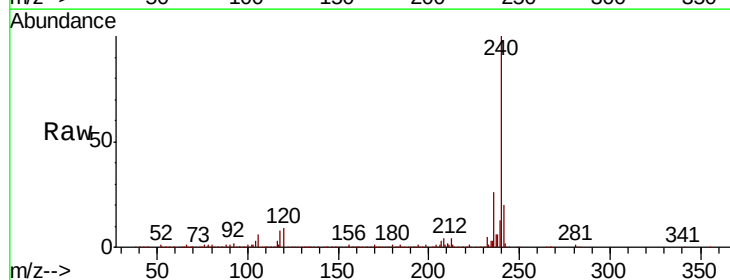

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

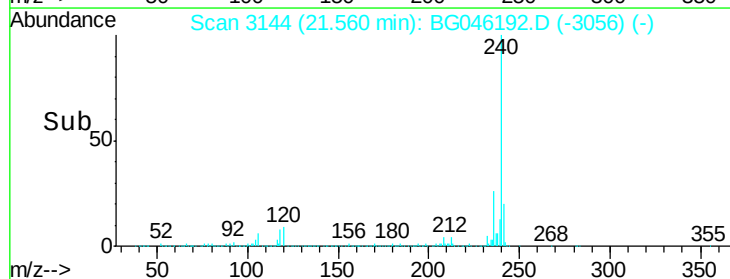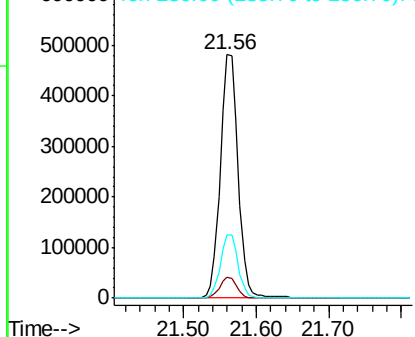

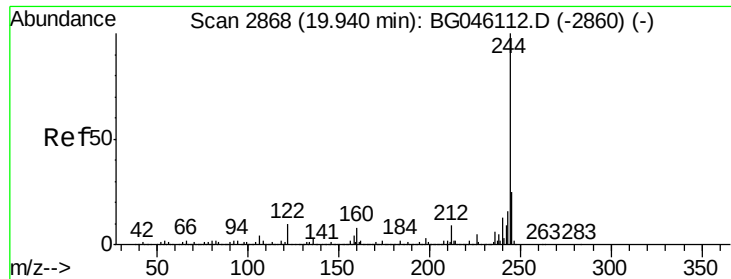

#79

Terphenyl-d14

Concen: 59.781 ng

RT: 19.93 min Scan# 2867

Delta R.T. -0.01 min

Lab File: BG046192.D

Acq: 7 Aug 2020 14:10

Instrument :

BNA_G

ClientSampleId :

PB130804BL


Tot Ion:244 Resp: 2415545

Ion Ratio Lower Upper

244 100

212 9.2 7.2 10.8




122 11.2 8.3 12.5

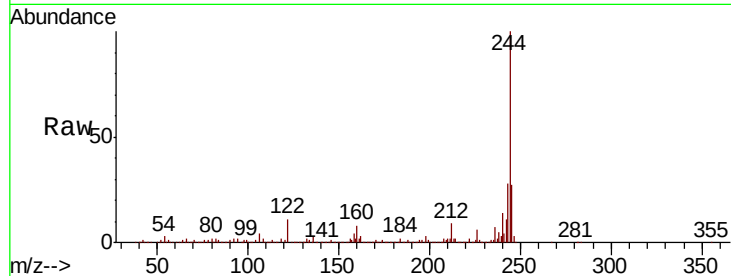

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

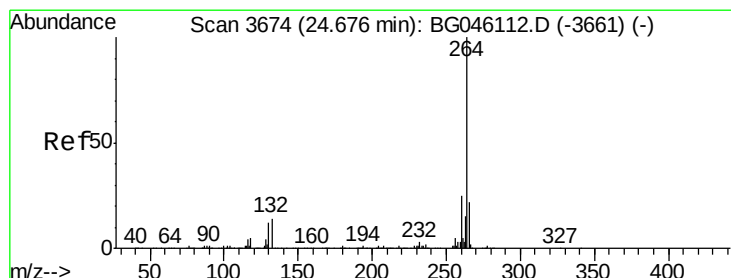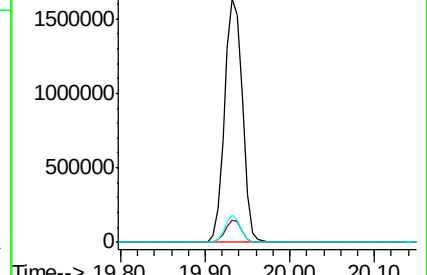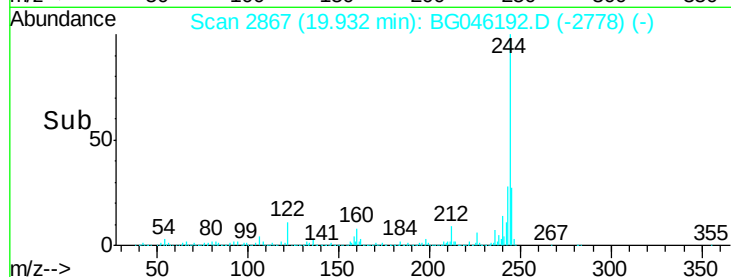

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.67 min Scan# 3673

Delta R.T. -0.01 min

Lab File: BG046192.D

Acq: 7 Aug 2020 14:10


Tgt Ion:264 Resp: 820277

Ion Ratio Lower Upper

264 100

260 23.7 19.7 29.5

265 22.4 17.6 26.4

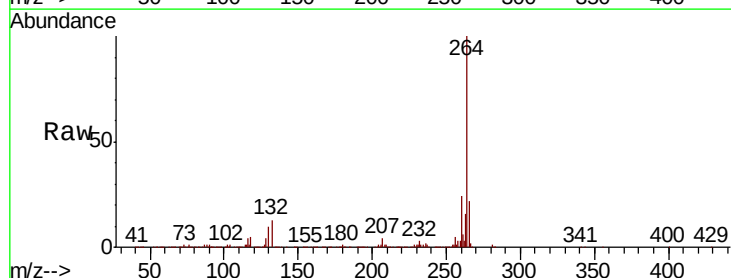

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

