
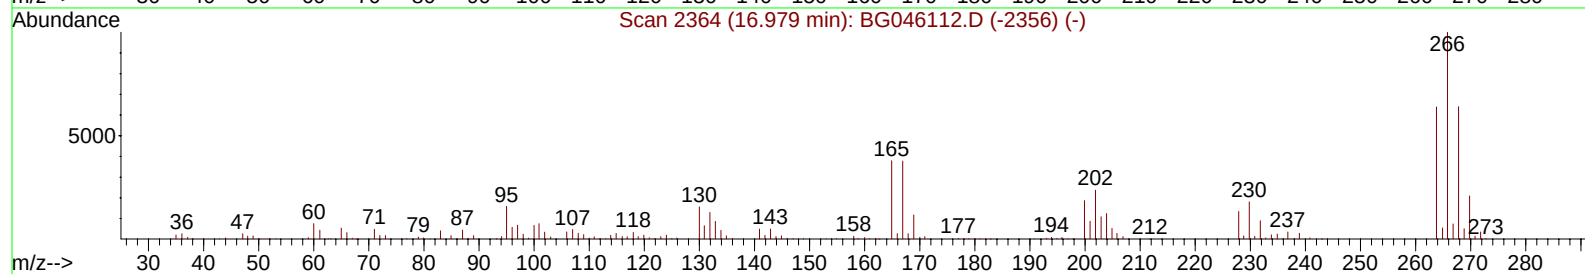
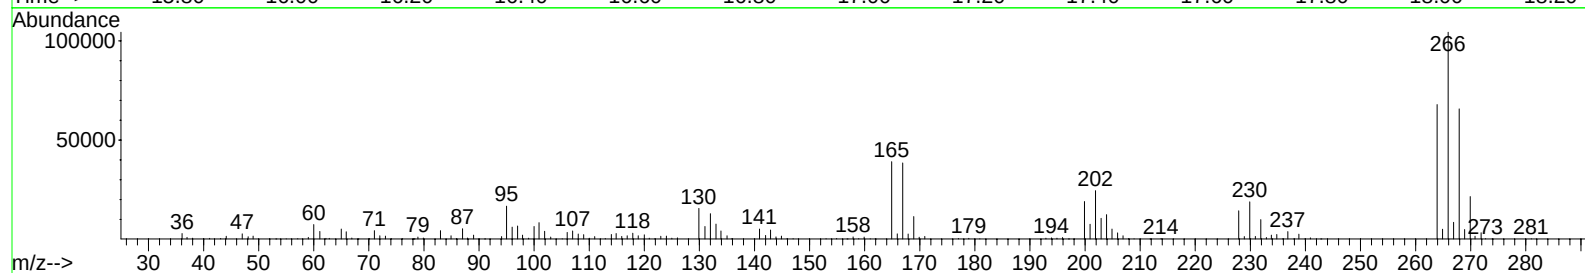


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG080720\
Data File : BG046187.D
Acq On : 7 Aug 2020 10:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 18:59:53 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 30 18:43:49 2020
Response via : Initial Calibration

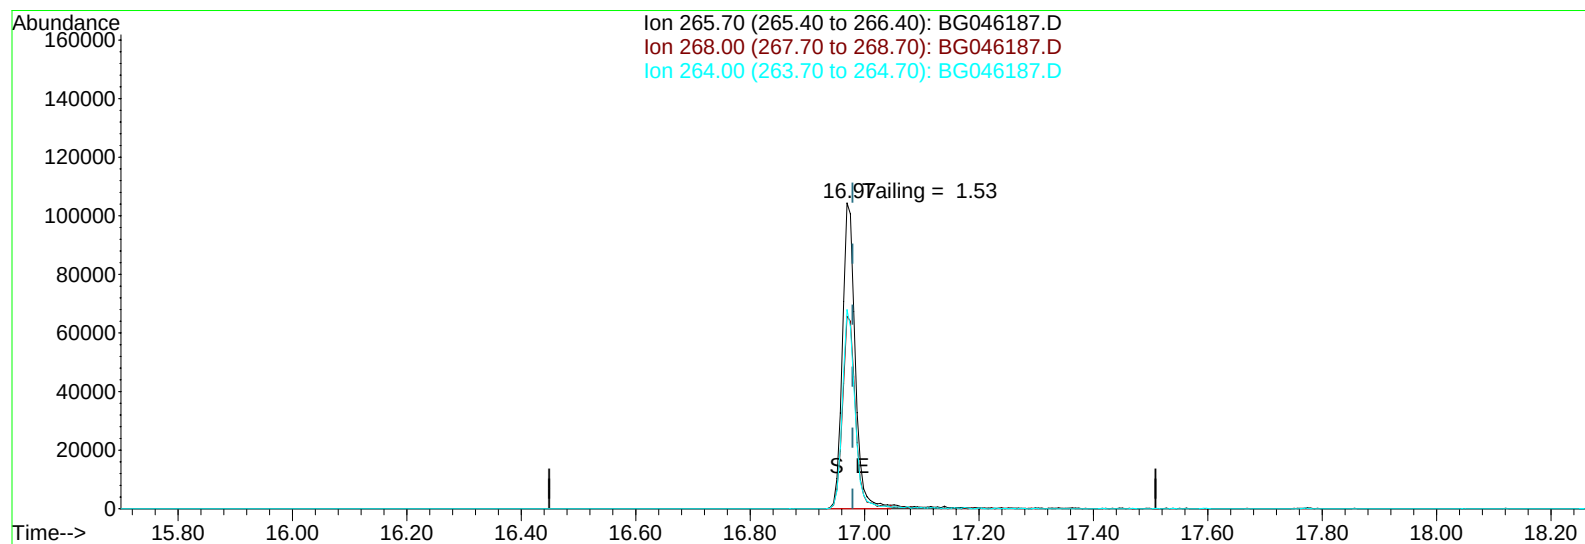

TIC: BG046187.D

(70) Pentachlorophenol (C)




16.969min (-0.010) 98508.09ng

response 163804

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	62.96
264.00	63.90	65.10
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG080720\
 Data File : BG046187.D
 Acq On : 7 Aug 2020 10:27
 Operator : CG/JU
 Sample : DF TPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 18:59:53 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 30 18:43:49 2020
 Response via : Initial Calibration

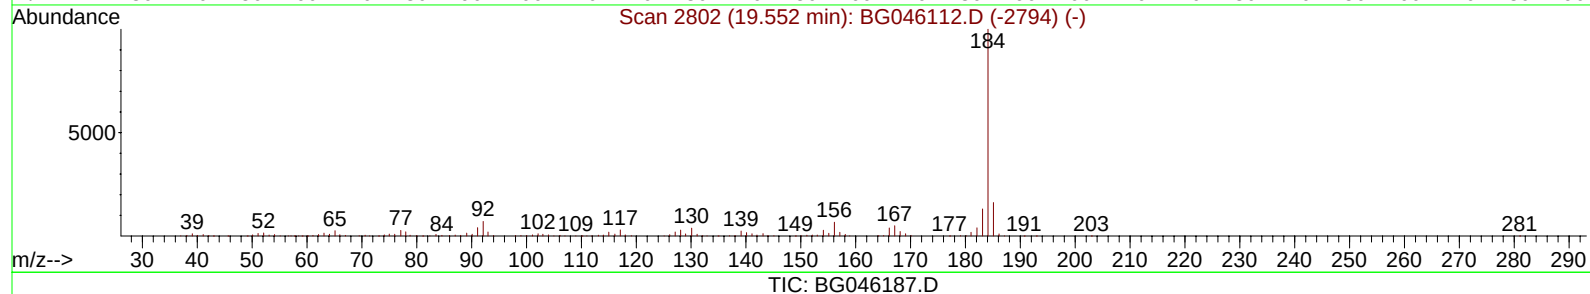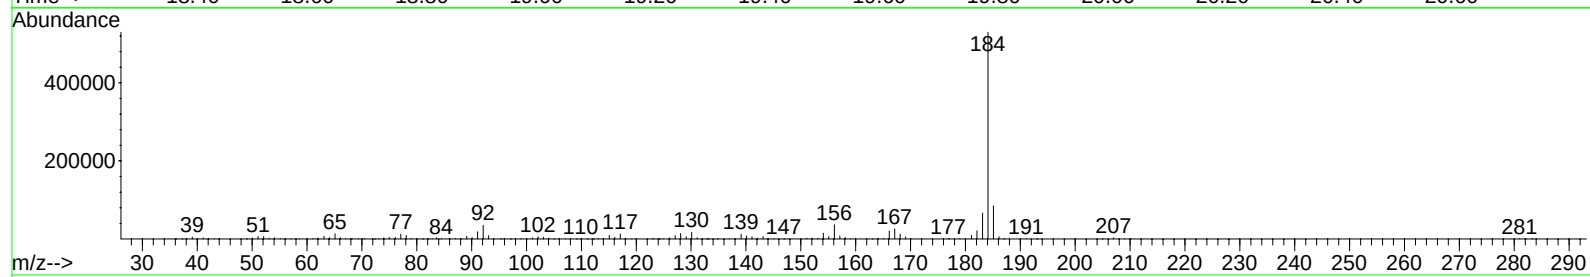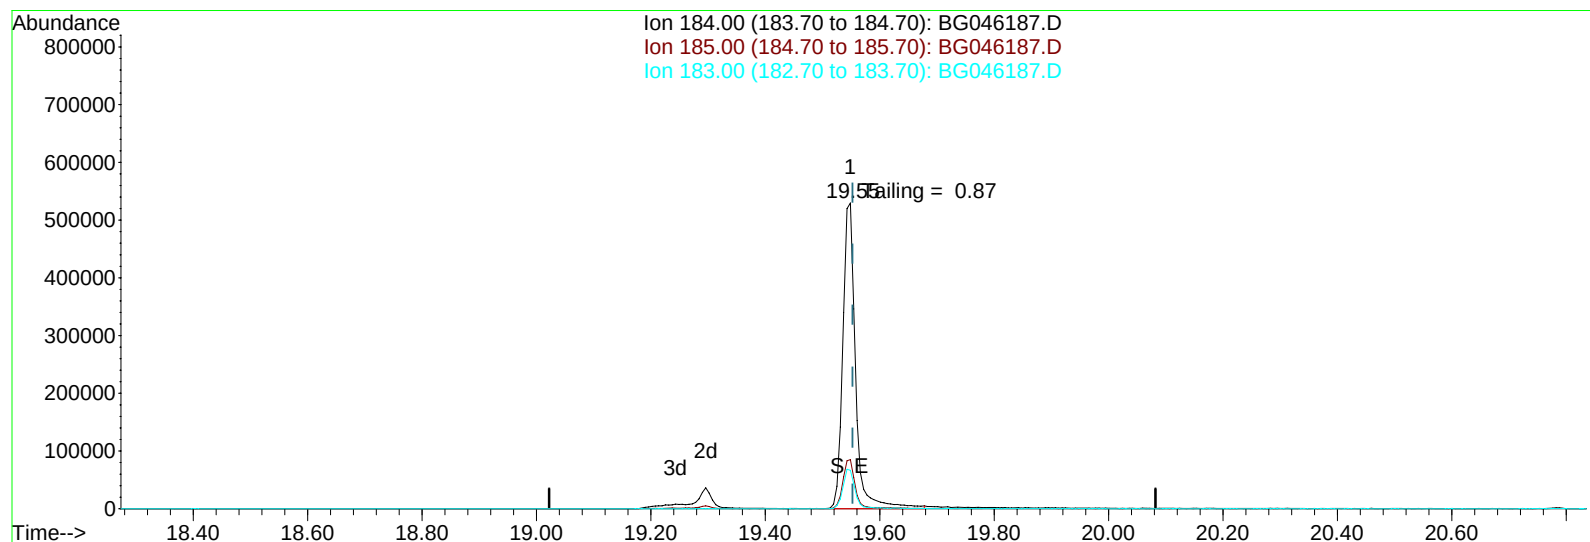

(77) Benzidine

19.549min (-0.004) 149268.09ng

response 832939

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	16.04
183.00	13.10	12.56
0.00	0.00	0.00