

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080724\
 Data File : BG062299.D
 Acq On : 7 Aug 2024 12:39
 Operator : MA/JU
 Sample : P3347-16
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B04

Quant Time: Aug 08 06:16:44 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 07 01:46:39 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.957	152	58620	20.000	ng/ul	0.00
20) Naphthalene-d8	10.754	136	283093	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.578	164	227912	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.315	188	482562	20.000	ng/ul	0.00
79) Chrysene-d12	21.557	240	462112	20.000	ng/ul	0.00
88) Perylene-d12	24.647	264	543828	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.422	96	5470	4.024	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.112	99	64556	11.538	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.288	67	97180	28.216	ng/ul	0.00
11) 2-Chlorophenol-d4	7.488	132	113272	28.257	ng/ul	0.00
15) 4-Methylphenol-d8	8.651	113	107909	23.154	ng/ul	0.00
21) Nitrobenzene-d5	9.109	128	60578	34.703	ng/ul	0.00
24) 2-Nitrophenol-d4	9.831	143	63146	38.454	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.366	165	134713	28.245	ng/ul	0.00
31) 4-Chloroaniline-d4	10.877	131	33957	4.909	ng/ul	0.00
46) Dimethylphthalate-d6	13.985	166	503754	28.648	ng/ul	0.00
49) Acenaphthylene-d8	14.272	160	559670	28.071	ng/ul	0.00
54) 4-Nitrophenol-d4	14.748	143	28233	11.468	ng/ul	0.00
60) Fluorene-d10	15.571	176	453746	28.748	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.671	200	57239	40.052	ng/ul	0.00
73) Anthracene-d10	17.415	188	752542	32.333	ng/ul	0.00
81) Pyrene-d10	19.700	212	919826	33.489	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.441	264	955249	32.858	ng/ul	0.00
Target Compounds						
35) 4-Chloro-3-methylphenol	12.011	107	14765	2.722	ng/ul	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080724\
Data File : BG062299.D
Acq On : 7 Aug 2024 12:39
Operator : MA/JU
Sample : P3347-16
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B04


Quant Time: Aug 08 06:16:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 07 01:46:39 2024
Response via : Initial Calibration

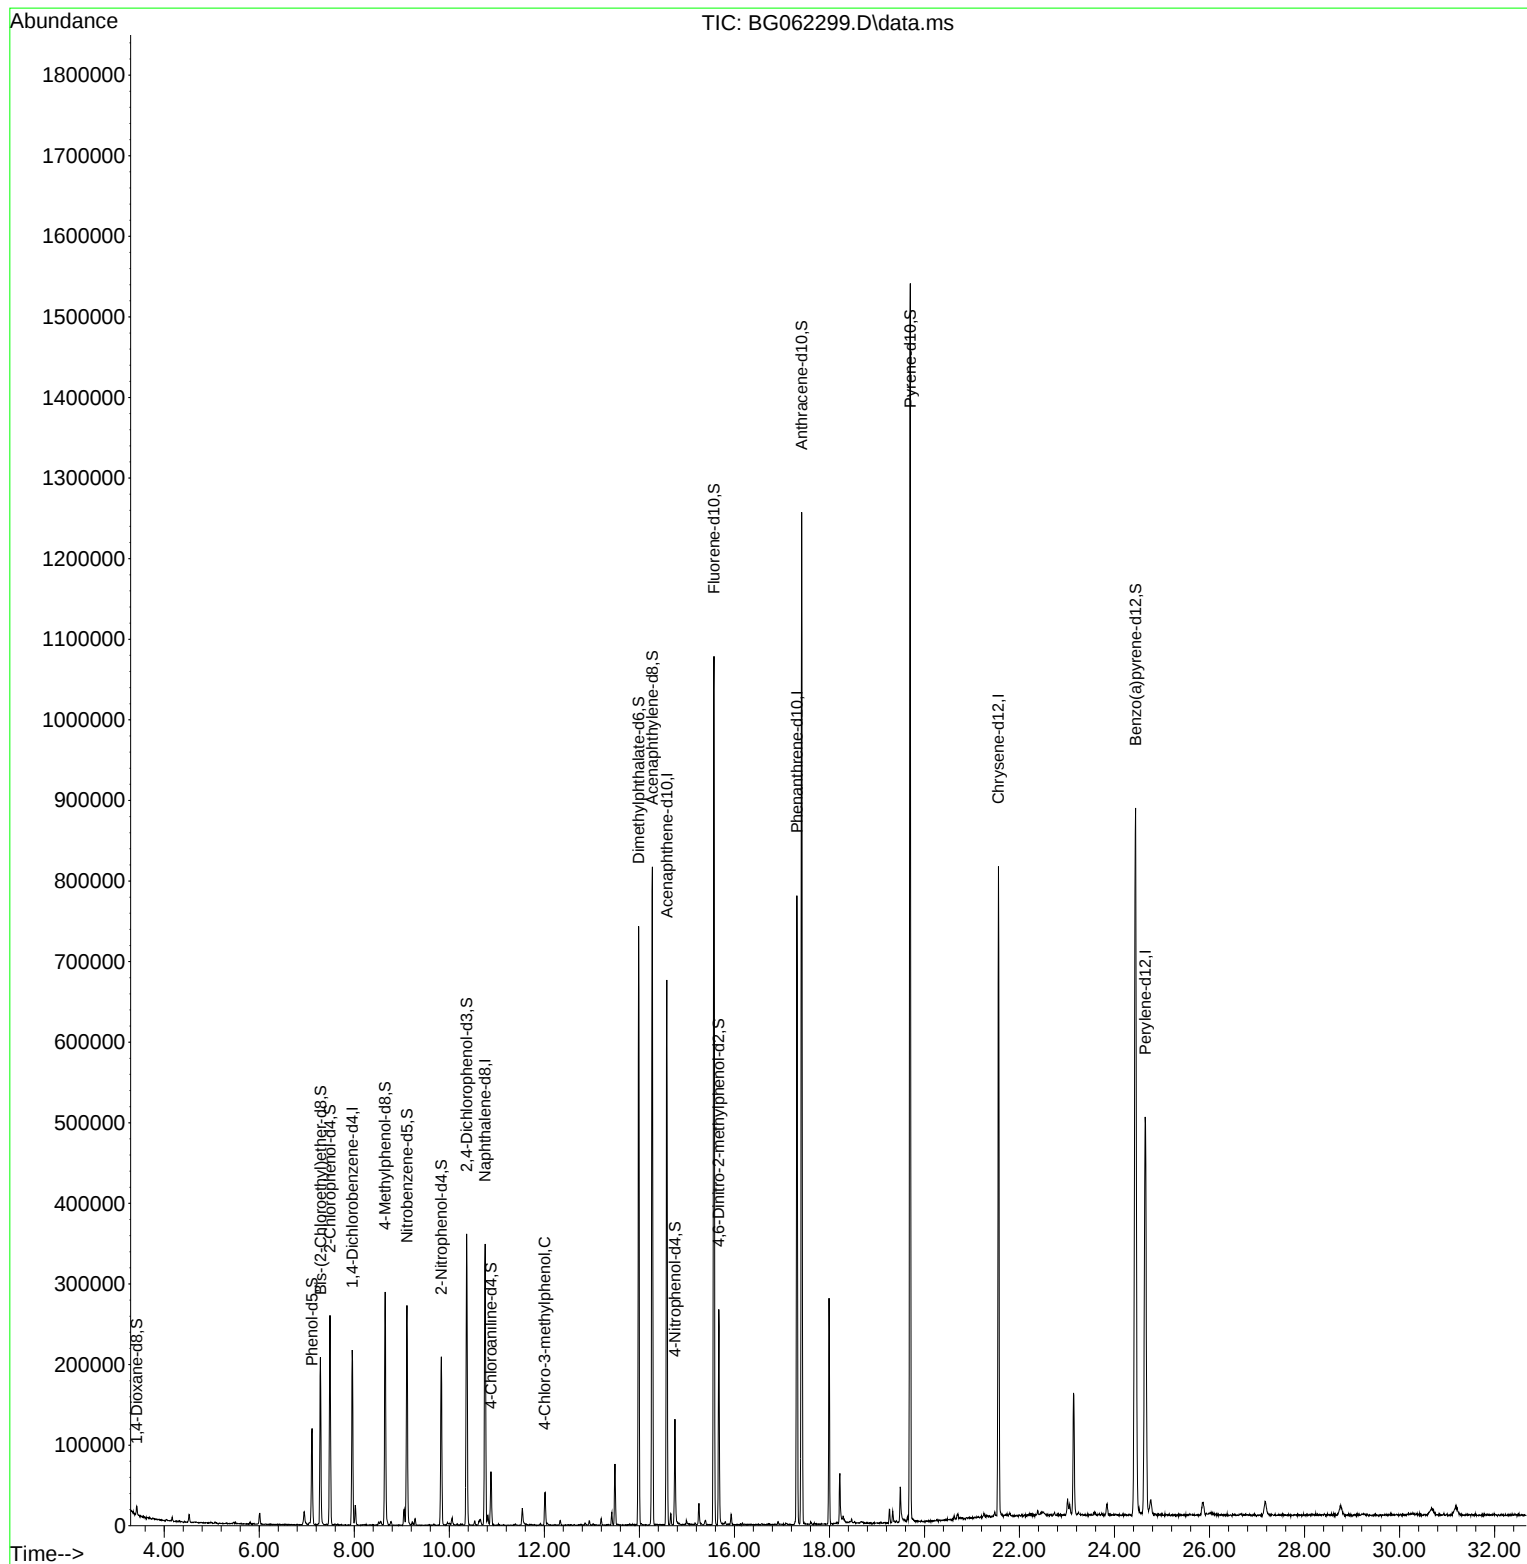

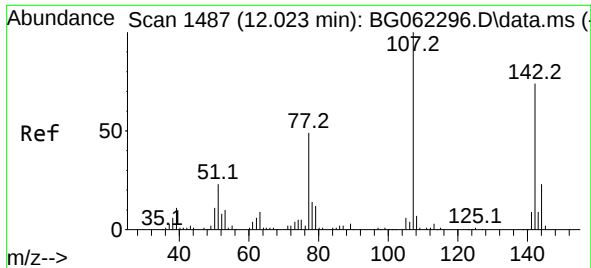

#35
4-Chloro-3-methylphenol
Concen: 2.722 ng/ul
RT: 12.011 min Scan# 14
Delta R.T. -0.012 min
Lab File: BG062299.D
Acq: 7 Aug 2024 12:39

Instrument :
BNA_G
ClientSampleId :
C0B04

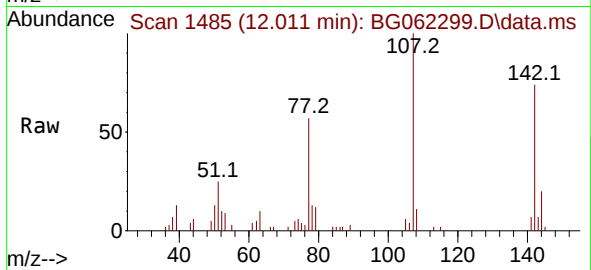

Tgt Ion:	107	Resp:	14765
Ion	Ratio	Lower	Upper
107	100		
144	20.3	20.0	30.0
142	74.4	57.8	86.8

