

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080724\
 Data File : BG062297.D
 Acq On : 7 Aug 2024 11:17
 Operator : MA/JU
 Sample : PB162305BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK305

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062297.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.420	19	22	29	rVB2	13936	20725	1.08%	0.108%
2	3.820	86	90	107	rBV	177241	317268	16.54%	1.653%
3	4.166	147	149	155	rVB6	3370	3487	0.18%	0.018%
4	4.654	227	232	234	rBV4	1312	2273	0.12%	0.012%
5	7.109	643	650	661	rBV	261111	438008	22.83%	2.282%
6	7.285	671	680	691	rBV	183606	306370	15.97%	1.596%
7	7.485	707	714	725	rBV	226718	389496	20.31%	2.029%
8	7.955	788	794	804	rVB	201162	341543	17.81%	1.780%
9	8.648	905	912	921	rBV	319911	543866	28.35%	2.834%
10	9.112	983	991	1001	rBV	236770	419771	21.88%	2.187%
11	9.829	1105	1113	1123	rBV	185598	328986	17.15%	1.714%
12	10.369	1196	1205	1213	rBV	336933	590791	30.80%	3.078%
13	10.757	1263	1271	1278	rVB	314205	565289	29.47%	2.945%
14	10.881	1284	1292	1301	rBV	348752	619593	32.30%	3.228%
15	12.337	1533	1540	1545	rBV3	5160	8688	0.45%	0.045%
16	13.988	1814	1821	1832	rBV	641250	913462	47.62%	4.760%
17	14.276	1861	1870	1877	rBV2	712519	1142465	59.56%	5.953%
18	14.581	1914	1922	1932	rBV	584541	894461	46.63%	4.661%
19	14.752	1945	1951	1962	rBV	265477	434796	22.67%	2.266%
20	15.574	2084	2091	2099	rBV	965766	1446876	75.43%	7.539%
21	15.674	2102	2108	2118	rBV	185835	284693	14.84%	1.483%
22	15.815	2128	2132	2135	rVB2	3066	4155	0.22%	0.022%
23	16.355	2221	2224	2228	rBV3	2150	2970	0.15%	0.015%
24	16.773	2292	2295	2300	rBV2	1655	2140	0.11%	0.011%
25	17.107	2346	2352	2356	rBV2	1024	2025	0.11%	0.011%
26	17.319	2380	2388	2396	rBV	680715	1045537	54.51%	5.448%
27	17.419	2398	2405	2418	rVV	1041166	1542733	80.43%	8.038%
28	17.613	2433	2438	2443	rVB2	1129	2156	0.11%	0.011%
29	17.712	2449	2455	2459	rVB2	3753	5432	0.28%	0.028%
30	18.224	2539	2542	2546	rVB	1603	2099	0.11%	0.011%
31	18.294	2551	2554	2558	rVV	3175	3204	0.17%	0.017%
32	19.269	2715	2720	2726	rVB2	14111	19892	1.04%	0.104%
33	19.334	2726	2731	2735	rBV2	10767	19016	0.99%	0.099%
34	19.369	2735	2737	2742	rVB2	7181	7387	0.39%	0.038%
35	19.645	2781	2784	2787	rBV6	1860	2280	0.12%	0.012%
36	19.704	2787	2794	2804	rVV	1230381	1788113	93.22%	9.317%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080724\
 Data File : BG062297.D
 Acq On : 7 Aug 2024 11:17
 Operator : MA/JU
 Sample : PB162305BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK305

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

37	20.632	2949	2952	2955	rVB2	3334	3438	0.18%	0.018%
38	20.691	2959	2962	2966	rBV6	3832	5287	0.28%	0.028%
39	21.472	3089	3095	3097	rBV6	4517	8835	0.46%	0.046%
40	21.566	3104	3111	3124	rVB	691175	1145597	59.72%	5.969%
41	21.795	3147	3150	3156	rVB6	4223	5854	0.31%	0.031%
42	22.389	3246	3251	3257	rBV6	7102	15330	0.80%	0.080%
43	22.494	3267	3269	3272	rBV4	3399	5155	0.27%	0.027%
44	23.064	3361	3366	3372	rBV6	14289	27603	1.44%	0.144%
45	23.663	3466	3468	3469	rBV2	2745	2252	0.12%	0.012%
46	23.681	3469	3471	3476	rVB7	4250	5364	0.28%	0.028%
47	23.851	3494	3500	3509	rBV3	19267	41277	2.15%	0.215%
48	24.450	3591	3602	3619	rBV2	713997	1918158	100.00%	9.995%
49	24.662	3627	3638	3649	rBV2	455310	1249847	65.16%	6.512%
50	24.774	3651	3657	3667	rVB4	26778	69487	3.62%	0.362%
51	25.872	3837	3844	3853	rVB4	24888	70666	3.68%	0.368%
52	26.289	3913	3915	3918	rBV4	2081	1951	0.10%	0.010%
53	26.501	3949	3951	3952	rVB	3313	2049	0.11%	0.011%
54	26.518	3952	3954	3956	rBV3	2333	2103	0.11%	0.011%
55	27.194	4059	4069	4080	rVB3	23291	79521	4.15%	0.414%
56	27.593	4135	4137	4140	rBV5	2620	3153	0.16%	0.016%
57	27.640	4141	4145	4147	rVB4	3032	3541	0.18%	0.018%
58	27.999	4204	4206	4209	rBV4	2314	1938	0.10%	0.010%
59	28.774	4330	4338	4351	rVB4	16561	59396	3.10%	0.309%
60	31.635	4823	4825	4828	rBV4	2043	1987	0.10%	0.010%




Sum of corrected areas: 19191835

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080724\
Data File : BG062297.D
Acq On : 7 Aug 2024 11:17
Operator : MA/JU
Sample : PB162305BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK305

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

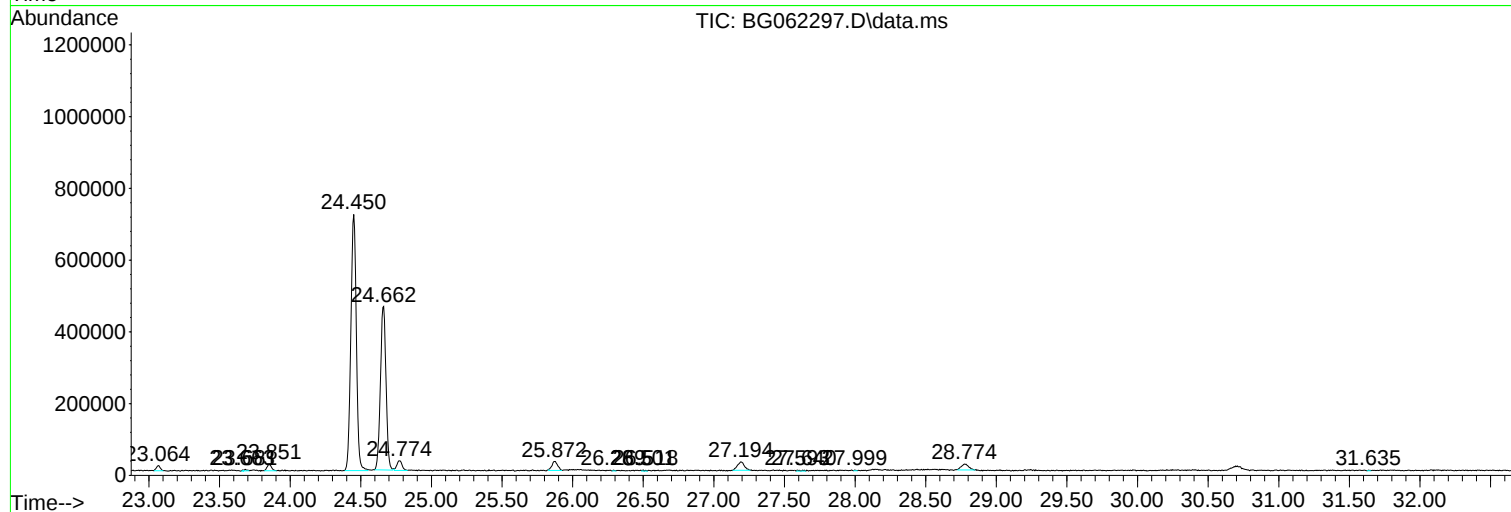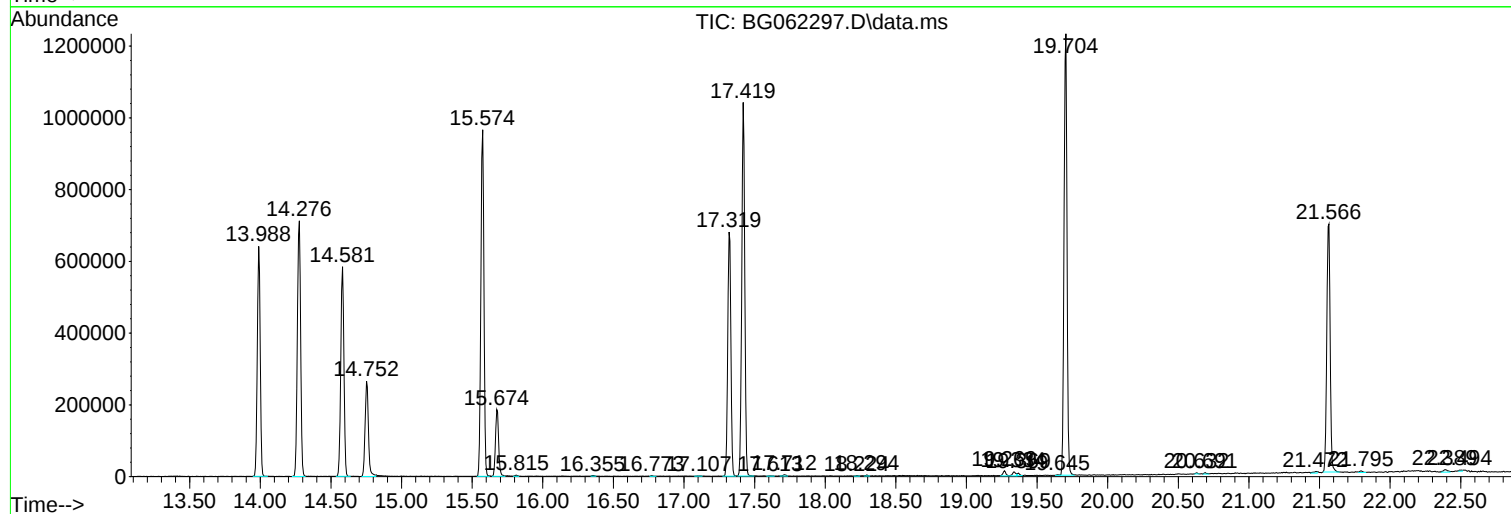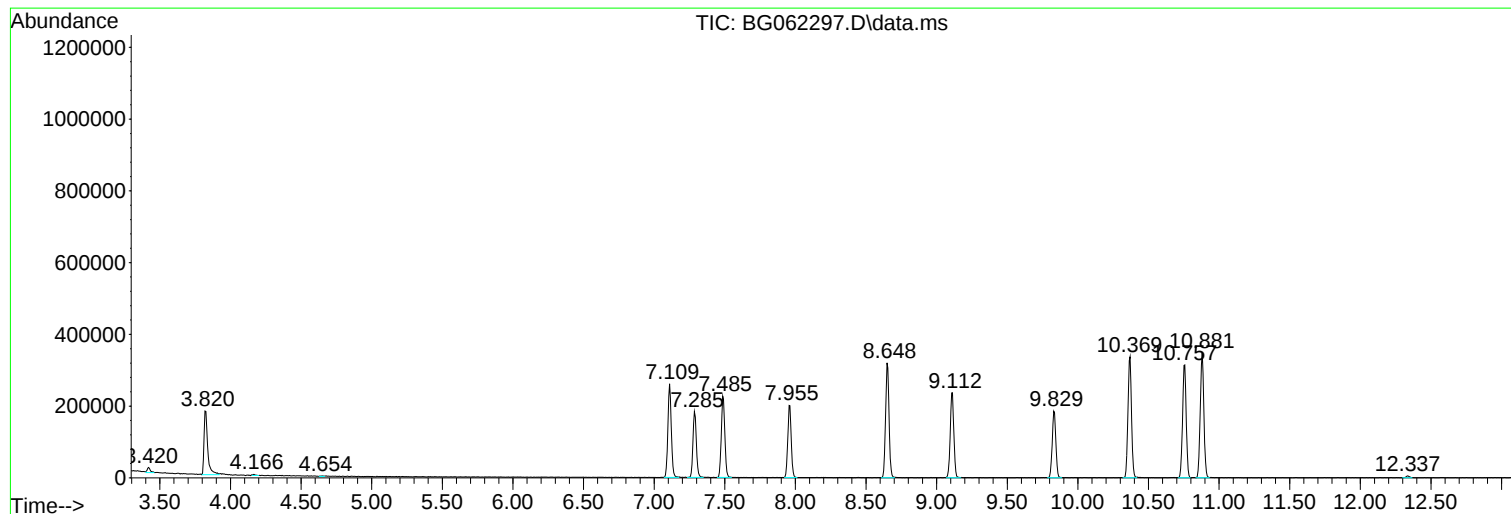

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080724\
Data File : BG062297.D
Acq On : 7 Aug 2024 11:17
Operator : MA/JU
Sample : PB162305BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK305

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080724\
Data File : BG062297.D
Acq On : 7 Aug 2024 11:17
Operator : MA/JU
Sample : PB162305BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK305

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc