

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080724\
 Data File : BG062300.D
 Acq On : 7 Aug 2024 13:20
 Operator : MA/JU
 Sample : P3359-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E1G97

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062300.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.426	18	23	29	rVB4	10064	19109	0.88%	0.097%
2	3.831	87	92	104	rBV	37955	72955	3.36%	0.370%
3	4.166	144	149	165	rVB	39111	71445	3.29%	0.362%
4	7.109	644	650	659	rVB	85295	154141	7.10%	0.782%
5	7.285	674	680	691	rBV	179711	315152	14.52%	1.598%
6	7.491	708	715	726	rVB	207374	379689	17.49%	1.926%
7	7.961	786	795	802	rBV	195782	334889	15.43%	1.698%
8	8.026	802	806	810	rVB2	5935	9317	0.43%	0.047%
9	8.648	905	912	921	rBV	244113	420221	19.36%	2.131%
10	9.112	983	991	1000	rBV	244117	442731	20.39%	2.245%
11	9.218	1005	1009	1019	rBV5	5198	11406	0.53%	0.058%
12	9.829	1105	1113	1122	rBV	202001	348467	16.05%	1.767%
13	9.964	1132	1136	1139	rBV4	1557	2695	0.12%	0.014%
14	10.064	1148	1153	1158	rBV3	1293	2583	0.12%	0.013%
15	10.369	1196	1205	1216	rBV	325888	581136	26.77%	2.947%
16	10.528	1227	1232	1237	rBV3	6887	10898	0.50%	0.055%
17	10.751	1262	1270	1280	rBV	303557	535008	24.64%	2.713%
18	10.881	1284	1292	1302	rBV	283702	502434	23.14%	2.548%
19	11.544	1401	1405	1406	rBV2	2152	2620	0.12%	0.013%
20	12.337	1535	1540	1547	rBV2	5215	8460	0.39%	0.043%
21	13.418	1719	1724	1728	rBV2	1612	2546	0.12%	0.013%
22	13.988	1814	1821	1829	rBV	696230	977336	45.02%	4.957%
23	14.270	1862	1869	1877	rBV2	778671	1223606	56.36%	6.206%
24	14.581	1915	1922	1929	rVB	580577	902707	41.58%	4.578%
25	14.746	1944	1950	1959	rBV	71422	118830	5.47%	0.603%
26	15.392	2055	2060	2064	rBV3	2992	4139	0.19%	0.021%
27	15.568	2083	2090	2101	rVB	1061453	1573158	72.47%	7.979%
28	15.674	2102	2108	2118	rVV	235153	343249	15.81%	1.741%
29	15.809	2126	2131	2135	rVB2	3650	5070	0.23%	0.026%
30	17.319	2381	2388	2397	rBV	768966	1114223	51.33%	5.651%
31	17.419	2397	2405	2414	rVV	1191235	1773555	81.70%	8.995%
32	18.218	2536	2541	2549	rBV4	17490	28547	1.31%	0.145%
33	18.288	2551	2553	2559	rVB3	3046	4269	0.20%	0.022%
34	18.652	2610	2615	2618	rBV3	1749	2328	0.11%	0.012%
35	19.269	2714	2720	2724	rBV2	15958	23153	1.07%	0.117%
36	19.334	2725	2731	2735	rBV2	14366	19770	0.91%	0.100%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080724\
 Data File : BG062300.D
 Acq On : 7 Aug 2024 13:20
 Operator : MA/JU
 Sample : P3359-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E1G97

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

37	19.492	2754	2758	2765	rBV2	10794	16468	0.76%	0.084%
38	19.651	2782	2785	2787	rBV2	3764	3583	0.17%	0.018%
39	19.698	2787	2793	2802	rVV	1471260	2133802	98.29%	10.822%
40	20.432	2916	2918	2922	rVV4	2235	2501	0.12%	0.013%
41	20.691	2959	2962	2964	rBV3	4027	3567	0.16%	0.018%
42	20.750	2969	2972	2978	rBV6	3258	6069	0.28%	0.031%
43	20.861	2987	2991	2992	rBV2	2215	2490	0.11%	0.013%
44	21.002	3012	3015	3017	rBV3	2555	2476	0.11%	0.013%
45	21.214	3047	3051	3052	rBV3	1940	2591	0.12%	0.013%
46	21.249	3053	3057	3061	rVV7	4349	8738	0.40%	0.044%
47	21.319	3067	3069	3073	rVB4	3325	3176	0.15%	0.016%
48	21.484	3092	3097	3101	rVB	21537	29742	1.37%	0.151%
49	21.560	3103	3110	3123	rBV2	776302	1251174	57.63%	6.346%
50	21.783	3146	3148	3149	rBV2	3890	2614	0.12%	0.013%
51	22.388	3247	3251	3256	rBV6	6167	9981	0.46%	0.051%
52	22.741	3307	3311	3317	rVB7	9261	13945	0.64%	0.071%
53	23.064	3360	3366	3372	rVV3	14868	27921	1.29%	0.142%
54	23.246	3392	3397	3403	rVB4	14809	26987	1.24%	0.137%
55	23.569	3450	3452	3453	rBV2	3393	2391	0.11%	0.012%
56	23.839	3493	3498	3507	rBV5	20468	42822	1.97%	0.217%
57	24.444	3590	3601	3622	rBV	823820	2170891	100.00%	11.010%
58	24.656	3625	3637	3648	rVV	479837	1336398	61.56%	6.778%
59	24.768	3649	3656	3663	rVB2	26085	65791	3.03%	0.334%
60	25.866	3834	3843	3853	rBV5	26254	79316	3.65%	0.402%
61	25.937	3853	3855	3857	rBV3	3063	2656	0.12%	0.013%
62	27.182	4058	4067	4082	rVB4	24163	86998	4.01%	0.441%
63	28.269	4248	4252	4255	rBV4	2920	4033	0.19%	0.020%
64	28.762	4325	4336	4337	rBV5	15623	36452	1.68%	0.185%




Sum of corrected areas: 19717415

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080724\
Data File : BG062300.D
Acq On : 7 Aug 2024 13:20
Operator : MA/JU
Sample : P3359-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1G97

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

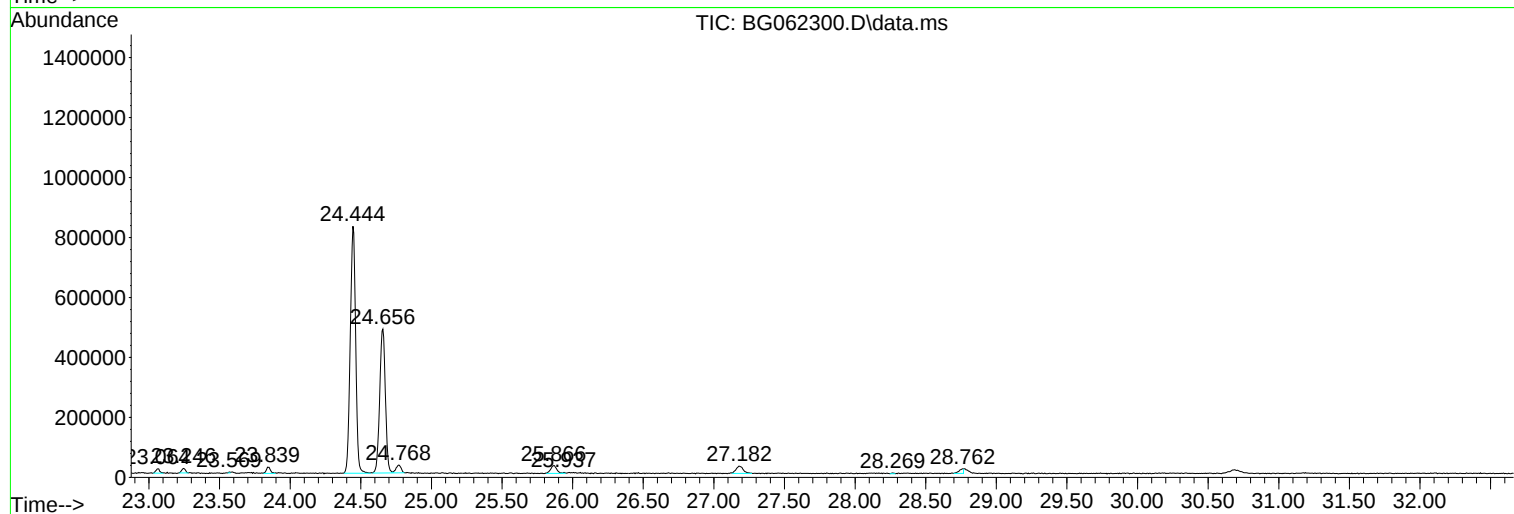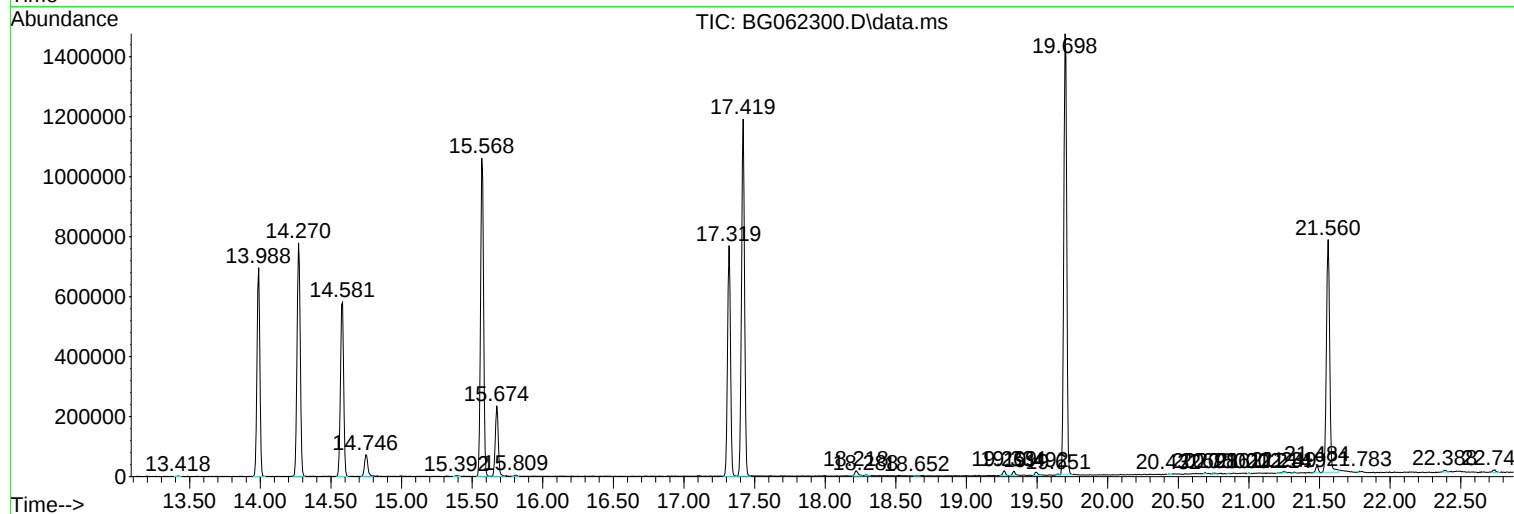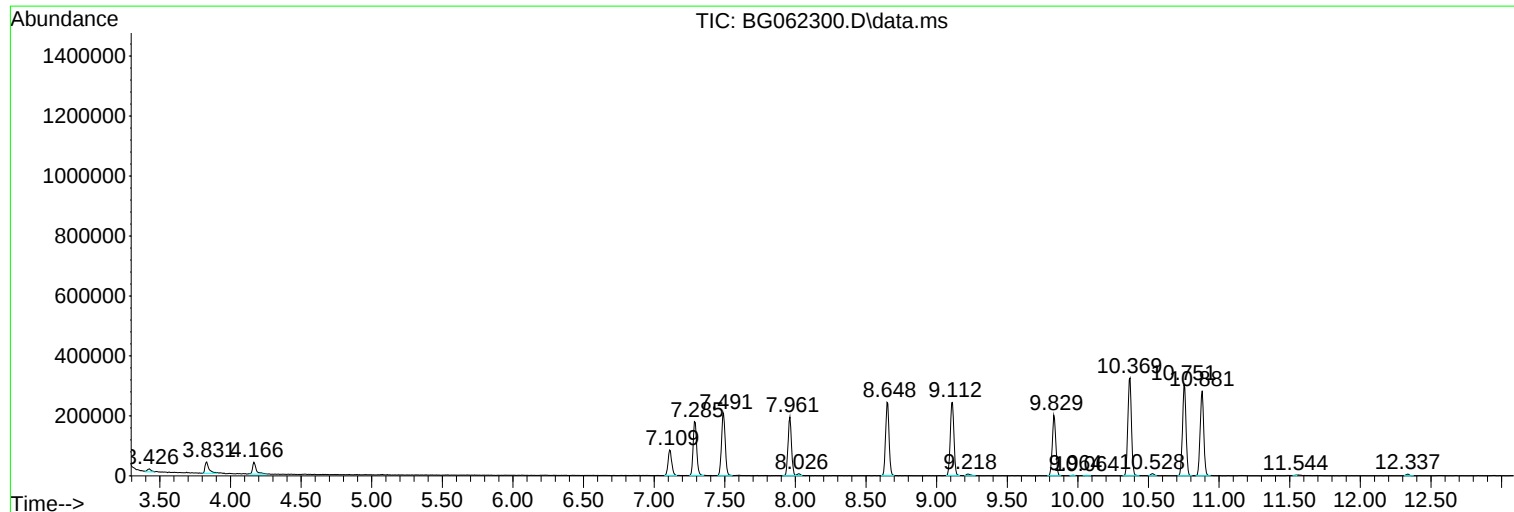

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080724\
Data File : BG062300.D
Acq On : 7 Aug 2024 13:20
Operator : MA/JU
Sample : P3359-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1G97

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080724\
Data File : BG062300.D
Acq On : 7 Aug 2024 13:20
Operator : MA/JU
Sample : P3359-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1G97

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc