

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080724\
 Data File : BG062307.D
 Acq On : 7 Aug 2024 18:08
 Operator : MA/JU
 Sample : P3359-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E1G77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG062307.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.419	19	22	29	rVB3	12644	20088	0.85%	0.095%
2	3.830	88	92	101	rBV	42467	74314	3.15%	0.350%
3	4.171	146	150	158	rVB3	6768	10936	0.46%	0.052%
4	7.108	643	650	660	rVB	72546	119067	5.04%	0.561%
5	7.284	674	680	689	rBV	206501	348738	14.77%	1.644%
6	7.490	708	715	726	rVB	234213	395859	16.76%	1.866%
7	7.960	787	795	802	rBV	225392	373267	15.80%	1.759%
8	8.024	803	806	811	rVB3	2559	3901	0.17%	0.018%
9	8.653	905	913	920	rBV	212054	362156	15.33%	1.707%
10	9.111	982	991	1002	rBV	269930	478121	20.24%	2.254%
11	9.828	1106	1113	1123	rVB	217685	384846	16.29%	1.814%
12	9.957	1131	1135	1138	rBV3	1839	3432	0.15%	0.016%
13	10.368	1197	1205	1213	rBV	371925	660052	27.95%	3.111%
14	10.750	1263	1270	1282	rVB	352294	627824	26.58%	2.959%
15	10.879	1282	1292	1301	rBV	253742	464923	19.69%	2.192%
16	11.490	1391	1396	1400	rBV4	3141	5037	0.21%	0.024%
17	12.336	1535	1540	1545	rVB3	6625	10319	0.44%	0.049%
18	13.194	1681	1686	1691	rVB3	1776	2362	0.10%	0.011%
19	13.423	1720	1725	1730	rVB3	7138	10689	0.45%	0.050%
20	13.987	1814	1821	1828	rVB	736937	1056107	44.72%	4.978%
21	14.075	1835	1836	1840	rVB2	2552	2768	0.12%	0.013%
22	14.116	1840	1843	1847	rVB4	2322	3504	0.15%	0.017%
23	14.269	1860	1869	1877	rBV	856343	1346256	57.00%	6.346%
24	14.492	1903	1907	1911	rBV2	12189	14861	0.63%	0.070%
25	14.574	1913	1921	1932	rBV	665845	1038924	43.99%	4.897%
26	14.745	1943	1950	1963	rBV	71739	121813	5.16%	0.574%
27	14.944	1979	1984	1987	rBV3	1546	2948	0.12%	0.014%
28	14.991	1989	1992	1996	rVV2	3731	3978	0.17%	0.019%
29	15.115	2009	2013	2016	rBV3	1916	2630	0.11%	0.012%
30	15.385	2054	2059	2064	rBV6	3629	6569	0.28%	0.031%
31	15.444	2065	2069	2072	rVB	7798	10190	0.43%	0.048%
32	15.567	2083	2090	2099	rVV	1111729	1704676	72.18%	8.035%
33	15.673	2102	2108	2116	rVV	273785	391459	16.57%	1.845%
34	15.732	2116	2118	2125	rVV5	3028	5063	0.21%	0.024%
35	15.802	2127	2130	2136	rVV4	4624	7577	0.32%	0.036%
36	15.855	2136	2139	2142	rVB4	2825	3142	0.13%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080724\
 Data File : BG062307.D
 Acq On : 7 Aug 2024 18:08
 Operator : MA/JU
 Sample : P3359-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E1G77

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
 Title : SVOA CALIBRATION

37	16.301	2212	2215	2217	rBV3	2949	3707	0.16%	0.017%
38	16.331	2218	2220	2227	rVB5	3263	5755	0.24%	0.027%
39	16.718	2283	2286	2290	rBV3	2023	3071	0.13%	0.014%
40	17.100	2347	2351	2355	rBV6	3002	5221	0.22%	0.025%
41	17.159	2355	2361	2364	rVB6	2992	5724	0.24%	0.027%
42	17.318	2381	2388	2394	rBV	816017	1212860	51.35%	5.717%
43	17.418	2397	2405	2413	rVV2	1179379	1838522	77.85%	8.666%
44	17.752	2460	2462	2467	rVB4	2354	3478	0.15%	0.016%
45	18.005	2501	2505	2507	rBV5	1879	2741	0.12%	0.013%
46	18.216	2536	2541	2547	rBV2	48741	70383	2.98%	0.332%
47	18.522	2590	2593	2595	rBV4	3655	3950	0.17%	0.019%
48	18.657	2611	2616	2618	rBV6	7700	10257	0.43%	0.048%
49	19.262	2715	2719	2726	rBV2	18975	27641	1.17%	0.130%
50	19.333	2726	2731	2735	rBV	20458	28710	1.22%	0.135%
51	19.491	2754	2758	2765	rBV2	44413	71541	3.03%	0.337%
52	19.697	2786	2793	2801	rBV	1537280	2213622	93.73%	10.434%
53	19.832	2814	2816	2821	rVB5	15480	18329	0.78%	0.086%
54	19.897	2826	2827	2828	rBV	5151	2853	0.12%	0.013%
55	21.477	3092	3096	3101	rVB	44581	54096	2.29%	0.255%
56	21.553	3103	3109	3119	rVV2	825009	1356595	57.44%	6.395%
57	23.832	3493	3497	3505	rVB3	27580	52328	2.22%	0.247%
58	24.437	3589	3600	3613	rBV	924039	2361756	100.00%	11.133%
59	24.643	3625	3635	3647	rVV	542922	1500350	63.53%	7.072%
60	24.761	3650	3655	3664	rVB4	33533	83772	3.55%	0.395%
61	25.847	3834	3840	3851	rBV3	29516	82693	3.50%	0.390%
62	27.163	4054	4064	4076	rBV5	27856	99738	4.22%	0.470%
63	28.074	4217	4219	4221	rBV2	4020	3561	0.15%	0.017%
64	30.606	4648	4650	4651	rBV2	4747	4451	0.19%	0.021%
65	30.841	4688	4690	4692	rVB3	4315	3143	0.13%	0.015%
66	31.269	4761	4763	4770	rBV7	3203	5216	0.22%	0.025%




Sum of corrected areas: 21214460

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080724\
Data File : BG062307.D
Acq On : 7 Aug 2024 18:08
Operator : MA/JU
Sample : P3359-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1G77

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

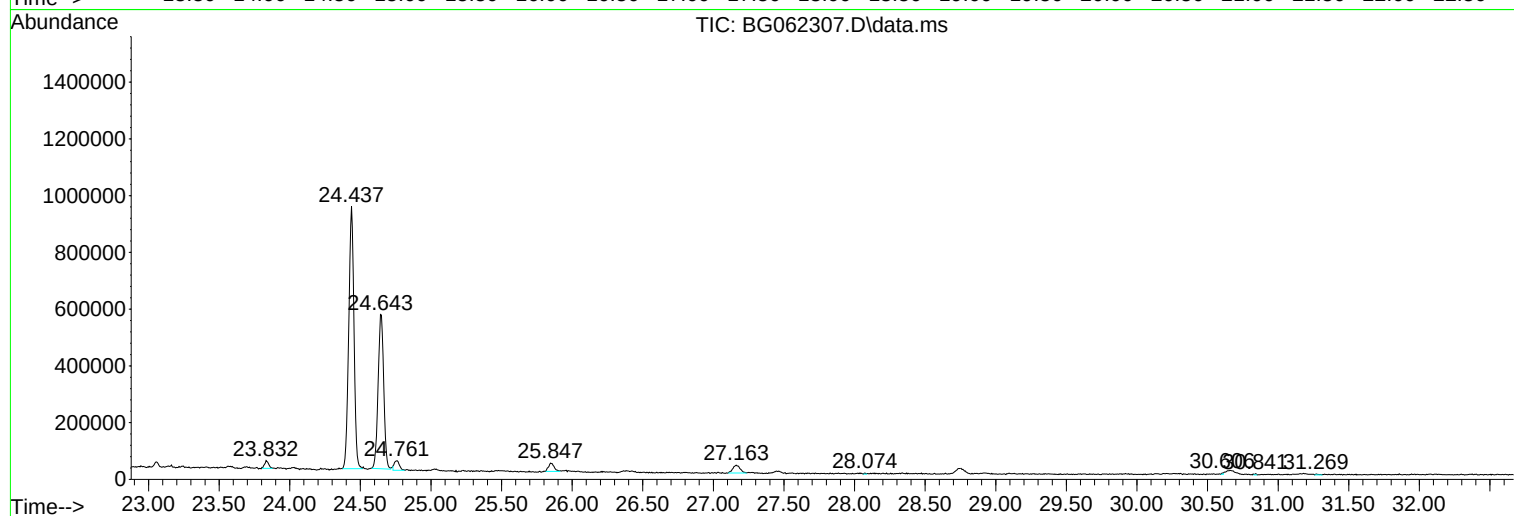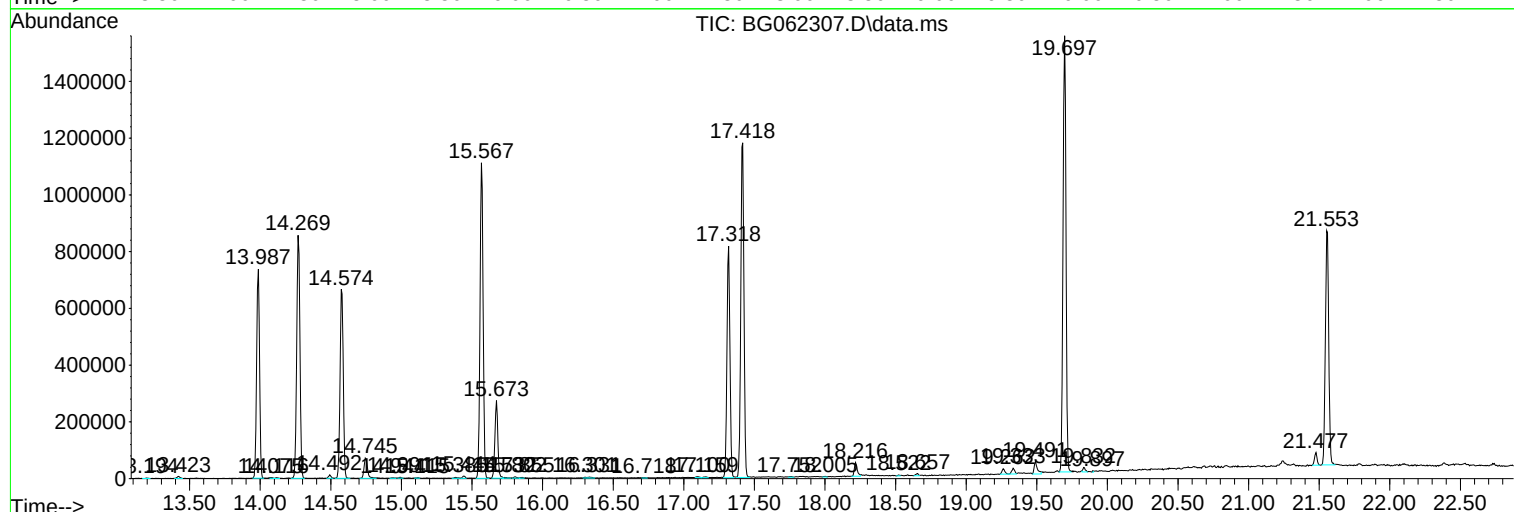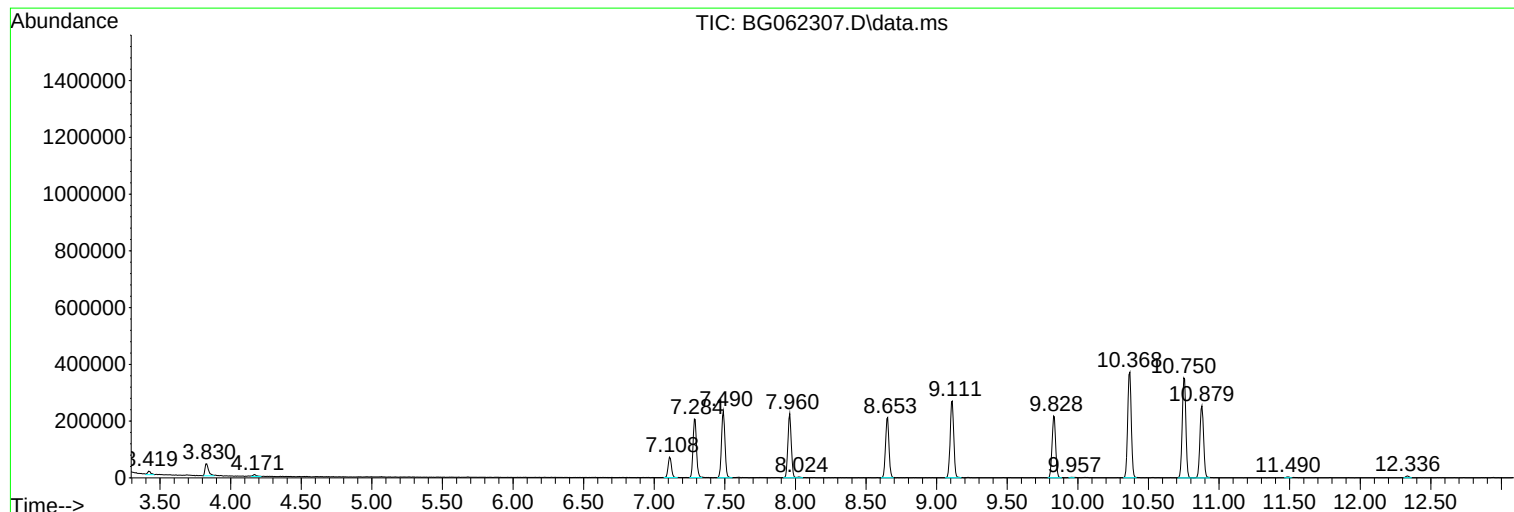

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080724\
Data File : BG062307.D
Acq On : 7 Aug 2024 18:08
Operator : MA/JU
Sample : P3359-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1G77

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080724\
Data File : BG062307.D
Acq On : 7 Aug 2024 18:08
Operator : MA/JU
Sample : P3359-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E1G77

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG080524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc