


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080815\
Data File : BG018321.D
Acq On : 8 Aug 2015 9:00
Operator : UM/TP
Sample : G3095-08DL 5X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Aug 10 02:58:35 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080815.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 10 01:57:33 2015
Response via : Initial Calibration

Instrument :
BNA_G
ClientSampleId :
C01R8DL

Manual Integrations
APPROVED
MMDadoda
8/10/2015 7:23:10 PM

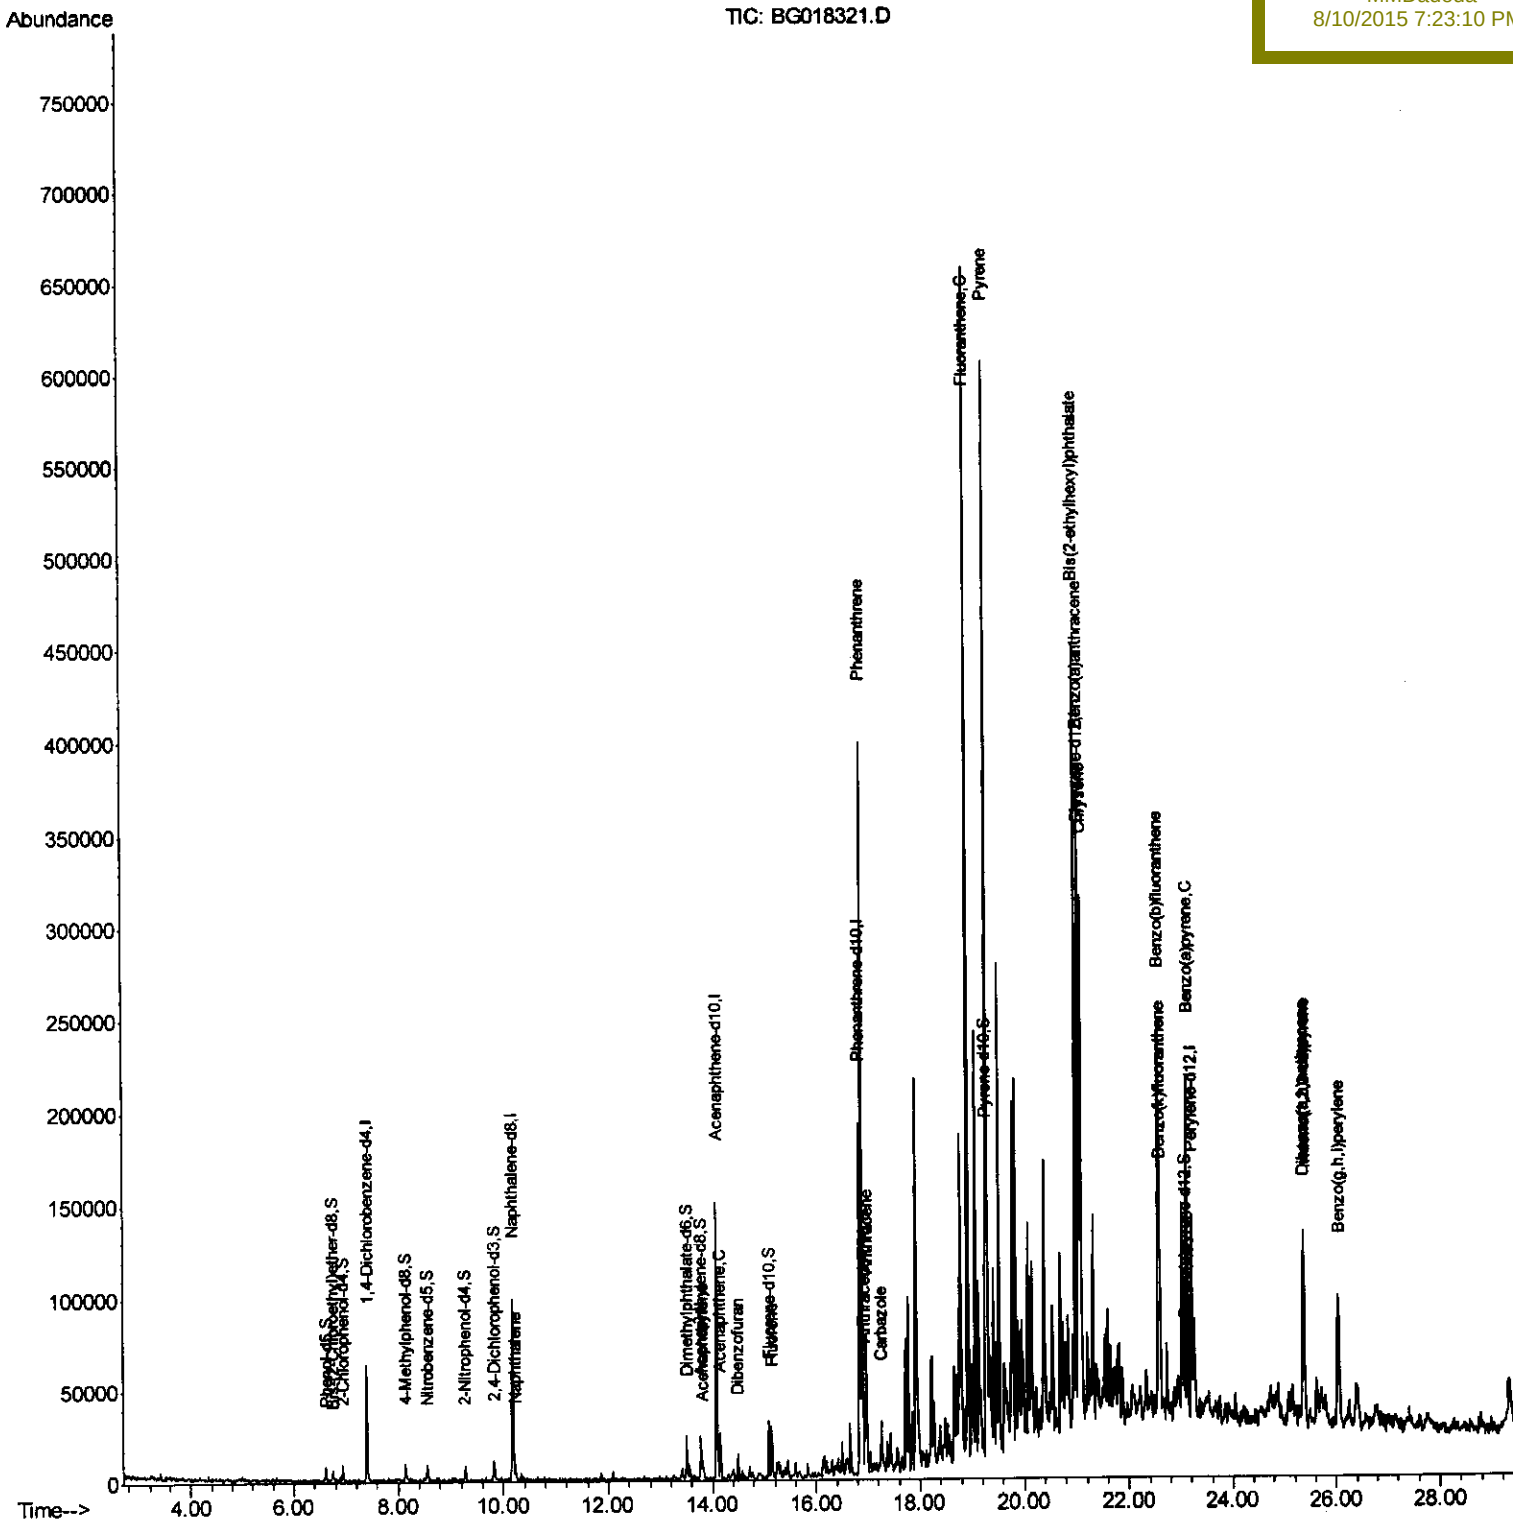


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080815\
Data File : BG018321.D
Acq On : 8 Aug 2015 9:00
Operator : UM/TP
Sample : G3095-08DL 5X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C01R8DL

Manual Integrations
APPROVED
MMDadoda
8/10/2015 7:23:10 PM

Quant Time: Aug 10 02:07:21 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080815.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 10 01:57:33 2015
Response via : Initial Calibration

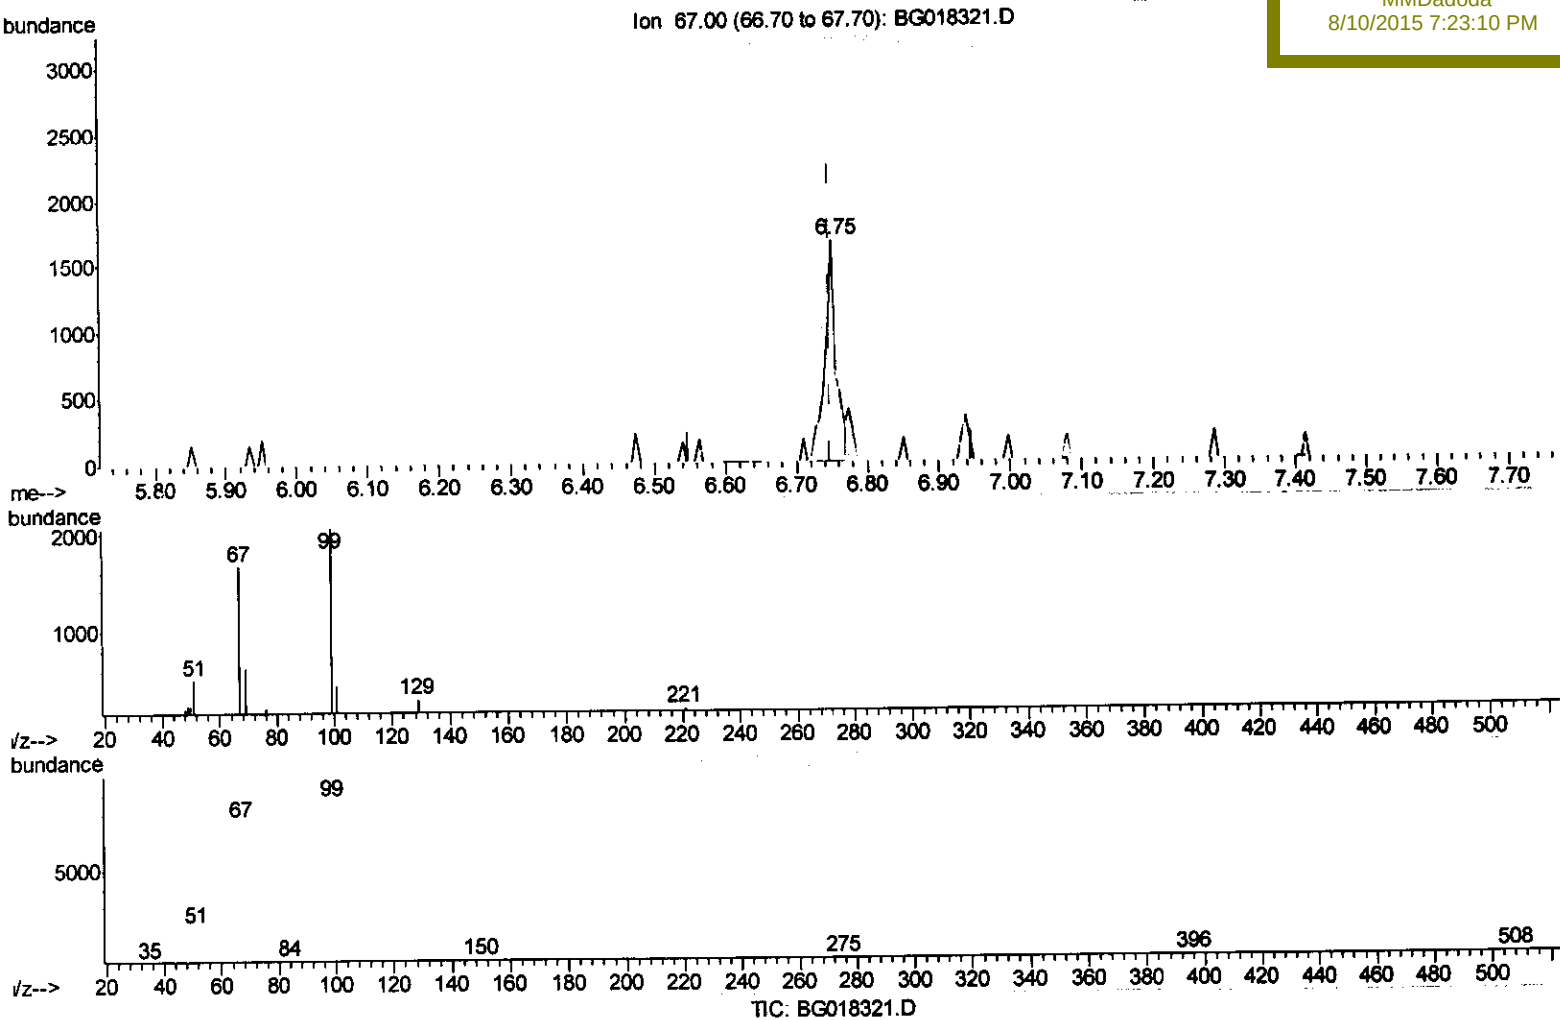

(7) Bis-(2-Chloroethyl)ether-d8 (S)

6.750min (+0.003) 2.57ng/ui

response 1843

Ion	Exp%	Act%
67.00	100	100
99.00	131.70	122.92
69.00	34.90	37.43
0.00	0.00	0.00


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080815\
 Data File : BG018321.D
 Acq On : 8 Aug 2015 9:00
 Operator : UM/TP
 Sample : G3095-08DL 5X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C01R8DL

Manual Integrations
 APPROVED

MMDadoda
 8/10/2015 7:23:10 PM

Quant Time: Aug 10 02:07:21 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 10 01:57:33 2015
 Response via : Initial Calibration

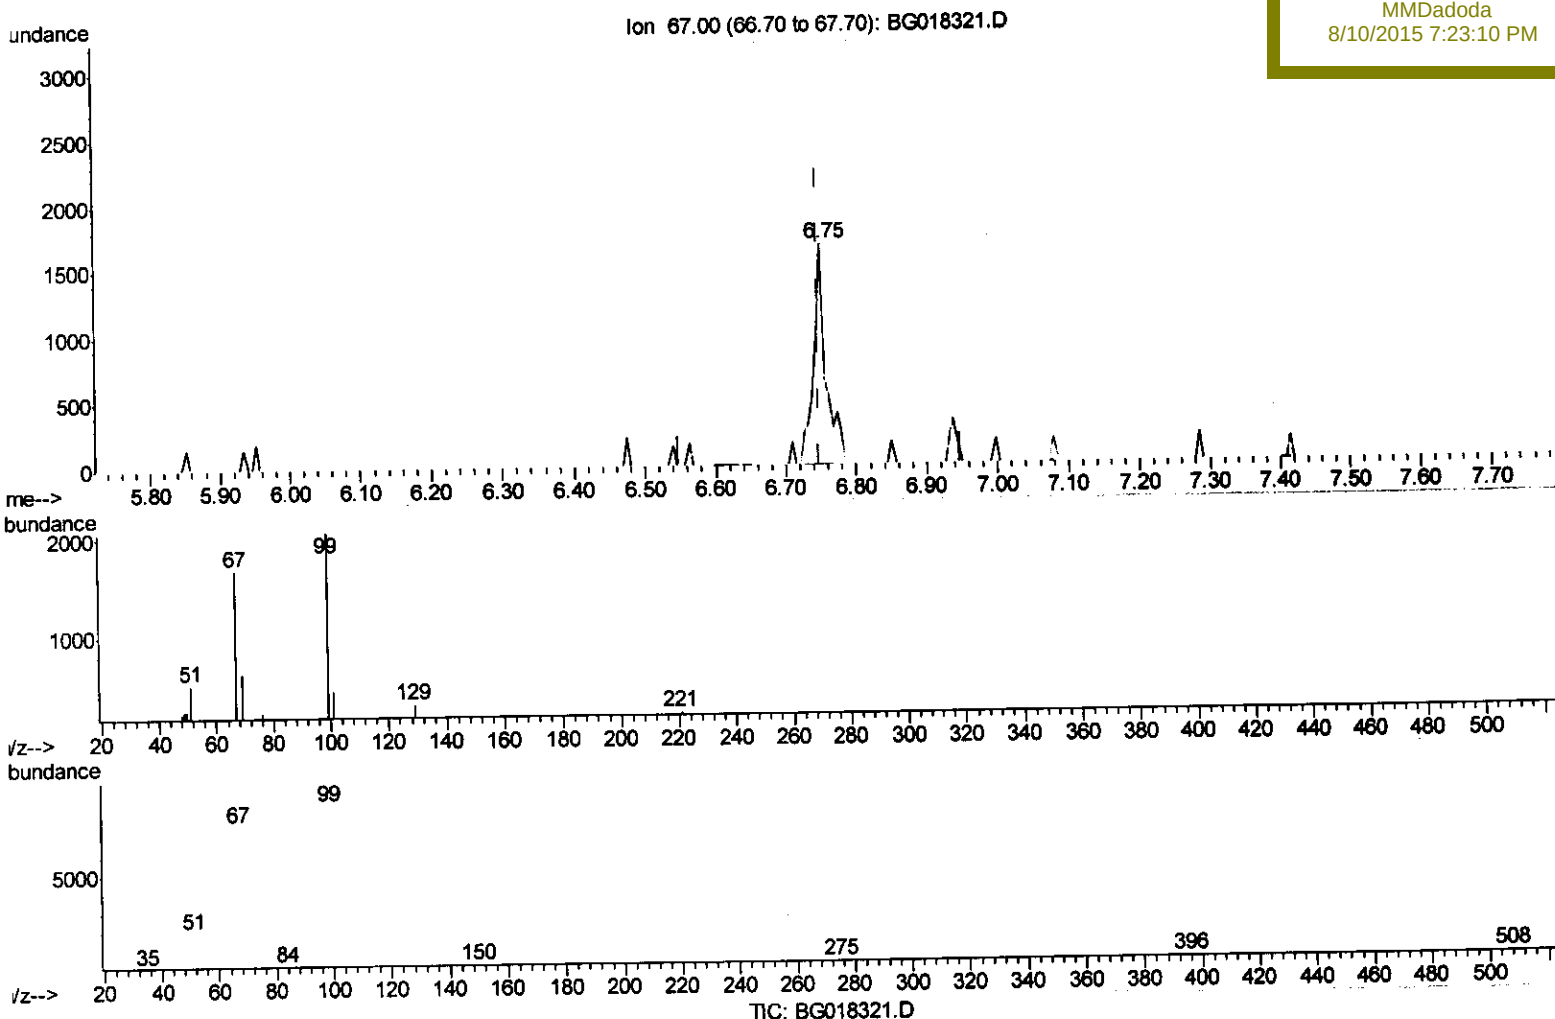

(7) Bis-(2-Chloroethyl)ether-d8 (S)

6.750min (+0.003) 2.87ng/ul m > 0.1M
 08111115

response 2063


Ion	Exp%	Act%
67.00	100	100
99.00	131.70	122.92
69.00	34.90	37.43
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080815\
Data File : BG018321.D
Acq On : 8 Aug 2015 9:00
Operator : UM/TP
Sample : G3095-08DL 5X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Aug 10 02:07:21 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080815.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 10 01:57:33 2015
Response via : Initial Calibration

Instrument :
BNA_G
ClientSampleId :
C01R8DL

Manual Integrations
APPROVED
MMDadoda
8/10/2015 7:23:10 PM

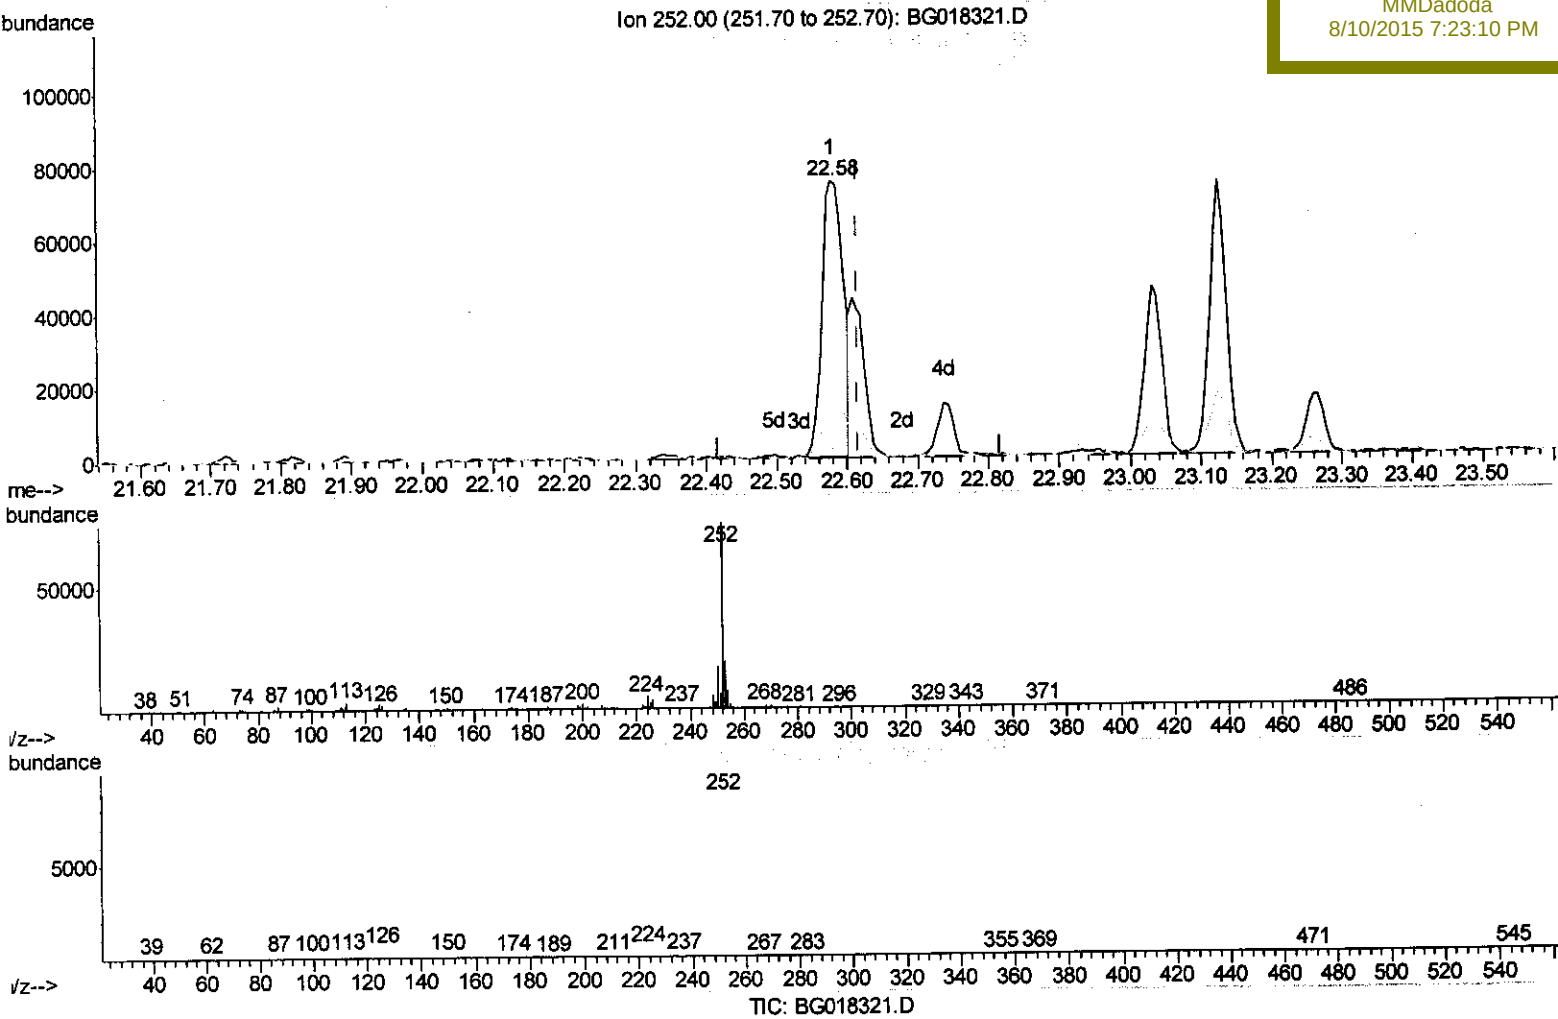

(89) Benzo(k)fluoranthene
22.579min (-0.038) 31.56ng/ul
response 160402


Ion	Exp%	Act%
252.00	100	100
253.00	21.70	25.85
125.00	4.10	3.73
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080815\
 Data File : BG018321.D
 Acq On : 8 Aug 2015 9:00
 Operator : UM/TP
 Sample : G3095-08DL 5X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Quant Time: Aug 10 02:07:21 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 10 01:57:33 2015
 Response via : Initial Calibration

Instrument :
 BNA_G
 ClientSampleId :
 C01R8DL

Manual Integrations
 APPROVED
 MMDadoda
 8/10/2015 7:23:10 PM

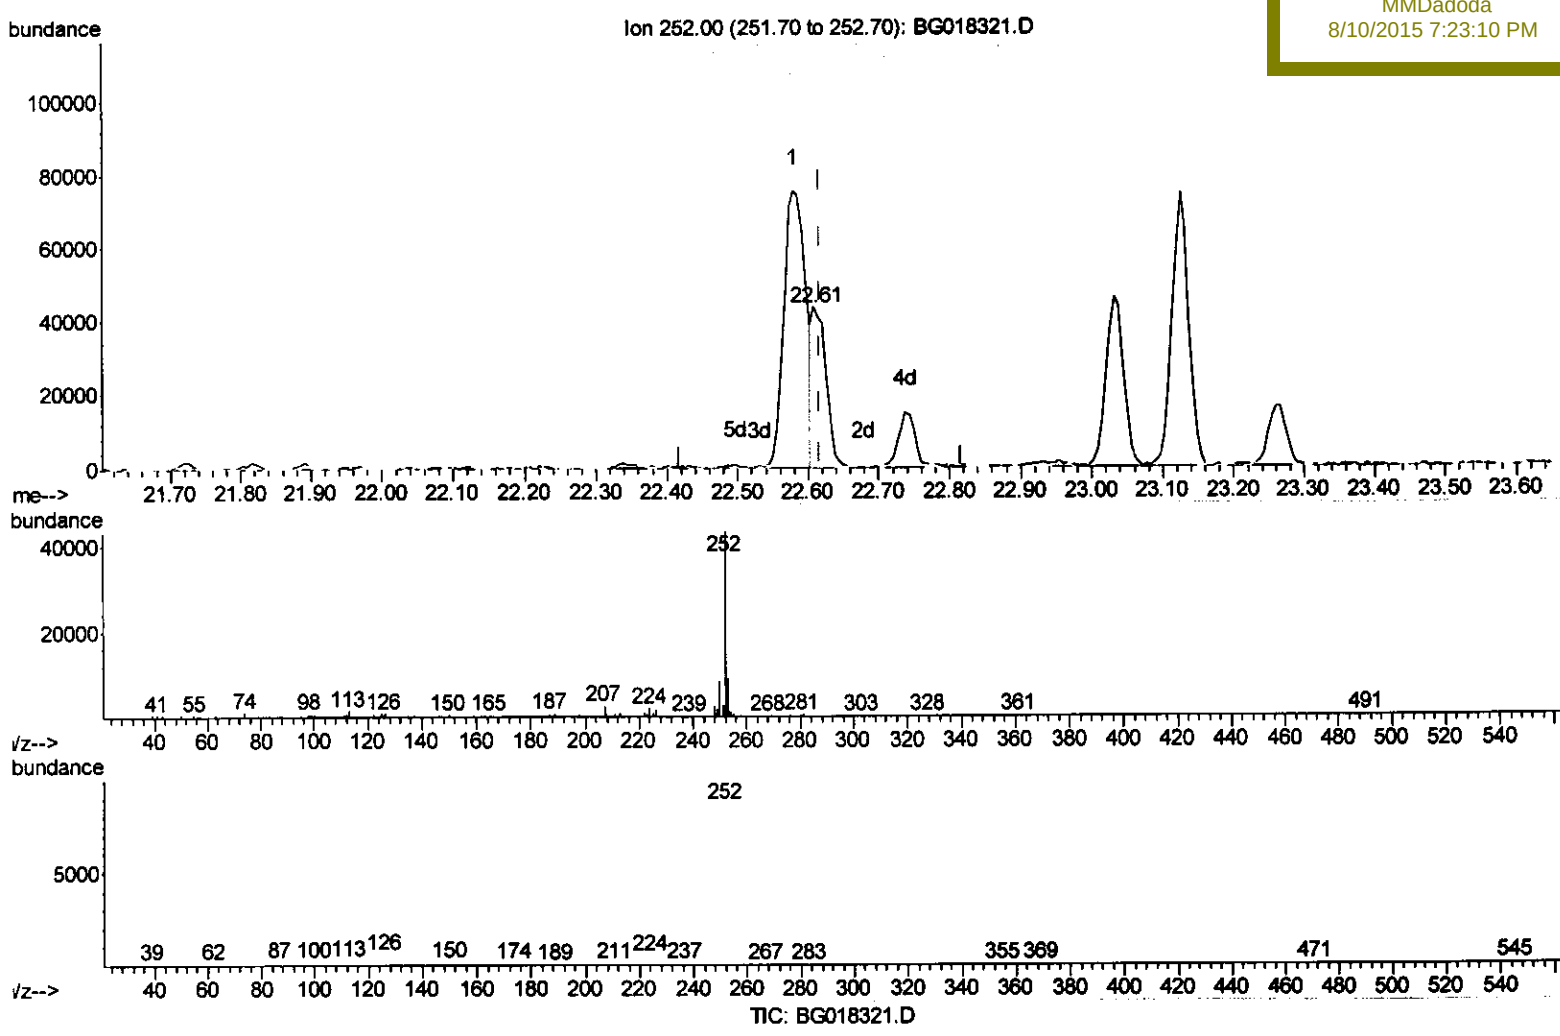

(89) Benzo(k)fluoranthene

22.608min (-0.009) 11.50ng/ul m > U.M
 0811115

response 58453

Ion	Exp%	Act%
252.00	100	100
253.00	21.70	20.65
125.00	4.10	2.50#
0.00	0.00	0.00


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080815\
 Data File : BG018321.D
 Acq On : 8 Aug 2015 9:00
 Operator : UM/TP
 Sample : G3095-08DL 5X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Quant Time: Aug 10 02:07:21 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 10 01:57:33 2015
 Response via : Initial Calibration

Instrument :
 BNA_G
 ClientSampleId :
 C01R8DL

Manual Integrations
 APPROVED

MMDadoda
 8/10/2015 7:23:10 PM

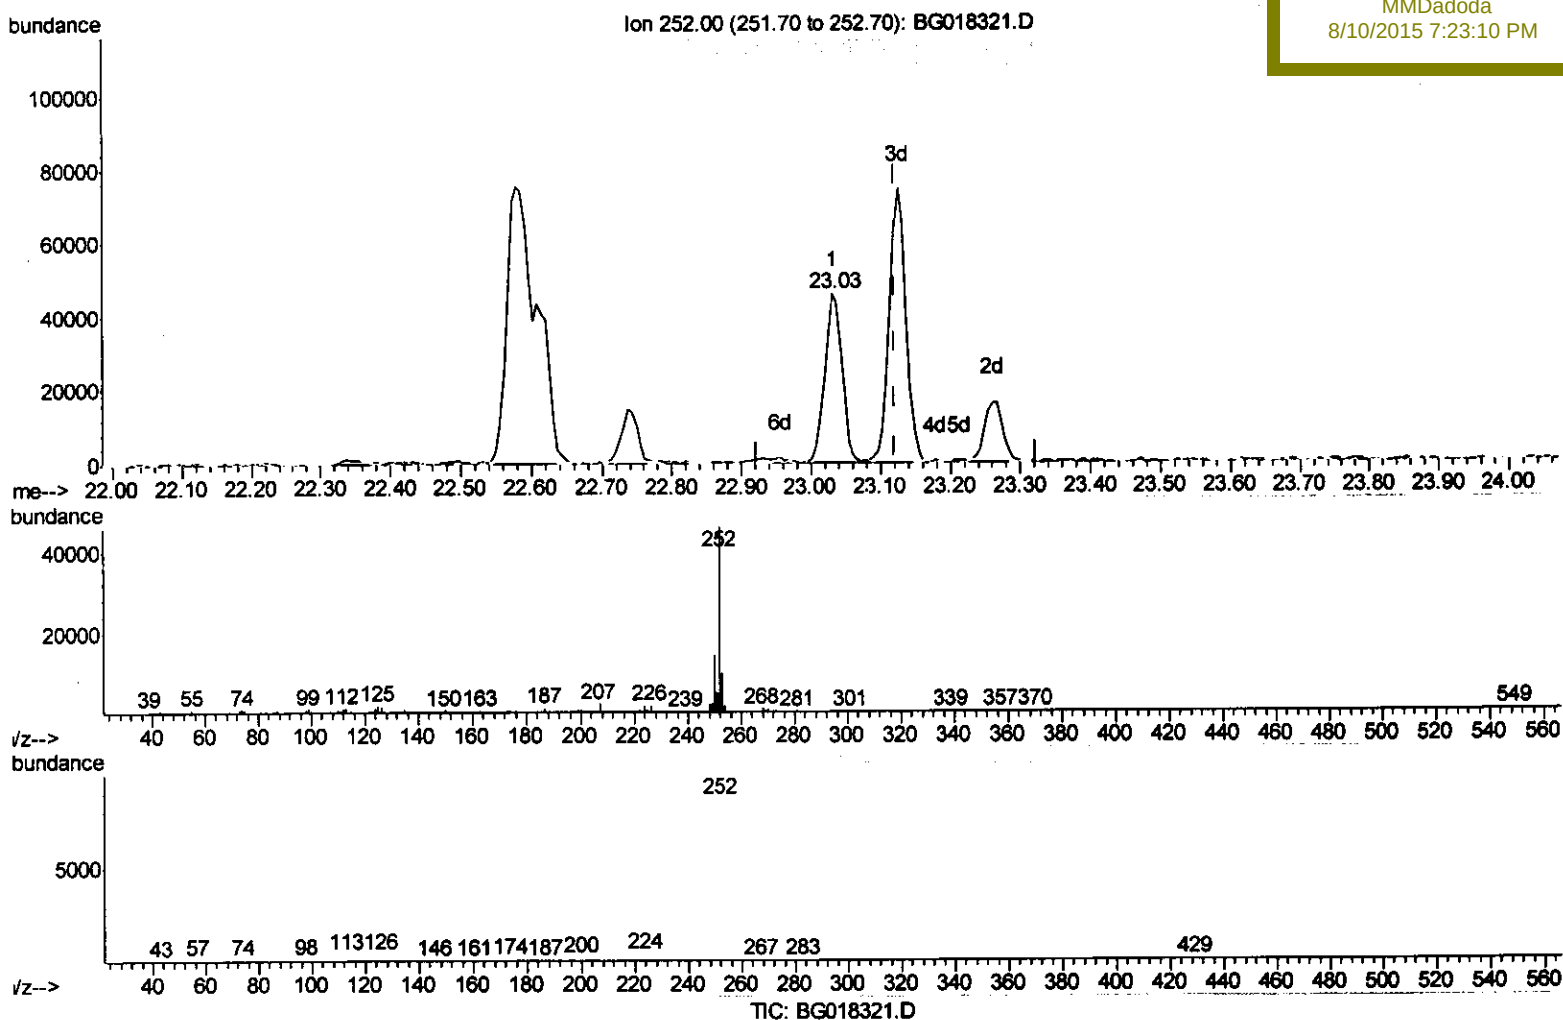

(91) Benzo(a)pyrene (C)

23.031min (-0.091) 16.30ng/ul

response 78096




Ion	Exp%	Act%
252.00	100	100
253.00	21.50	21.58
125.00	3.50	4.08
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080815\
 Data File : BG018321.D
 Acq On : 8 Aug 2015 9:00
 Operator : UM/TP
 Sample : G3095-08DL 5X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Quant Time: Aug 10 02:07:21 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 10 01:57:33 2015
 Response via : Initial Calibration

Instrument :
 BNA_G
 ClientSampleId :
 C01R8DL

Manual Integrations
 APPROVED
 MMDadoda
 8/10/2015 7:23:10 PM

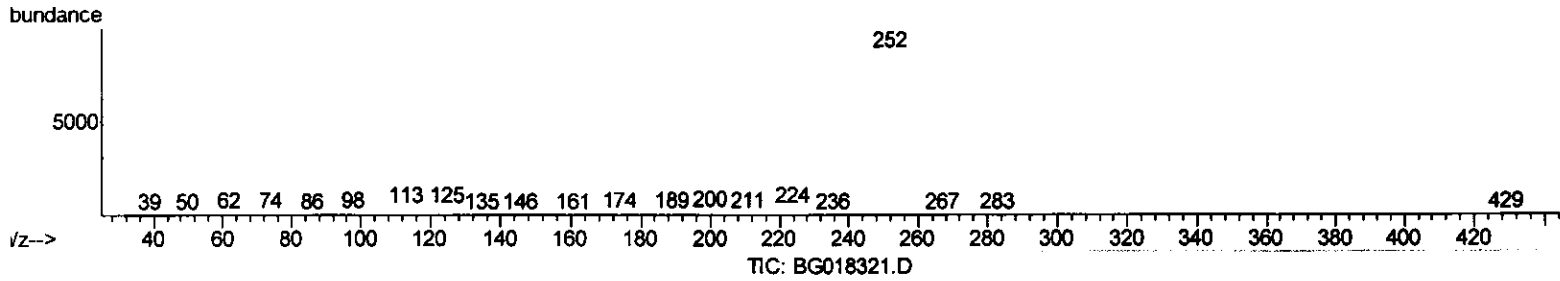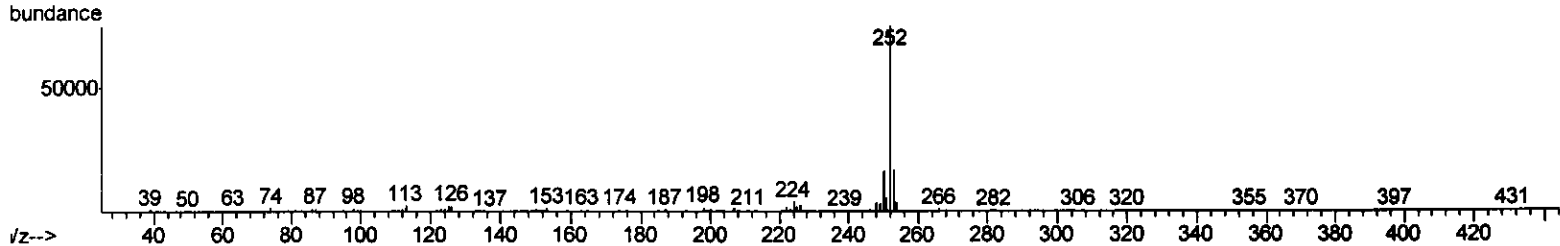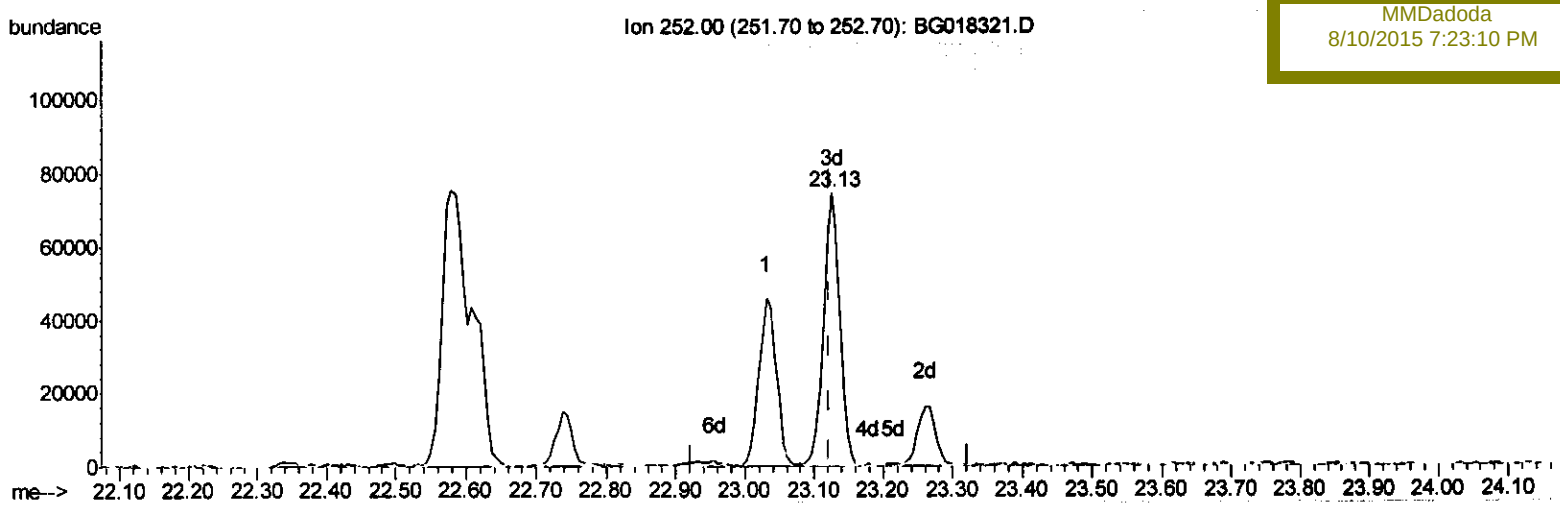

(91) Benzo(a)pyrene (C)

23.125min (+0.003) 25.53ng/ul m > U.M
 08/11/15

response 122334




Ion	Exp%	Act%
252.00	100	100
253.00	21.50	22.80
125.00	3.50	2.72#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080815\
 Data File : BG018321.D
 Acq On : 8 Aug 2015 9:00
 Operator : UM/TP
 Sample : G3095-08DL 5X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Quant Time: Aug 10 02:07:21 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 10 01:57:33 2015
 Response via : Initial Calibration

Instrument :
 BNA_G
 ClientSampleId :
 C01R8DL

Manual Integrations
 APPROVED
 MMDadoda
 8/10/2015 7:23:10 PM

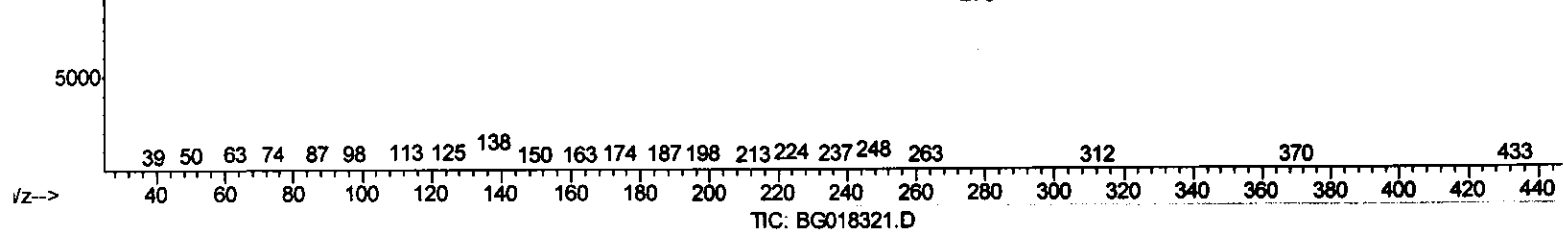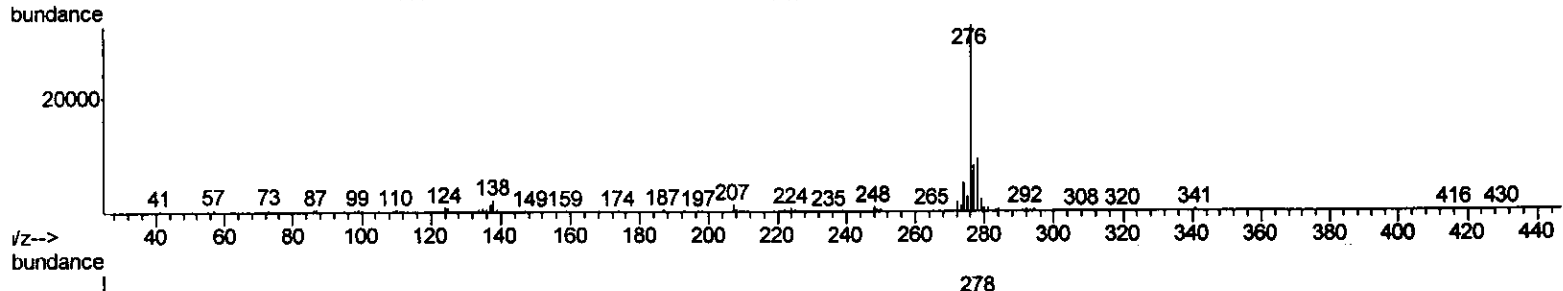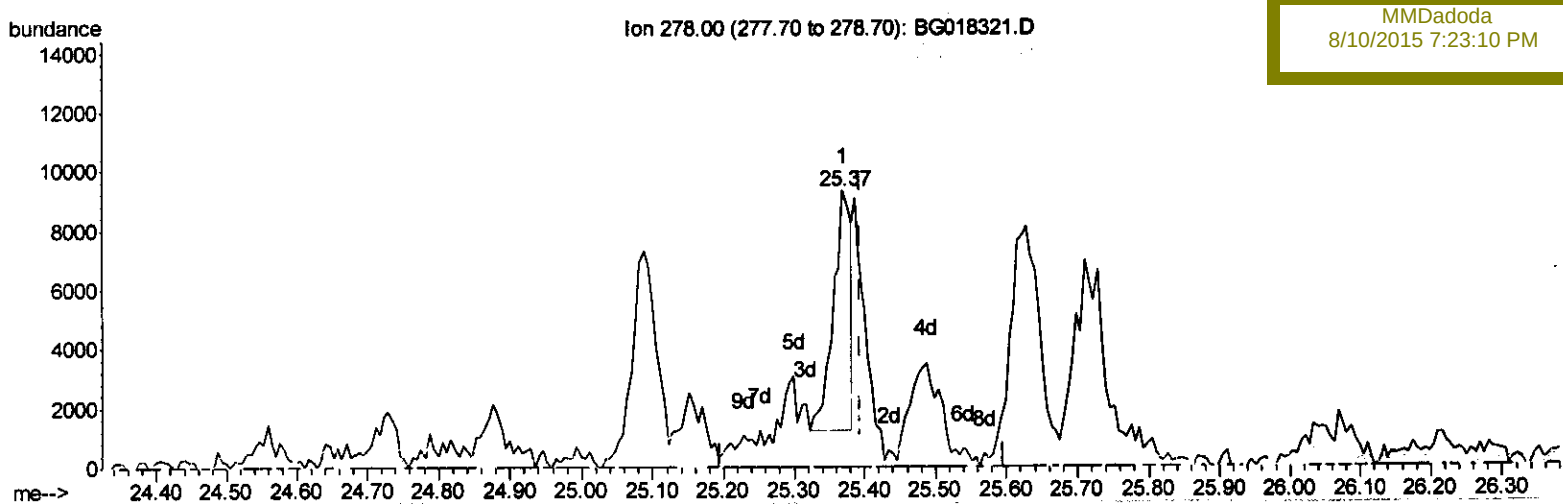

(93) Dibenzo(a,h)anthracene

25.370min (-0.026) 2.76ng/ul

response 14083

Ion	Exp%	Act%
278.00	100	100
139.00	6.70	7.17
279.00	22.80	25.29
0.00	0.00	0.00


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080815\
 Data File : BG018321.D
 Acq On : 8 Aug 2015 9:00
 Operator : UM/TP
 Sample : G3095-08DL 5X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C01R8DL

Quant Time: Aug 10 02:07:21 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080815.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 10 01:57:33 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 8/10/2015 7:23:10 PM

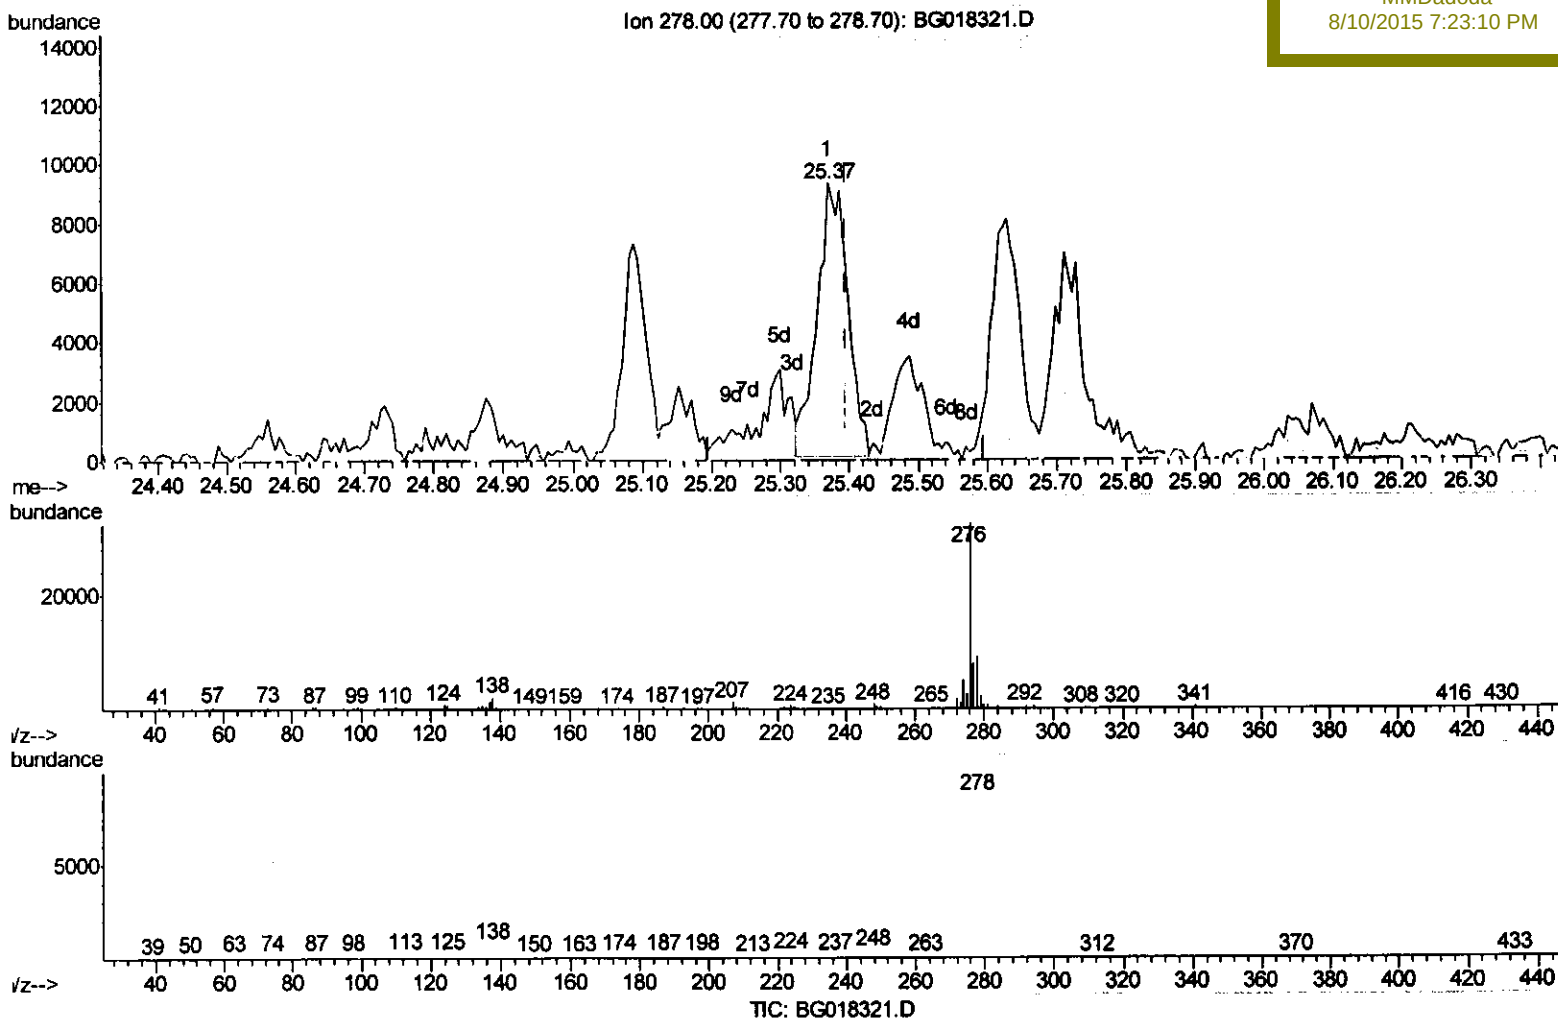

(93) Dibenzo(a,h)anthracene

25.370min (-0.026) 5.57ng/ul m

response 28393

Ion	Exp%	Act%
278.00	100	100
139.00	6.70	5.28#
279.00	22.80	25.29
0.00	0.00	0.00

U.M
 08/11/15

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080815\
Data File : BG018321.D
Acq On : 8 Aug 2015 9:00
Operator : UM/TP
Sample : G3095-08DL 5X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Aug 10 02:58:35 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080815.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 10 01:57:33 2015
Response via : Initial Calibration

Instrument :
BNA_G
ClientSampled :
C01R8DL

Manual Integrations
APPROVED

MMDadoda
8/10/2015 7:23:10 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	13444	20.00	ng/ul	0.00
18) Naphthalene-d8	10.19	136	65824	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.09	164	43417	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.85	188	95870	20.00	ng/ul	0.00
78) Chrysene-d12	21.07	240	72900	20.00	ng/ul	0.00
86) Perylene-d12	23.22	264	70232	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	6.62	99	3455	2.77	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.75	67	2063m	2.87	ng/ul	0.00
9) 2-Chlorophenol-d4	6.95	132	2728	2.65	ng/ul	0.00
13) 4-Methylphenol-d8	8.14	113	2826	2.65	ng/ul	0.00
19) Nitrobenzene-d5	8.55	128	1364	2.28	ng/ul	0.00
22) 2-Nitrophenol-d4	9.28	143	1662	2.41	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.84	165	3080	2.42	ng/ul	0.00
29) 4-Chloroaniline-d4	10.35	131	1367	0.97	ng/ul	0.00
44) Dimethylphthalate-d6	13.51	166	12432	2.84	ng/ul	0.00
47) Acenaphthylene-d8	13.78	160	14477	2.99	ng/ul	0.00
52) 4-Nitrophenol-d4	14.37	143	499	0.90	ng/ul	0.02
58) Fluorene-d10	15.09	176	12142	3.17	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	0.00	200	0d	0.00	ng/ul	
71) Anthracene-d10	16.95	188	15056	2.91	ng/ul	0.00
79) Pyrene-d10	19.27	212	14137	3.35	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.08	264	12253	2.70	ng/ul	0.00

U.M
08/11/15

Target Compounds					Qvalue
28) Naphthalene	10.23	128	4785	1.27 ng/ul#	91
48) Acenaphthylene	13.81	152	6963	1.44 ng/ul	94
50) Acenaphthene	14.15	153	8223	2.53 ng/ul#	89
54) Dibenzofuran	14.49	168	5561	1.16 ng/ul	96
59) Fluorene	15.15	166	10217	2.46 ng/ul	88
70) Phenanthrene	16.89	178	199715	33.31 ng/ul	98
72) Anthracene	16.99	178	41059	6.81 ng/ul	99
75) Carbazole	17.26	167	11405	2.45 ng/ul#	93
77) Fluoranthene	18.93	202	334741	51.20 ng/ul#	98
80) Pyrene	19.29	202	321129	60.44 ng/ul	98
83) Benzo(a)anthracene	21.05	228	134189	27.04 ng/ul	96
84) Bis(2-ethylhexyl)phthalate	21.00	149	128877	41.00 ng/ul#	96
85) Chrysene	21.10	228	129591	28.23 ng/ul#	91
88) Benzo(b)fluoranthene	22.58	252	160402	30.15 ng/ul#	89
89) Benzo(k)fluoranthene	22.61	252	58453m	11.50 ng/ul	
91) Benzo(a)pyrene	23.13	252	122334m	25.53 ng/ul	
92) Indeno(1,2,3-cd)pyrene	25.38	276	95408	16.30 ng/ul	98
93) Dibenzo(a,h)anthracene	25.37	278	28393m	5.57 ng/ul	
94) Benzo(g,h,i)perylene	26.05	276	89347	18.74 ng/ul	94

U.M
08/11/15
U.M
08/11/15

(#) = qualifier out of range (m) = manual integration (+) = signals summed