

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080816\
 Data File : BG023551.D
 Acq On : 9 Aug 2016 2:12
 Operator : UM/SJ
 Sample : PB92715BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK15

Quant Time: Aug 09 04:45:42 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 09 02:15:40 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	135983	20.00	ng/ul	0.00
18) Naphthalene-d8	10.94	136	630394	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.78	164	467292	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.54	188	1178820	20.00	ng/ul	0.00
75) Chrysene-d12	21.85	240	1159260	20.00	ng/ul	0.00
83) Perylene-d12	25.23	264	1091325	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.49	96	17894	5.59	ng/uL	0.00
5) Phenol-d5	7.27	99	493350	36.01	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.43	67	329905	37.59	ng/ul	0.00
9) 2-Chlorophenol-d4	7.64	132	345437	36.96	ng/ul	0.00
13) 4-Methylphenol-d8	8.83	113	399093	37.32	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	193289	38.90	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	232005	40.65	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.57	165	388065	36.05	ng/ul	0.00
29) 4-Chloroaniline-d4	11.31	131	878	0.07	ng/ul	0.22
43) Dimethylphthalate-d6	14.17	166	1421981	37.17	ng/ul	0.00
46) Acenaphthylene-d8	14.47	160	1612174	37.44	ng/ul	0.00
51) 4-Nitrophenol-d4	14.99	143	238875	36.57	ng/ul	0.00
57) Fluorene-d10	15.77	176	1288994	36.46	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	281503	37.22	ng/ul	0.00
70) Anthracene-d10	17.64	188	1941053	36.55	ng/ul	0.00
76) Pyrene-d10	19.93	212	2095747	35.71	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.00	264	1976524	40.01	ng/ul	0.00


Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	8.83	70	11899	1.15 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080816\
Data File : BG023551.D
Acq On : 9 Aug 2016 2:12
Operator : UM/SJ
Sample : PB92715BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK15

Quant Time: Aug 09 04:45:42 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 09 02:15:40 2016
Response via : Initial Calibration

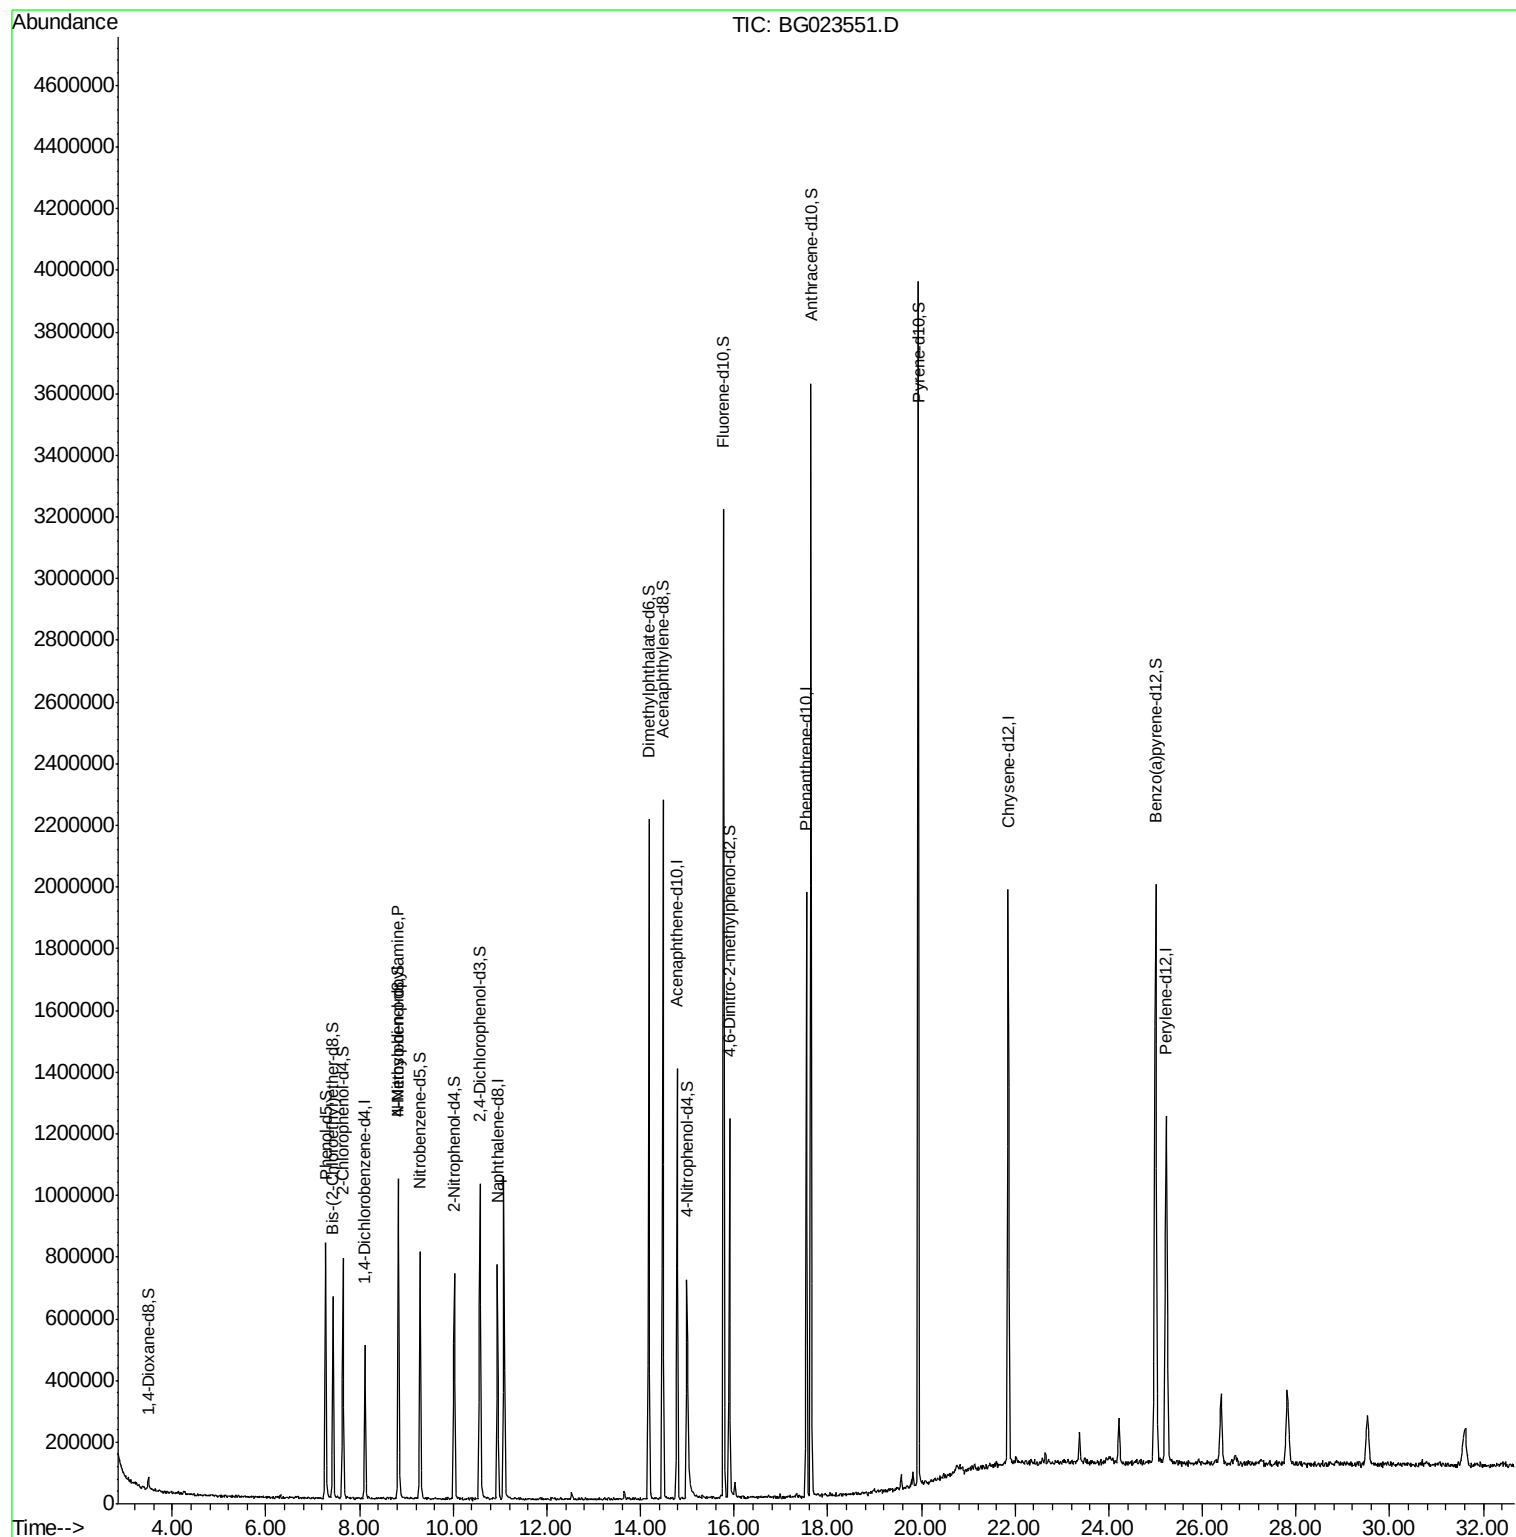

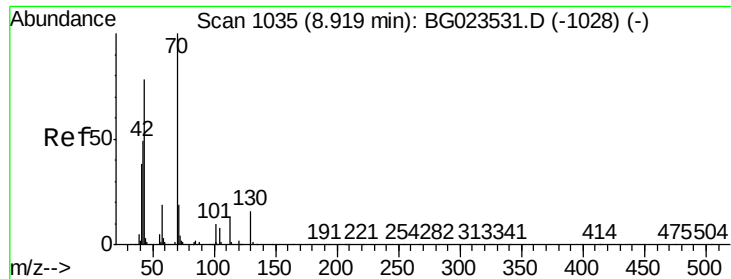

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.15 ng/ul
 RT: 8.83 min Scan# 1020
 Delta R.T. -0.09 min
 Lab File: BG023551.D
 Acq: 9 Aug 2016 2:12

Instrument :
 BNA_G
 ClientSampleId :
 SBLK15

Tgt Ion	Ratio	Lower	Upper
70	100		
42	354.1	31.4	47.2#
101	0.0	8.6	13.0#
130	0.0	19.0	28.4#

