

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080816\
 Data File : BG023549.D
 Acq On : 9 Aug 2016 00:53
 Operator : UM/SJ
 Sample : H4338-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4V16

Manual Integrations
 APPROVED

sohil
 8/9/2016 6:20:29 PM

Quant Time: Aug 09 05:53:56 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Aug 09 02:15:40 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	146750	20.00	ng/ul	0.00
18) Naphthalene-d8	10.95	136	678069	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.78	164	482012	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.54	188	1030643	20.00	ng/ul	0.00
75) Chrysene-d12	21.85	240	1025643	20.00	ng/ul	0.00
83) Perylene-d12	25.23	264	1016727	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.49	96	2354	0.68	ng/uL	0.01
5) Phenol-d5	7.27	99	115812	7.83	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.43	67	285170	30.11	ng/ul	0.00
9) 2-Chlorophenol-d4	7.64	132	265862	26.36	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	212704	18.43	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	169668m	31.74	ng/ul	0.00
22) 2-Nitrophenol-d4	10.02	143	199944	32.57	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.57	165	371420	32.08	ng/ul	0.00
29) 4-Chloroaniline-d4	11.10	131	20141m	1.48	ng/ul	0.01
43) Dimethylphthalate-d6	14.17	166	1260226	31.93	ng/ul	0.00
46) Acenaphthylene-d8	14.47	160	1438483	32.39	ng/ul	0.00
51) 4-Nitrophenol-d4	15.01	143	59998m	8.91	ng/ul	0.03
57) Fluorene-d10	15.77	176	1151339	31.57	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	239390	36.20	ng/ul	0.00
70) Anthracene-d10	17.64	188	1621866	34.93	ng/ul	0.00
76) Pyrene-d10	19.93	212	1681724	32.39	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.00	264	1637149	35.57	ng/ul	0.00

Target Compounds					Qvalue
44) Dimethylphthalate	14.22	163	130624	3.34 ng/ul#	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080816\
Data File : BG023549.D
Acq On : 9 Aug 2016 00:53
Operator : UM/SJ
Sample : H4338-06
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
A4V16

Manual Integrations
APPROVED

sohil
8/9/2016 6:20:29 PM

Quant Time: Aug 09 05:53:56 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG080416.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Aug 09 02:15:40 2016
Response via : Initial Calibration

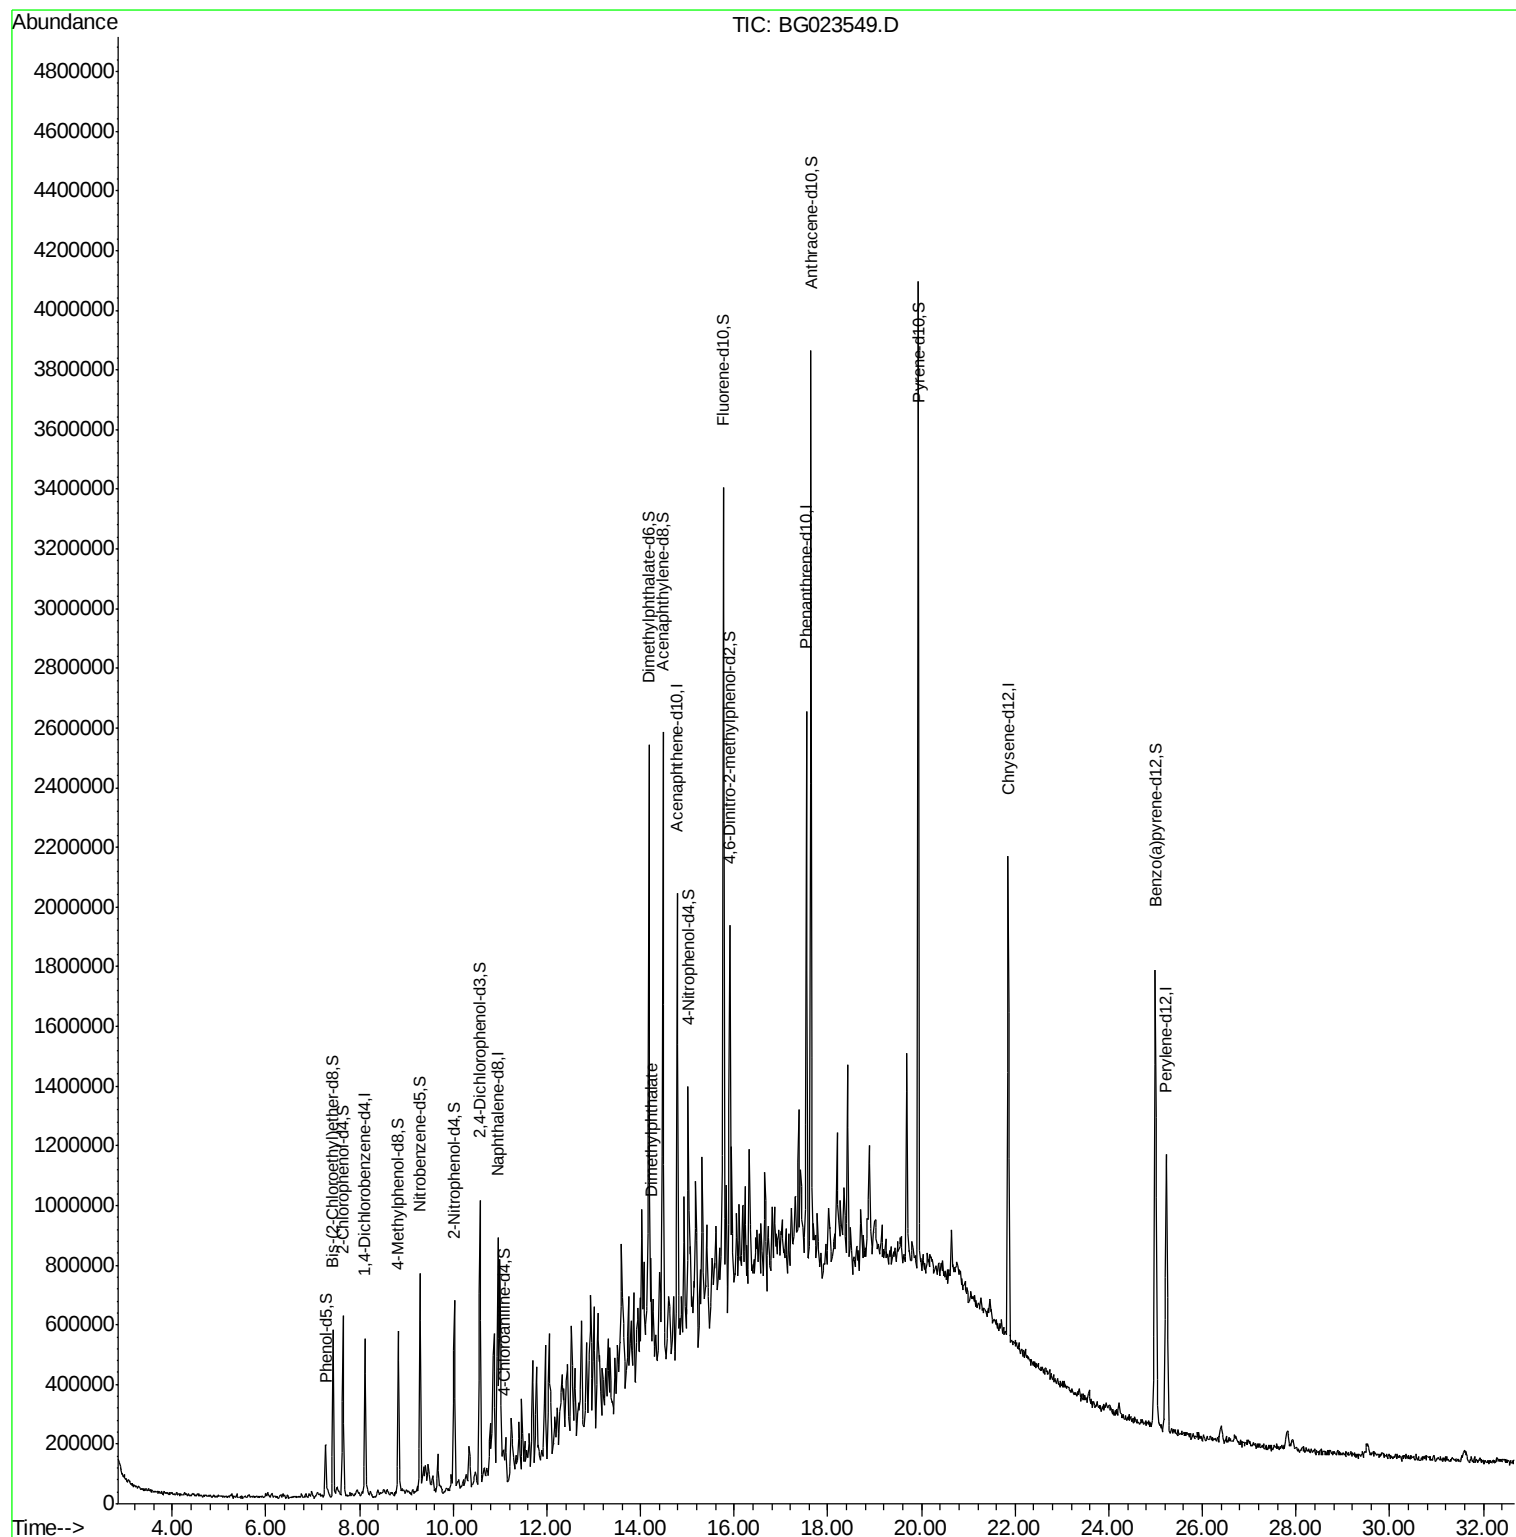

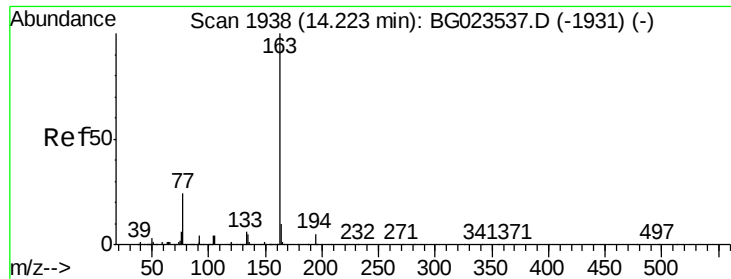

#44
 Dimethylphthalate
 Concen: 3.34 ng/ul
 RT: 14.22 min Scan# 1938
 Delta R.T. -0.00 min
 Lab File: BG023549.D
 Acq: 9 Aug 2016 00:53

Instrument :
 BNA_G
 ClientSampleId :
 A4V16

Tgt Ion	Ratio	Resp	Lower	Upper
163	100	130624		
194	3.2		3.4	5.2#
164	11.4		8.8	13.2

Manual Integrations
 APPROVED

sohil
 8/9/2016 6:20:29 PM

