

Data Path : Z:\HPCHEM1\BNA G\DATA\BG080817\
 Data File : BG028189.D
 Acq On : 8 Aug 2017 14:27
 Operator : SJ/JU
 Sample : PB101301BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Aug 09 01:12:17 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 09 01:09:22 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.35	152	33674	20.00	ng/ul	0.00
18) Naphthalene-d8	11.17	136	154062	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.96	164	116286	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.71	188	323585	20.00	ng/ul	0.00
75) Chrysene-d12	22.04	240	340148	20.00	ng/ul	0.00
83) Perylene-d12	25.55	264	326619	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.84	96	5193	7.18	ng/uL	0.00
5) Phenol-d5	7.50	99	103235	27.91	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.67	67	74118	31.65	ng/ul	0.00
9) 2-Chlorophenol-d4	7.89	132	75364	32.30	ng/ul	0.00
13) 4-Methylphenol-d8	9.05	113	85876	27.78	ng/ul	0.00
19) Nitrobenzene-d5	9.52	128	39913	33.13	ng/ul	0.00
22) 2-Nitrophenol-d4	10.24	143	46355	35.09	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.78	165	82951	30.35	ng/ul	0.00
29) 4-Chloroaniline-d4	11.31	131	115199	37.87	ng/ul	0.00
43) Dimethylphthalate-d6	14.35	166	385481	37.27	ng/ul	0.00
46) Acenaphthylene-d8	14.66	160	386622	33.15	ng/ul	0.00
51) 4-Nitrophenol-d4	15.15	143	50662	30.81	ng/ul	0.00
57) Fluorene-d10	15.95	176	306370	33.02	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.06	200	66957	31.85	ng/ul	0.00
70) Anthracene-d10	17.81	188	560296	36.11	ng/ul	0.00
76) Pyrene-d10	20.09	212	651572	37.35	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.31	264	542798	35.50	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	9.04	70	2598	1.037	ng/ul# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG080817\
Data File : BG028189.D
Acq On : 8 Aug 2017 14:27
Operator : SJ/JU
Sample : PB101301BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Aug 09 01:12:17 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 09 01:09:22 2017
Response via : Initial Calibration

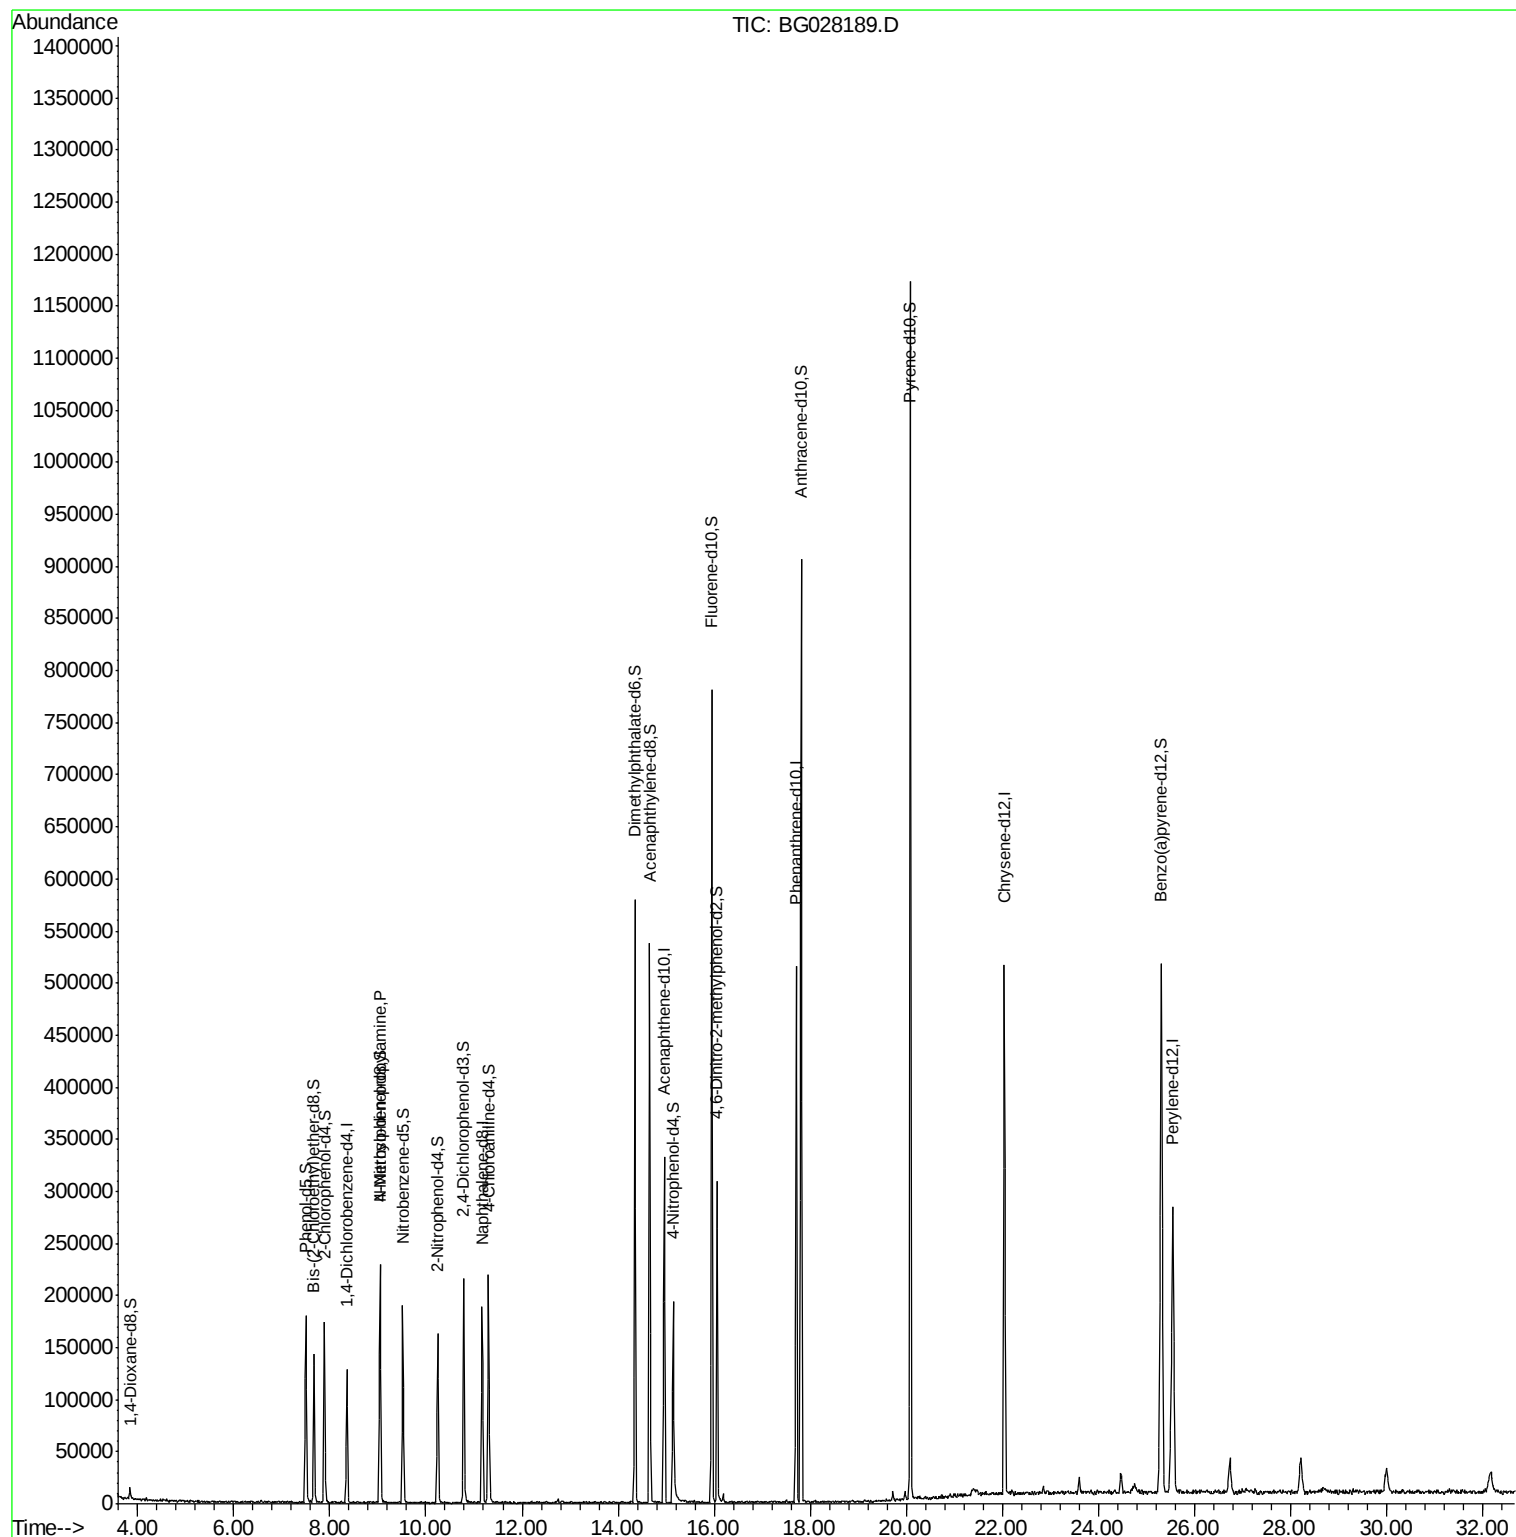

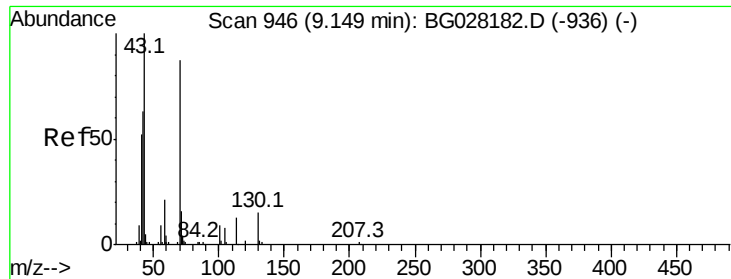

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.037 ng/ul
 RT: 9.04 min Scan# 928
 Delta R.T. -0.11 min
 Lab File: BG028189.D
 Acq: 8 Aug 2017 14:27

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion: 70 Resp: 2598
 Ion Ratio Lower Upper
 70 100
 42 343.3 59.0 88.6#
 101 0.0 6.6 9.8#
 130 0.0 15.6 23.4#

