

Data Path : Z:\HPCHEM1\BNA G\DATA\BG080817\
 Data File : BG028201.D
 Acq On : 8 Aug 2017 22:22
 Operator : SJ/JU
 Sample : PB101302BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Aug 09 02:34:36 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 09 02:30:54 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.35	152	34094	20.00	ng/ul	0.00
18) Naphthalene-d8	11.17	136	151892	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.96	164	112810	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.71	188	325648	20.00	ng/ul	0.00
75) Chrysene-d12	22.04	240	371303	20.00	ng/ul	0.00
83) Perylene-d12	25.55	264	355622	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.84	96	5785	7.90	ng/uL	0.00
5) Phenol-d5	7.50	99	106296	28.39	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.67	67	78265	33.00	ng/ul	0.00
9) 2-Chlorophenol-d4	7.89	132	78457	33.21	ng/ul	0.00
13) 4-Methylphenol-d8	9.05	113	91783	29.33	ng/ul	0.00
19) Nitrobenzene-d5	9.53	128	41471	34.92	ng/ul	0.00
22) 2-Nitrophenol-d4	10.25	143	49445	37.97	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.79	165	86744	32.19	ng/ul	0.00
29) 4-Chloroaniline-d4	11.30	131	119391	39.81	ng/ul	0.00
43) Dimethylphthalate-d6	14.35	166	390591	38.93	ng/ul	0.00
46) Acenaphthylene-d8	14.66	160	399396	35.31	ng/ul	0.00
51) 4-Nitrophenol-d4	15.15	143	54175	33.96	ng/ul	0.00
57) Fluorene-d10	15.95	176	313425	34.82	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.06	200	71803	33.94	ng/ul	0.00
70) Anthracene-d10	17.81	188	591344	37.87	ng/ul	0.00
76) Pyrene-d10	20.08	212	720782	37.85	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.30	264	624515	37.51	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	9.04	70	2671	1.053	ng/ul# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG080817\
Data File : BG028201.D
Acq On : 8 Aug 2017 22:22
Operator : SJ/JU
Sample : PB101302BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Aug 09 02:34:36 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG080217.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 09 02:30:54 2017
Response via : Initial Calibration

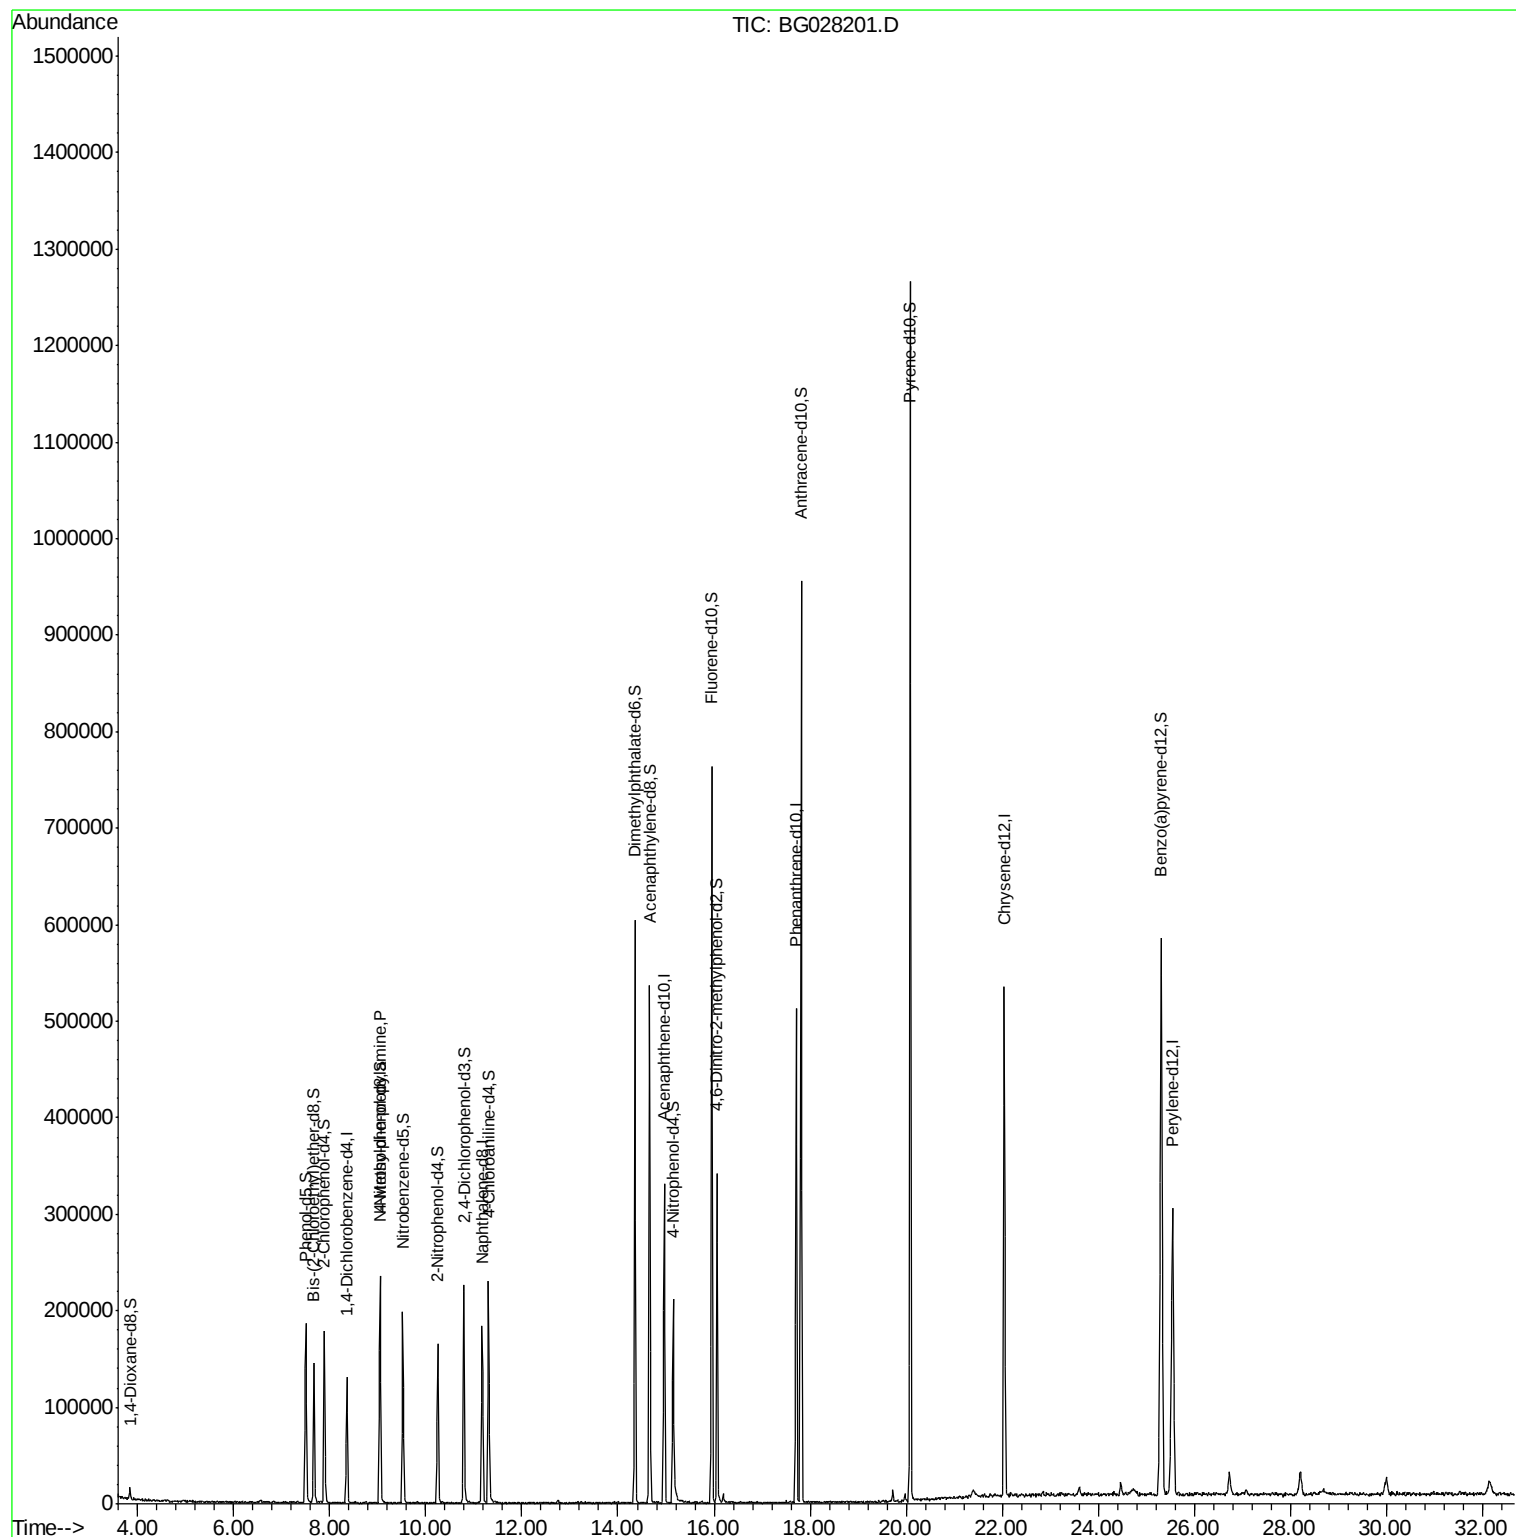

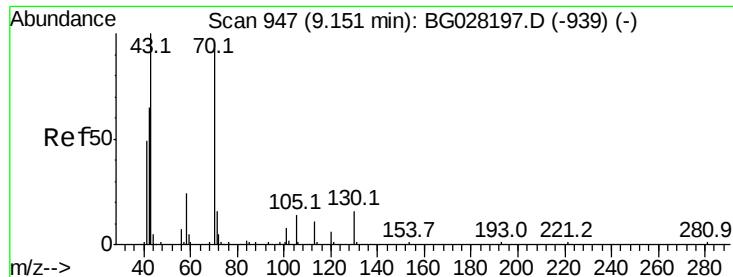

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.053 ng/ul
 RT: 9.04 min Scan# 927
 Delta R.T. -0.12 min
 Lab File: BG028201.D
 Acq: 8 Aug 2017 22:22

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion: 70 Resp: 2671
 Ion Ratio Lower Upper
 70 100
 42 278.2 59.0 88.6#
 101 0.0 6.6 9.8#
 130 0.0 15.6 23.4#

