

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080817\
 Data File : BG028215.D
 Acq On : 9 Aug 2017 7:35
 Operator : SJ/JU
 Sample : I4557-07
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AJ0

Quant Time: Aug 09 08:26:37 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Aug 09 08:20:51 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.36	152	38249	20.00	ng/ul	0.00
18) Naphthalene-d8	11.17	136	171889	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.96	164	128415	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.71	188	340792	20.00	ng/ul	0.00
75) Chrysene-d12	22.04	240	377394	20.00	ng/ul	0.00
83) Perylene-d12	25.54	264	359658	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.83	96	5031	6.13	ng/uL	0.00
5) Phenol-d5	7.50	99	34353	8.18	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.67	67	76931	28.92	ng/ul	0.00
9) 2-Chlorophenol-d4	7.88	132	71420	26.95	ng/ul	0.00
13) 4-Methylphenol-d8	9.05	113	61675	17.57	ng/ul	0.00
19) Nitrobenzene-d5	9.52	128	44867	33.38	ng/ul	0.00
22) 2-Nitrophenol-d4	10.24	143	53437	36.26	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.79	165	103946	34.09	ng/ul	0.00
29) 4-Chloroaniline-d4	11.33	131	68	0.02	ng/ul	0.02
43) Dimethylphthalate-d6	14.35	166	421922	36.94	ng/ul	0.00
46) Acenaphthylene-d8	14.66	160	445659	34.61	ng/ul	0.00
51) 4-Nitrophenol-d4	15.15	143	18034	9.93	ng/ul	0.00
57) Fluorene-d10	15.95	176	350748	34.23	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.06	200	78200	35.32	ng/ul	0.00
70) Anthracene-d10	17.81	188	589826	36.09	ng/ul	0.00
76) Pyrene-d10	20.08	212	706101	36.48	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.30	264	608022	36.11	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	14.40	163	10814	1.028 ng/ul#	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080817\
Data File : BG028215.D
Acq On : 9 Aug 2017 7:35
Operator : SJ/JU
Sample : I4557-07
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AJ0

Quant Time: Aug 09 08:26:37 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Aug 09 08:20:51 2017
Response via : Initial Calibration

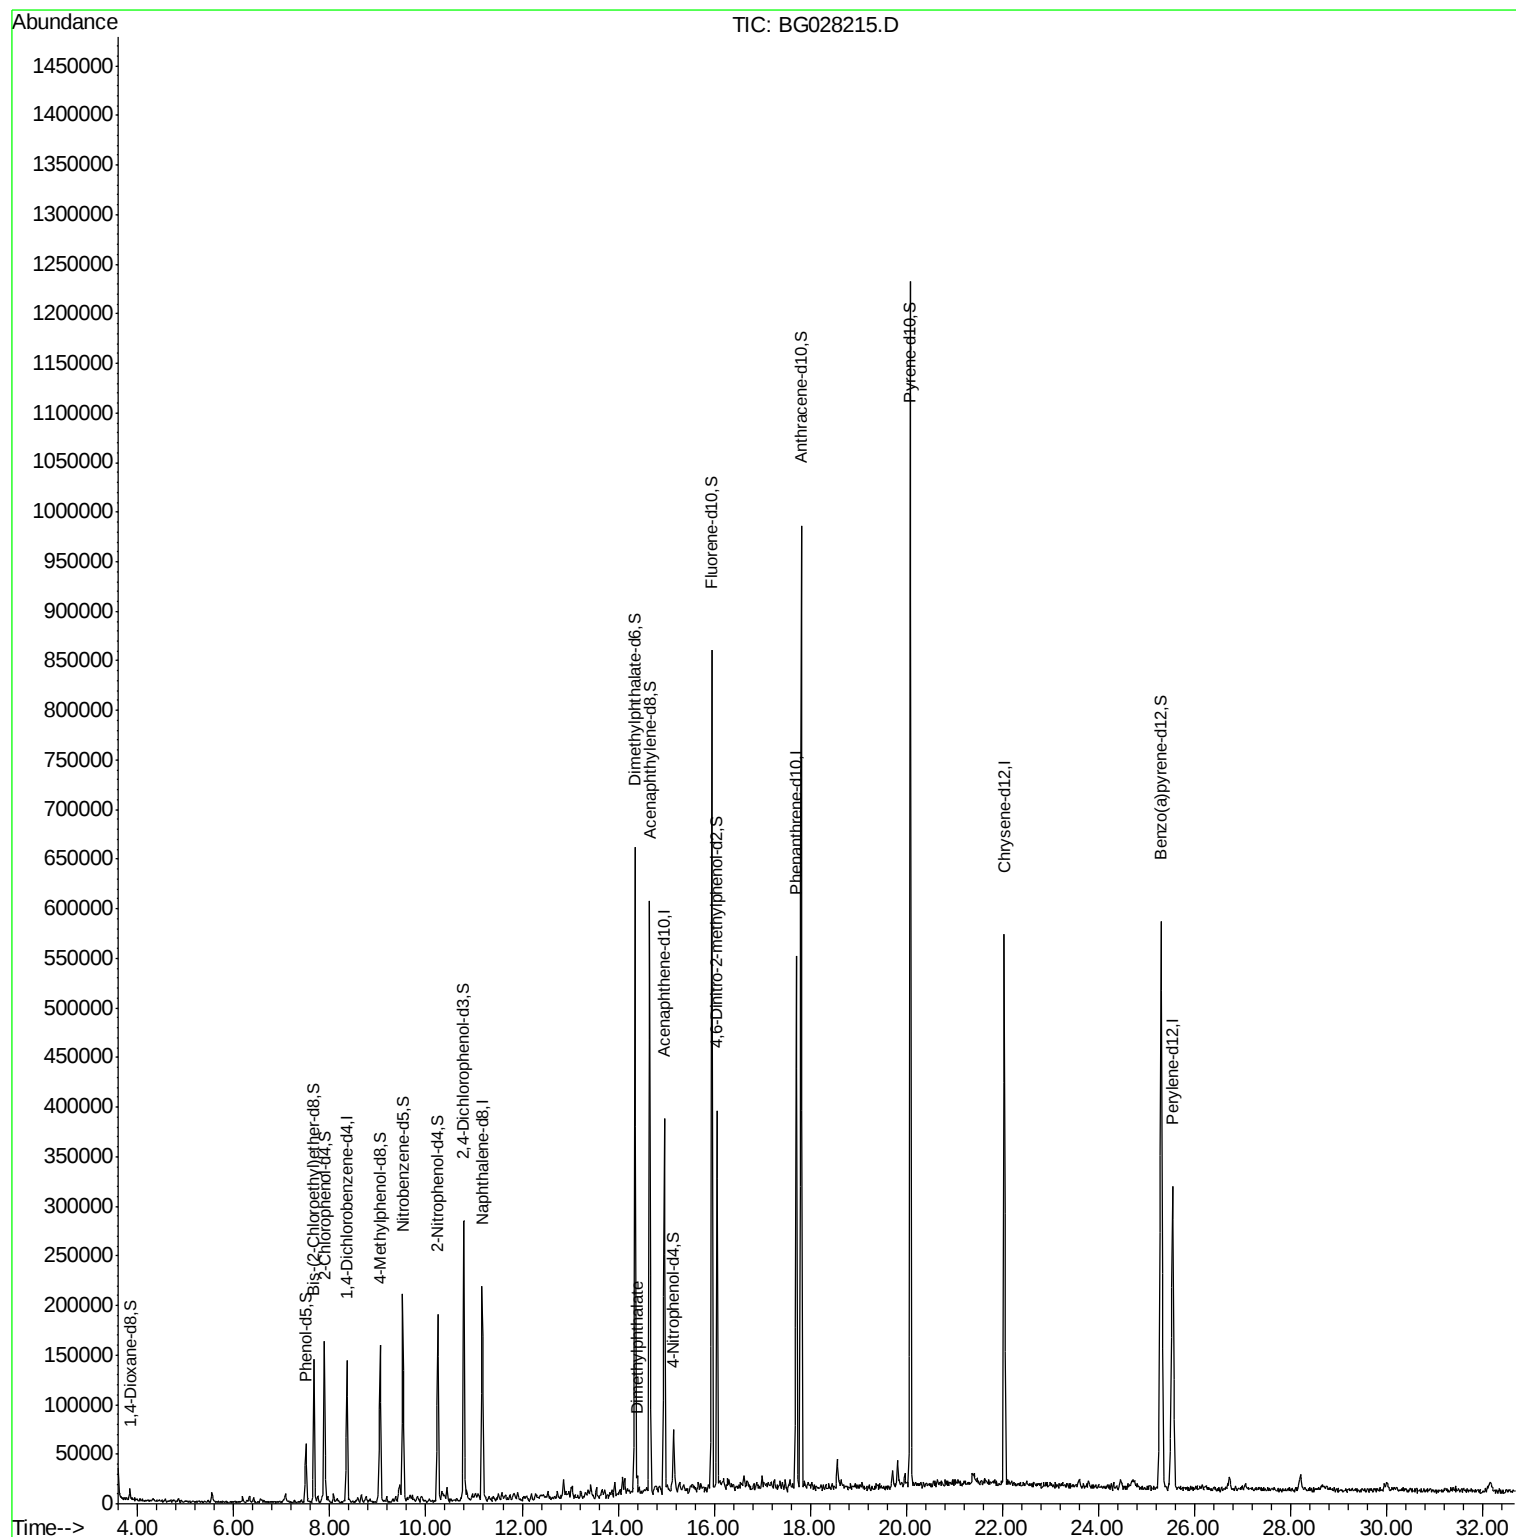

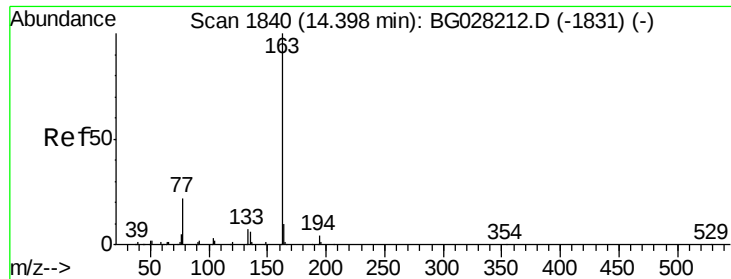

#44

Dimethylphthalate

Concen: 1.028 ng/ul

RT: 14.40 min Scan# 1840

Delta R.T. 0.00 min

Lab File: BG028215.D

Acq: 9 Aug 2017 7:35

Instrument :

BNA_G

ClientSampleId :

C0AJ0


Tgt Ion:163 Resp: 10814

Ion Ratio Lower Upper

163 100

194 3.9 3.4 5.0

164 8.7 9.0 13.4#

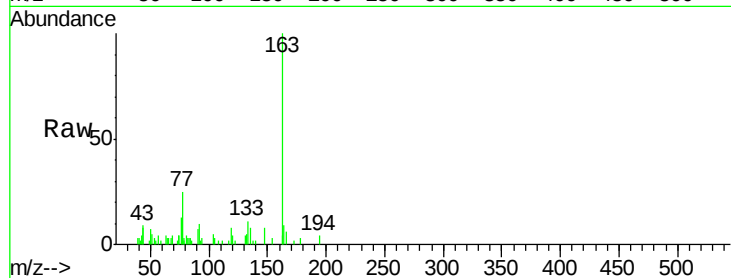

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

