

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080817\
 Data File : BG028188.D
 Acq On : 8 Aug 2017 13:47
 Operator : SJ/JU
 Sample : I4600-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C02X9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.840	38	43	46	rBV4	8919	12940	0.71%	0.089%
2	4.022	70	74	76	rVB3	2332	2947	0.16%	0.020%
3	4.751	197	198	205	rBV4	2201	4194	0.23%	0.029%
4	4.892	220	222	225	rBV3	2200	2711	0.15%	0.019%
5	4.992	231	239	240	rBV3	1657	3636	0.20%	0.025%
6	5.591	340	341	346	rBV2	1744	2712	0.15%	0.019%
7	7.083	590	595	600	rVB3	1555	2419	0.13%	0.017%
8	7.330	632	637	642	rVB4	1458	3050	0.17%	0.021%
9	7.424	648	653	656	rBV2	1568	2602	0.14%	0.018%
10	7.501	656	666	679	rVB	40623	82346	4.54%	0.566%
11	7.671	685	695	706	rBV	131094	228047	12.56%	1.568%
12	7.888	722	732	746	rBV2	134148	255310	14.07%	1.755%
13	8.358	804	812	825	rVB	117996	219381	12.09%	1.508%
14	9.046	922	929	942	rVB	115795	220874	12.17%	1.518%
15	9.522	999	1010	1022	rBV2	178591	353374	19.47%	2.429%
16	9.674	1028	1036	1039	rBV5	2383	4782	0.26%	0.033%
17	10.250	1123	1134	1143	rBV2	153478	297217	16.37%	2.043%
18	10.338	1147	1149	1157	rVB3	1783	2793	0.15%	0.019%
19	10.791	1216	1226	1238	rBV	191898	391097	21.55%	2.688%
20	11.102	1275	1279	1284	rBV4	1945	4287	0.24%	0.029%
21	11.173	1284	1291	1304	rVB	185311	345116	19.01%	2.372%
22	11.314	1310	1315	1325	rVB4	11204	24298	1.34%	0.167%
23	12.747	1553	1559	1564	rBV2	2918	4256	0.23%	0.029%
24	13.311	1652	1655	1663	rVB3	2206	2485	0.14%	0.017%
25	13.552	1693	1696	1701	rBV3	2216	3980	0.22%	0.027%
26	14.351	1824	1832	1845	rBV	578478	860011	47.38%	5.912%
27	14.657	1877	1884	1896	rBV	518825	847946	46.72%	5.829%
28	14.962	1927	1936	1944	rVB2	316464	547445	30.16%	3.763%
29	15.162	1960	1970	1984	rBV4	35308	90035	4.96%	0.619%
30	15.949	2095	2104	2116	rBV	786506	1212003	66.77%	8.331%
31	16.061	2116	2123	2137	rBV	326140	502952	27.71%	3.457%
32	16.190	2141	2145	2154	rVB5	8192	14840	0.82%	0.102%
33	16.320	2164	2167	2173	rBV3	1683	2602	0.14%	0.018%
34	17.289	2327	2332	2337	rBV3	1583	3714	0.20%	0.026%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080817\
 Data File : BG028188.D
 Acq On : 8 Aug 2017 13:47
 Operator : SJ/JU
 Sample : I4600-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C02X9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
 Title : SVOA CALIBRATION

35	17.336	2337	2340	2347	rVV3	1493	2842	0.16%	0.020%
36	17.506	2363	2369	2372	rBV3	2057	3893	0.21%	0.027%
37	17.712	2394	2404	2413	rBV	512544	779069	42.92%	5.355%
38	17.812	2413	2421	2433	rVV	1001781	1501451	82.72%	10.321%
39	18.358	2511	2514	2519	rVB2	2193	3228	0.18%	0.022%
40	18.405	2519	2522	2526	rBV2	1995	2459	0.14%	0.017%
41	18.640	2559	2562	2565	rVB3	2644	3679	0.20%	0.025%
42	19.022	2624	2627	2631	rVB4	2636	2771	0.15%	0.019%
43	19.721	2738	2746	2752	rVB2	13095	22775	1.25%	0.157%
44	19.792	2752	2758	2761	rBV3	2445	5769	0.32%	0.040%
45	19.915	2774	2779	2782	rBV5	2140	3337	0.18%	0.023%
46	19.980	2784	2790	2793	rBV3	8260	13937	0.77%	0.096%
47	20.086	2798	2808	2816	rBV	1259278	1815113	100.00%	12.477%
48	20.526	2880	2883	2885	rVB3	2620	2693	0.15%	0.019%
49	20.550	2885	2887	2890	rBV3	3523	3268	0.18%	0.022%
50	20.714	2913	2915	2917	rBV2	3125	2642	0.15%	0.018%
51	21.402	3025	3032	3033	rBV6	8810	14068	0.78%	0.097%
52	21.884	3110	3114	3121	rVB7	6416	12673	0.70%	0.087%
53	22.042	3133	3141	3154	rBV	518448	902096	49.70%	6.201%
54	23.411	3372	3374	3377	rBV4	3551	2772	0.15%	0.019%
55	23.599	3403	3406	3416	rVB7	7993	15654	0.86%	0.108%
56	23.770	3433	3435	3437	rBV2	4661	3275	0.18%	0.023%
57	23.993	3470	3473	3476	rBV5	2911	3882	0.21%	0.027%
58	24.322	3526	3529	3539	rVB9	4640	10862	0.60%	0.075%
59	24.469	3548	3554	3565	rVB6	13836	33266	1.83%	0.229%
60	24.727	3594	3598	3599	rBV4	5050	7078	0.39%	0.049%
61	25.015	3645	3647	3650	rBV2	3472	2723	0.15%	0.019%
62	25.309	3684	3697	3715	rBV2	542330	1636893	90.18%	11.252%
63	25.556	3723	3739	3756	rVB	269639	905596	49.89%	6.225%
64	26.731	3931	3939	3956	rBV6	18711	62177	3.43%	0.427%
65	27.477	4064	4066	4069	rBV4	3177	3864	0.21%	0.027%
66	28.118	4172	4175	4179	rVB3	3002	4763	0.26%	0.033%
67	28.212	4180	4191	4200	rVV5	21346	72407	3.99%	0.498%
68	29.293	4373	4375	4385	rVB8	5397	9000	0.50%	0.062%
69	29.992	4486	4494	4496	rBV7	13212	30348	1.67%	0.209%
70	30.967	4655	4660	4662	rBV5	4778	7874	0.43%	0.054%
71	31.678	4779	4781	4787	rVB5	2415	3770	0.21%	0.026%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080817\
Data File : BG028188.D
Acq On : 8 Aug 2017 13:47
Operator : SJ/JU
Sample : I4600-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C02X9

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.1 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
Title : SVOA CALIBRATION

72	32.160	4845	4863	4875	rBV5	13942	75455	4.16%	0.519%
----	--------	------	------	------	------	-------	-------	-------	--------


Sum of corrected areas: 14547824

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080817\
Data File : BG028188.D
Acq On : 8 Aug 2017 13:47
Operator : SJ/JU
Sample : I4600-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C02X9

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

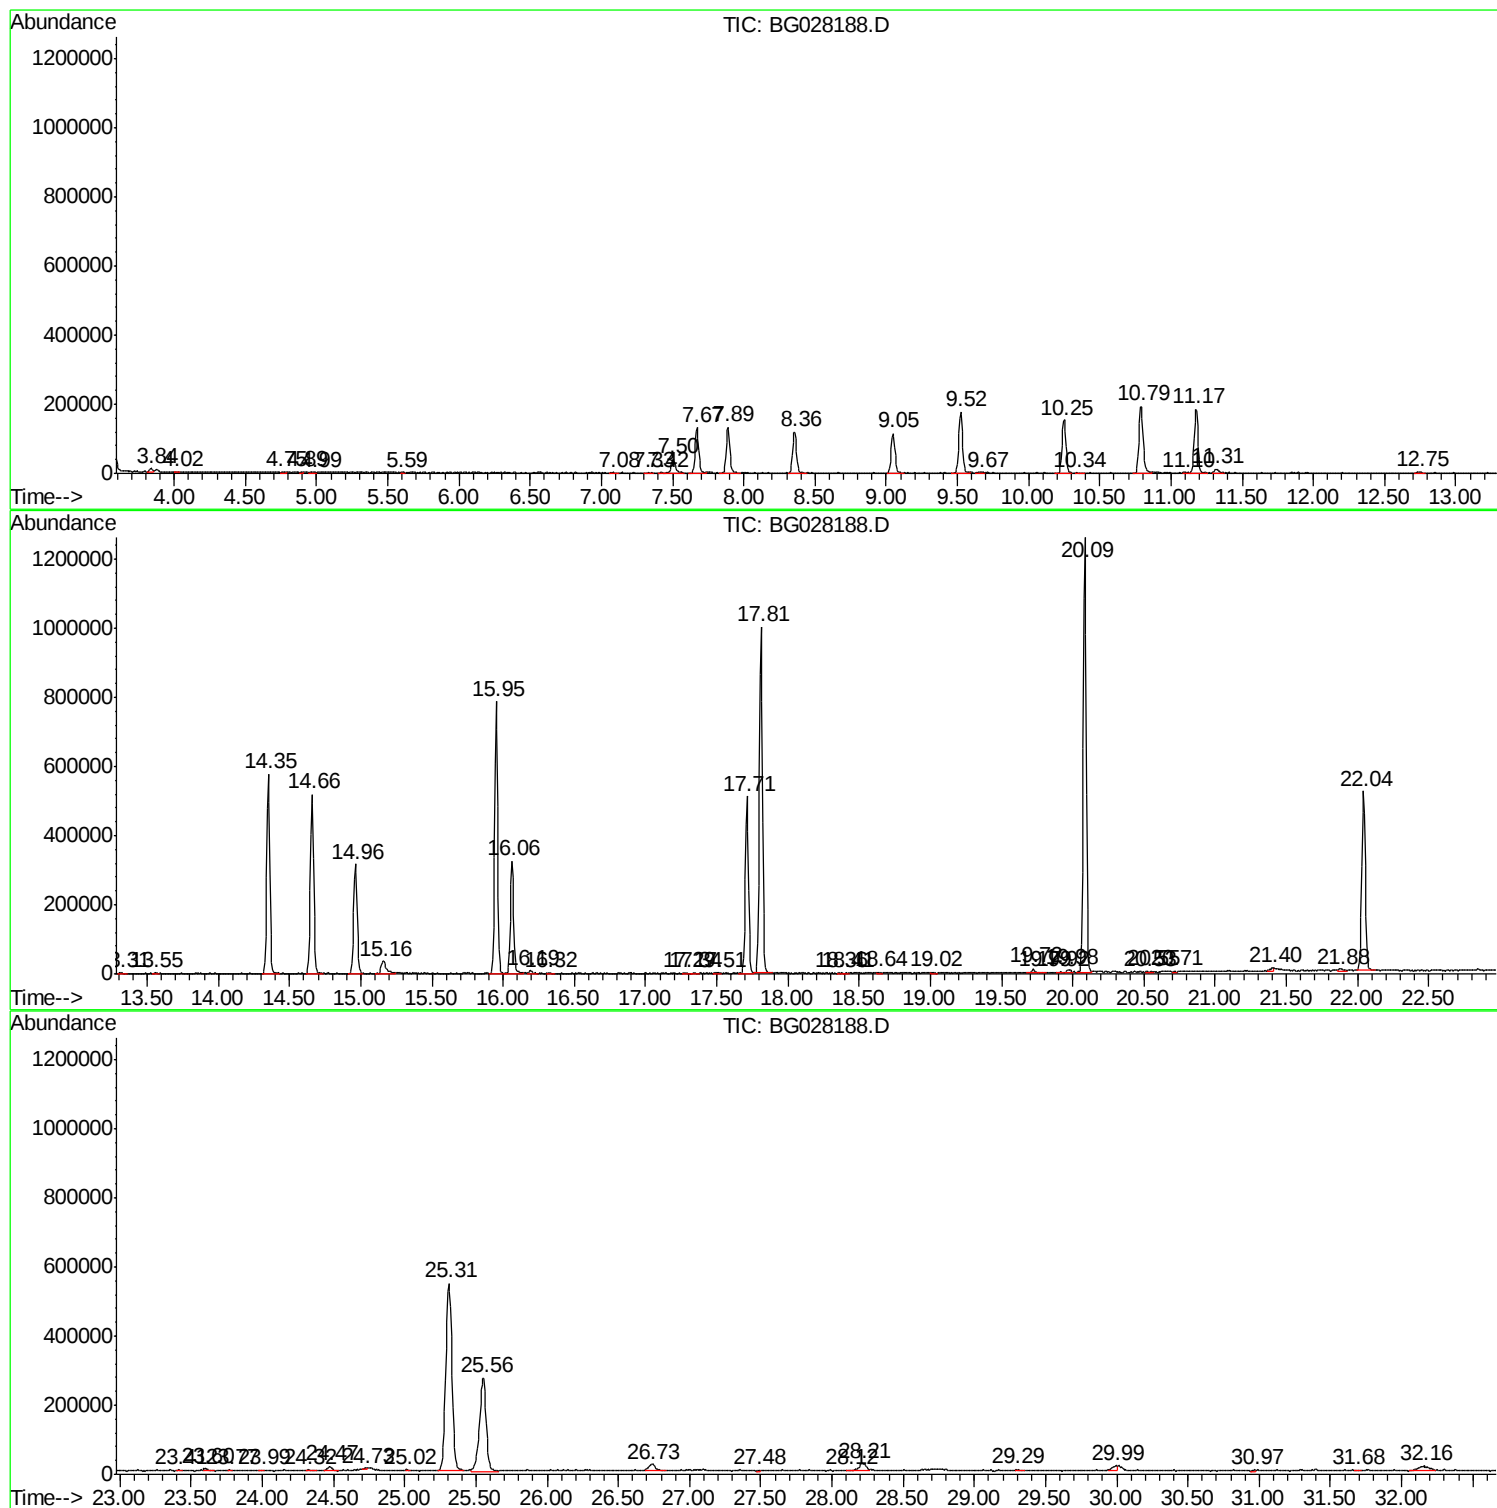

DbaaaPathh::ZZ\NRPBHHM1BBAAGCDBAAAB0000017\
 DbaaaFile::BB002388DD
 Aeqq00n :: 88Aagg2007 133447
 Opeaaor ::SSJUU
 Sample ::I4000005
 Misc ::
 AASSVal ::88 SampleMultiplier:11

Instrument :
 BNA_G
 ClientSampleId :
 C02X9

QqaabMebbdd::ZZ\NRPBHHM1BBAAGCMEEH00SS00MEPRABB000217MM
 QqaabTitle ::S00ACALIBRATION

TICLibbaay ::CC\DATAABASENOSTI11LL
 TICIntegratíonPaaameess:LS6CNTPP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
