

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080817\
 Data File : BG028214.D
 Acq On : 9 Aug 2017 6:55
 Operator : SJ/JU
 Sample : I4557-04
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AC7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.840	38	43	53	rVB2	13849	25144	1.01%	0.124%
2	4.774	195	202	209	rBV5	5167	10809	0.44%	0.053%
3	5.174	267	270	276	rVB4	2877	3771	0.15%	0.019%
4	6.690	522	528	535	rBV4	1536	3740	0.15%	0.018%
5	7.501	654	666	677	rBV	56674	115790	4.67%	0.572%
6	7.671	686	695	706	rBV	157720	281176	11.35%	1.390%
7	7.888	724	732	741	rBV	175419	317770	12.83%	1.570%
8	8.353	801	811	822	rBV	173938	313644	12.66%	1.550%
9	9.046	921	929	944	rBV2	157948	293861	11.86%	1.452%
10	9.522	1001	1010	1023	rBV	228460	419924	16.95%	2.075%
11	9.886	1067	1072	1076	rVB2	1863	3453	0.14%	0.017%
12	10.244	1124	1133	1144	rBV	192950	367706	14.84%	1.817%
13	10.785	1216	1225	1238	rBV	284719	554087	22.37%	2.738%
14	11.173	1281	1291	1301	rVB	252641	487040	19.66%	2.407%
15	11.343	1310	1320	1325	rBV3	3161	9201	0.37%	0.045%
16	12.742	1552	1558	1564	rBV4	3920	8764	0.35%	0.043%
17	13.564	1693	1698	1701	rVB3	2703	4051	0.16%	0.020%
18	13.834	1738	1744	1749	rVB4	2761	4690	0.19%	0.023%
19	14.351	1824	1832	1838	rBV	778109	1154079	46.59%	5.703%
20	14.398	1838	1840	1848	rVB2	53300	67518	2.73%	0.334%
21	14.657	1877	1884	1893	rBV	703213	1129663	45.60%	5.583%
22	14.962	1927	1936	1946	rVB2	442015	746599	30.14%	3.690%
23	15.150	1962	1968	1986	rBV2	58642	137132	5.54%	0.678%
24	15.762	2061	2072	2077	rBV5	4830	12373	0.50%	0.061%
25	15.950	2092	2104	2115	rBV	1017741	1587811	64.09%	7.847%
26	16.061	2115	2123	2136	rBV	479096	730839	29.50%	3.612%
27	16.196	2138	2146	2151	rVB7	13304	25071	1.01%	0.124%
28	16.625	2215	2219	2228	rBV2	11633	21583	0.87%	0.107%
29	16.907	2263	2267	2273	rVB5	3708	5819	0.23%	0.029%
30	17.095	2293	2299	2303	rBV5	3904	8777	0.35%	0.043%
31	17.242	2322	2324	2327	rBV2	3121	3629	0.15%	0.018%
32	17.418	2349	2354	2360	rBV4	9923	15624	0.63%	0.077%
33	17.495	2360	2367	2375	rVB4	4627	13101	0.53%	0.065%
34	17.577	2377	2381	2385	rBV5	4147	5967	0.24%	0.029%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080817\
 Data File : BG028214.D
 Acq On : 9 Aug 2017 6:55
 Operator : SJ/JU
 Sample : I4557-04
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AC7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
 Title : SVOA CALIBRATION

35	17.712	2397	2404	2412	rBV2	699389	1107003	44.69%	5.471%
36	17.812	2412	2421	2431	rVB	1294844	2009594	81.12%	9.931%
37	17.959	2443	2446	2454	rVB5	3199	7158	0.29%	0.035%
38	18.047	2455	2461	2462	rVV5	2587	3795	0.15%	0.019%
39	18.165	2478	2481	2485	rVB3	5252	7467	0.30%	0.037%
40	18.447	2523	2529	2531	rBV3	2543	3726	0.15%	0.018%
41	18.499	2535	2538	2541	rBV3	2526	3356	0.14%	0.017%
42	18.564	2544	2549	2558	rBV5	22824	44652	1.80%	0.221%
43	18.635	2558	2561	2566	rVV4	4537	5022	0.20%	0.025%
44	18.729	2575	2577	2585	rVB6	2945	4264	0.17%	0.021%
45	18.928	2606	2611	2620	rBV8	5115	11920	0.48%	0.059%
46	19.228	2655	2662	2664	rVB5	3843	6670	0.27%	0.033%
47	19.334	2676	2680	2682	rBV4	3140	4134	0.17%	0.020%
48	19.575	2718	2721	2725	rBV4	4505	8266	0.33%	0.041%
49	19.722	2740	2746	2750	rBV	15681	23270	0.94%	0.115%
50	19.816	2759	2762	2769	rBV5	24194	40254	1.62%	0.199%
51	19.974	2784	2789	2795	rBV3	15639	23267	0.94%	0.115%
52	20.086	2801	2808	2820	rBV	1707454	2477329	100.00%	12.243%
53	21.073	2974	2976	2981	rBV6	4512	7642	0.31%	0.038%
54	21.290	3012	3013	3017	rBV3	5072	6539	0.26%	0.032%
55	21.408	3026	3033	3036	rBV7	6694	12514	0.51%	0.062%
56	21.637	3066	3072	3075	rBV7	5236	11666	0.47%	0.058%
57	21.778	3093	3096	3097	rBV3	5543	5270	0.21%	0.026%
58	21.884	3111	3114	3119	rVB7	6143	8011	0.32%	0.040%
59	22.042	3133	3141	3153	rBV	739713	1349757	54.48%	6.671%
60	22.413	3200	3204	3208	rBV6	5326	11947	0.48%	0.059%
61	23.317	3356	3358	3363	rBV5	6756	11407	0.46%	0.056%
62	23.593	3400	3405	3414	rBV5	18164	37770	1.52%	0.187%
63	23.805	3438	3441	3447	rVB8	4644	6917	0.28%	0.034%
64	24.169	3501	3503	3506	rVB3	3951	3331	0.13%	0.016%
65	24.393	3539	3541	3543	rBV3	4141	3716	0.15%	0.018%
66	24.475	3547	3555	3563	rVB4	18118	47972	1.94%	0.237%
67	24.633	3581	3582	3585	rVB3	5599	4458	0.18%	0.022%
68	25.315	3684	3698	3715	rVB2	765960	2323695	93.80%	11.484%
69	25.550	3721	3738	3753	rVB2	385861	1321769	53.35%	6.532%
70	25.814	3779	3783	3784	rBV4	3603	4985	0.20%	0.025%
71	26.067	3823	3826	3831	rBV6	5564	11502	0.46%	0.057%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080817\
Data File : BG028214.D
Acq On : 9 Aug 2017 6:55
Operator : SJ/JU
Sample : I4557-04
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AC7

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.1 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 1

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
Title : SVOA CALIBRATION

72	26.731	3929	3939	3951	rVB5	29143	98520	3.98%	0.487%
73	27.266	4028	4030	4033	rBV4	4684	3437	0.14%	0.017%
74	27.601	4085	4087	4089	rBV3	3727	3585	0.14%	0.018%
75	28.212	4178	4191	4203	rVB4	32115	121177	4.89%	0.599%
76	28.981	4320	4322	4328	rVB6	3417	5446	0.22%	0.027%
77	29.263	4368	4370	4374	rVB5	3586	5157	0.21%	0.025%
78	29.992	4482	4494	4507	rVB5	21436	85032	3.43%	0.420%
79	31.690	4781	4783	4791	rVB6	3697	7221	0.29%	0.036%
80	32.131	4848	4858	4860	rBV5	15239	32865	1.33%	0.162%


Sum of corrected areas: 20234661

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080817\
Data File : BG028214.D
Acq On : 9 Aug 2017 6:55
Operator : SJ/JU
Sample : I4557-04
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AC7

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

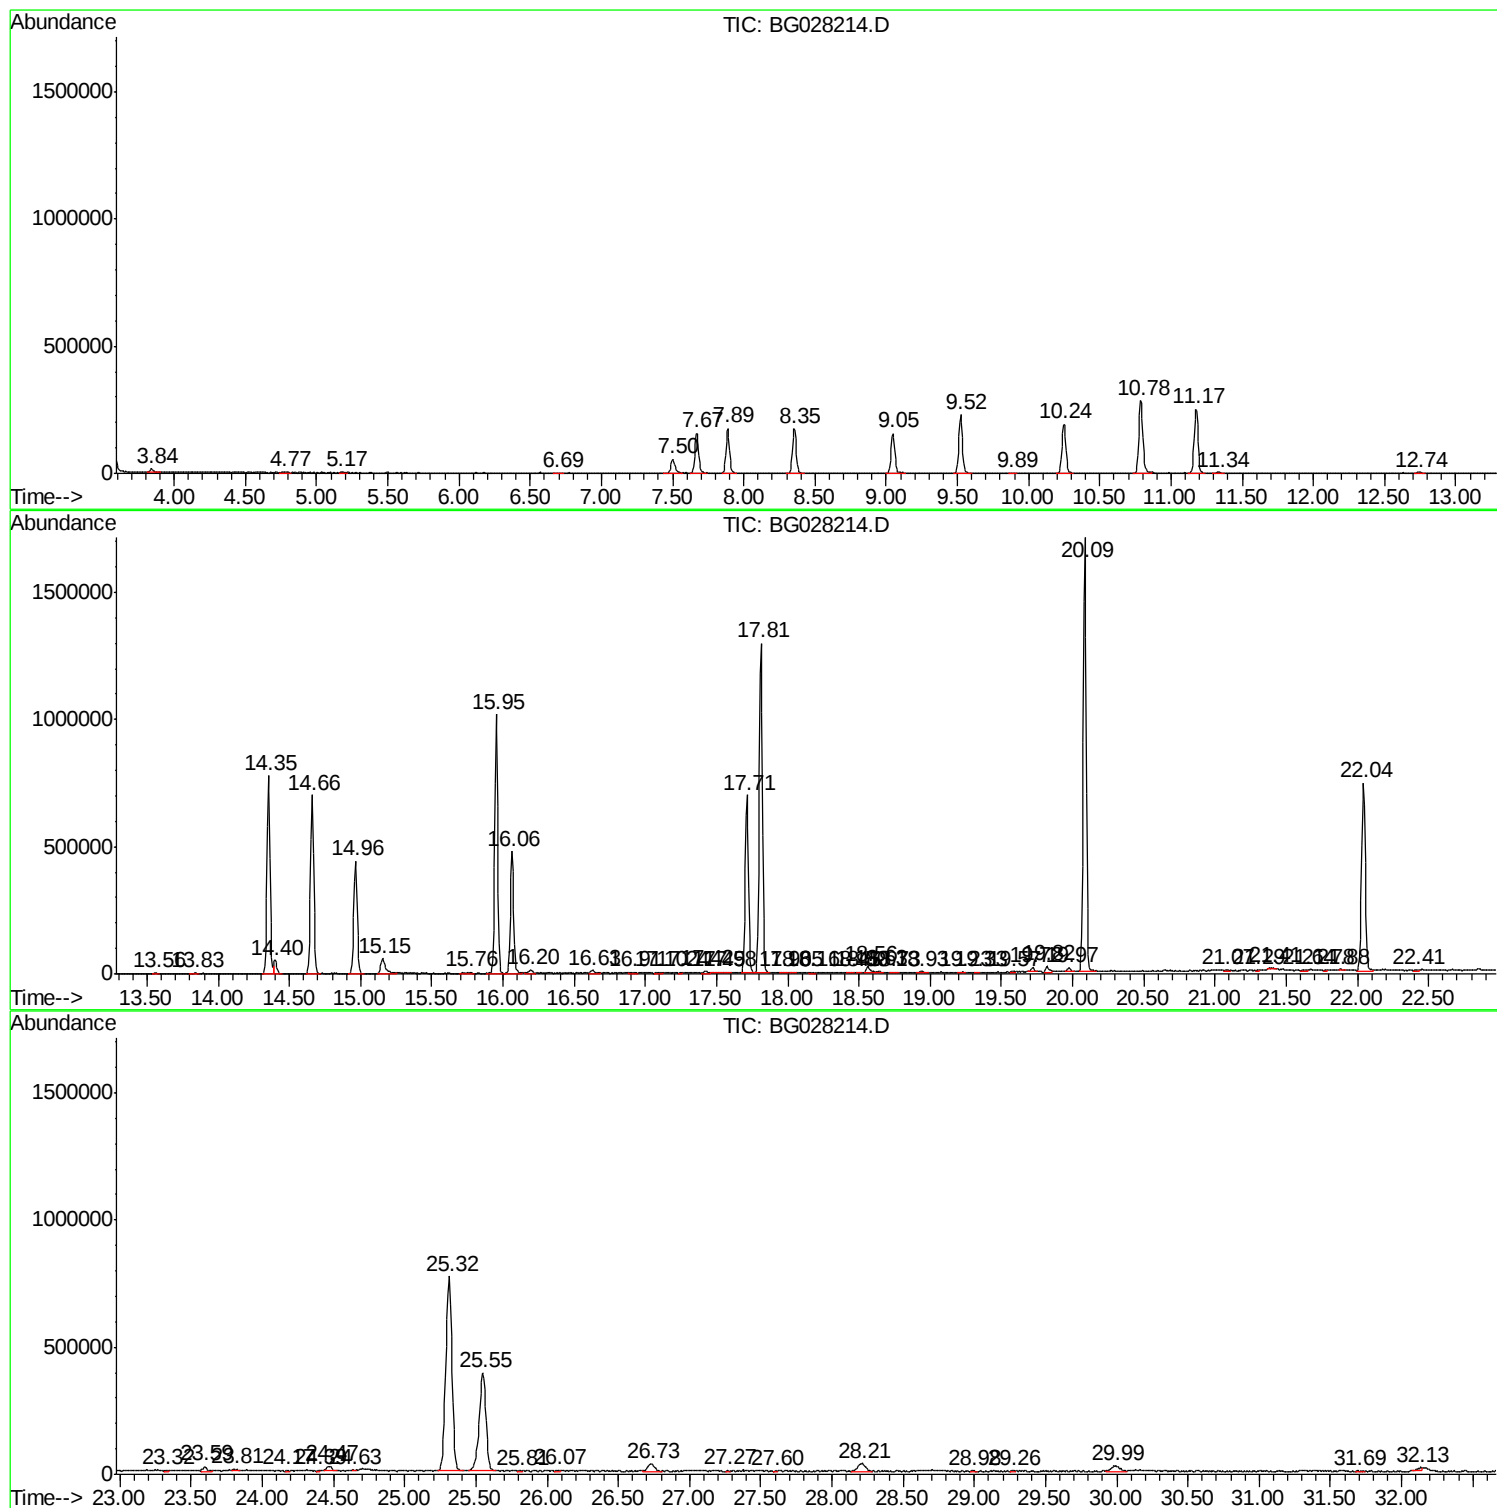

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080817\
Data File : BG028214.D
Acq On : 9 Aug 2017 6:55
Operator : SJ/JU
Sample : I4557-04
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AC7

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG080817\
Data File : BG028214.D
Acq On : 9 Aug 2017 6:55
Operator : SJ/JU
Sample : I4557-04
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AC7

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG080217.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc